


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121818\
 Data File : BG038691.D
 Acq On : 18 Dec 2018 11:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

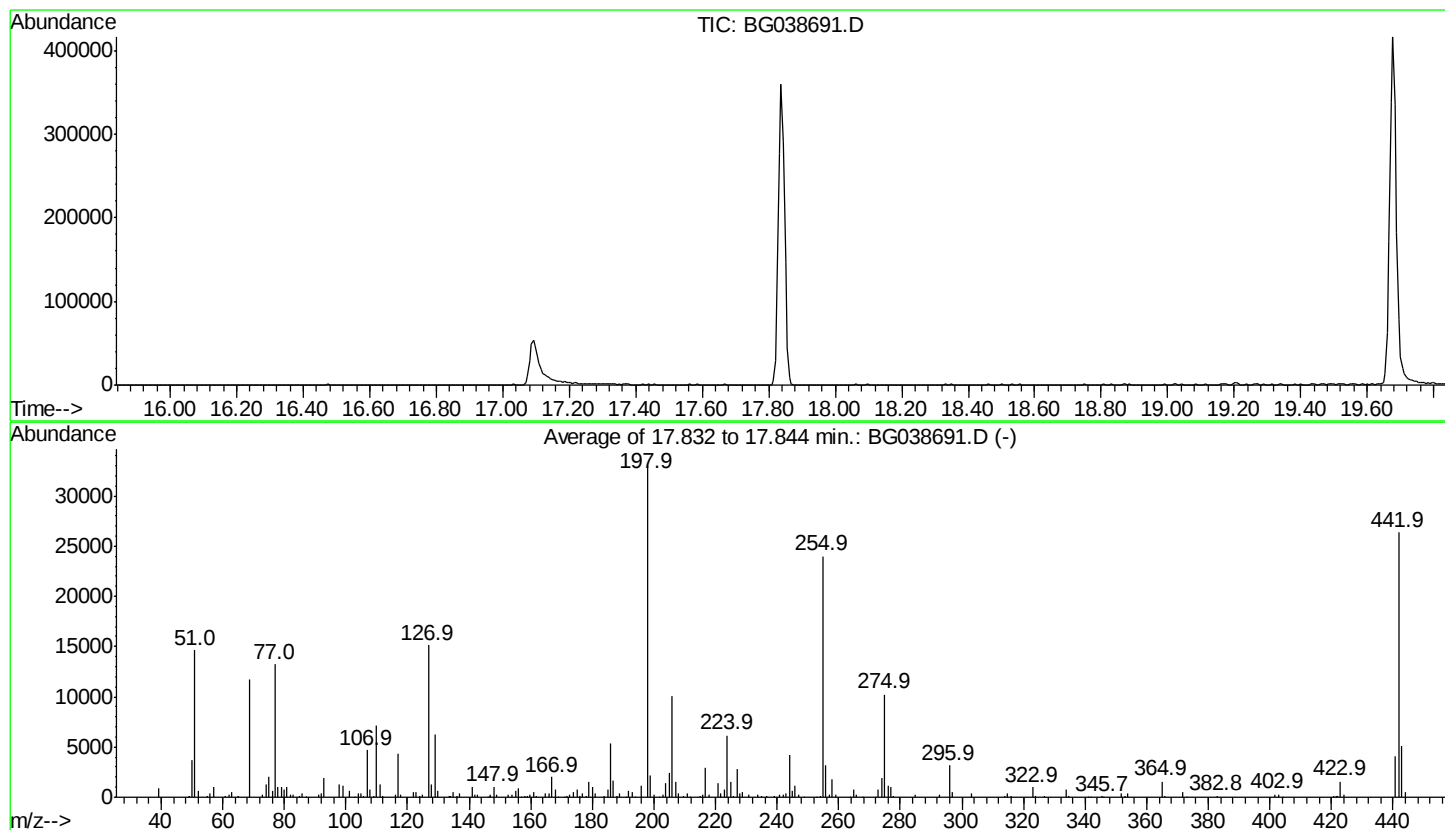

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	14629	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.6	11755	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.8	15138	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	33018	PASS
199	198	5	9	6.6	2175	PASS
275	198	10	60	30.9	10219	PASS
365	198	1	100	4.7	1553	PASS
441	198	0.01	100	12.5	4140	PASS
442	198	50	100	79.8	26336	PASS
443	442	15	24	19.6	5165	PASS