
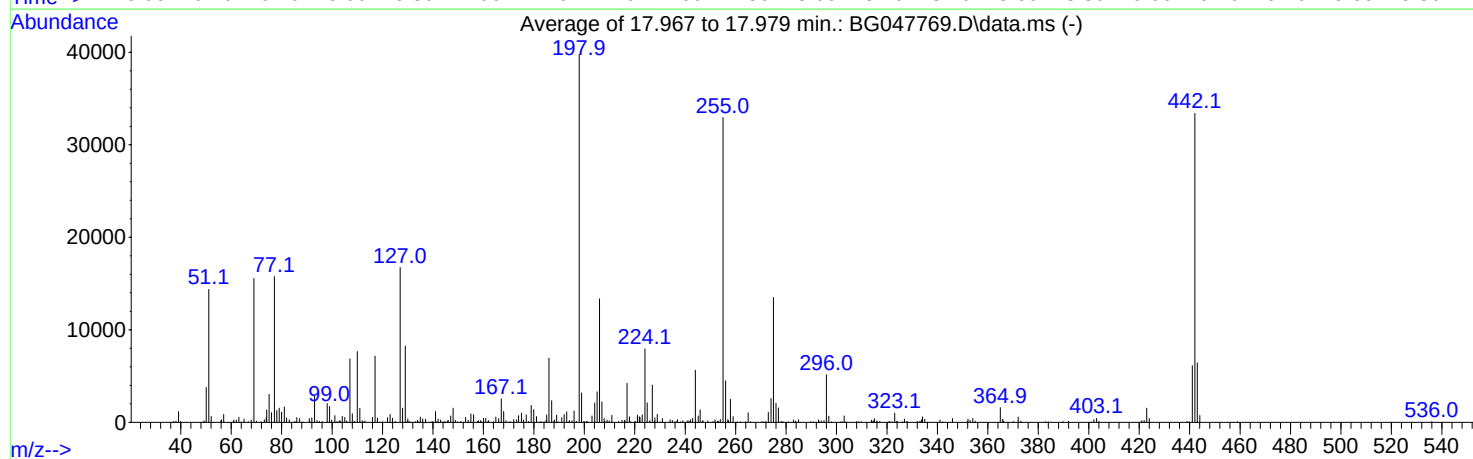


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121820\
 Data File : BG047769.D
 Acq On : 18 Dec 2020 10:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 17 15:55:16 2020

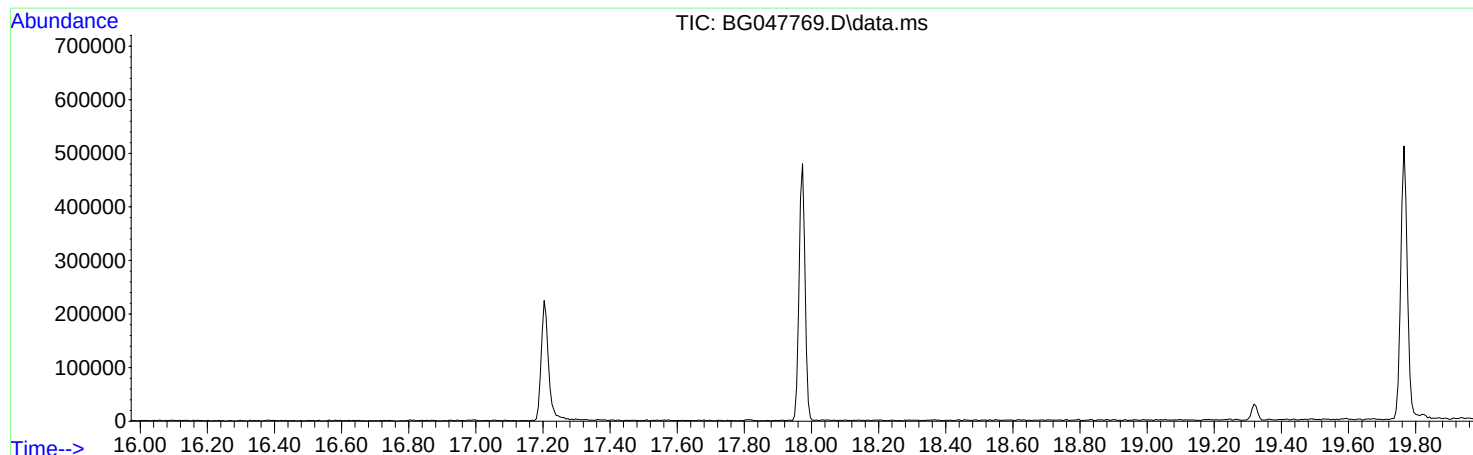

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	14376	PASS
68	69	0.00	2	1.5	239	PASS
69	198	0.00	100	39.1	15540	PASS
70	69	0.00	2	0.8	128	PASS
127	198	10	80	42.1	16737	PASS
197	198	0.00	2	0.3	128	PASS
198	198	100	100	100.0	39757	PASS
199	198	5	9	8.0	3180	PASS
275	198	10	60	34.0	13506	PASS
365	198	1	100	4.0	1601	PASS
441	198	0.01	100	15.4	6125	PASS
442	198	50	100	84.0	33397	PASS
443	442	15	24	19.2	6427	PASS