

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG121918\
 Data File : BG038755.D
 Acq On : 20 Dec 2018 9:35
 Operator : JU/SJ
 Sample : J6445-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EB02_12-14

Quant Time: Dec 20 11:15:59 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 12 15:26:27 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	28424	20.00	ng	0.00
21) Naphthalene-d8	10.87	136	113311	20.00	ng	0.00
39) Acenaphthene-d10	14.69	164	75234	20.00	ng	0.00
64) Phenanthrene-d10	17.44	188	187088	20.00	ng	0.00
76) Chrysene-d12	21.72	240	192153	20.00	ng	0.00
87) Perylene-d12	25.02	264	203619	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	206761	129.02	ng	0.00
7) Phenol-d6	7.21	99	285014	129.55	ng	0.00
23) Nitrobenzene-d5	9.23	82	173476	78.21	ng	0.00
42) 2,4,6-Tribromophenol	16.18	330	137663	132.77	ng	0.00
45) 2-Fluorobiphenyl	13.31	172	451028	82.24	ng	0.00
79) Terphenyl-d14	20.04	244	813498	92.14	ng	0.00
Target Compounds						
10) Phenol	7.24	94	16359	6.999	ng	91
50) Dimethylphthalate	14.14	163	31376	5.107	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG121918\
Data File : BG038755.D
Acq On : 20 Dec 2018 9:35
Operator : JU/SJ
Sample : J6445-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EB02_12-14

Quant Time: Dec 20 11:15:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

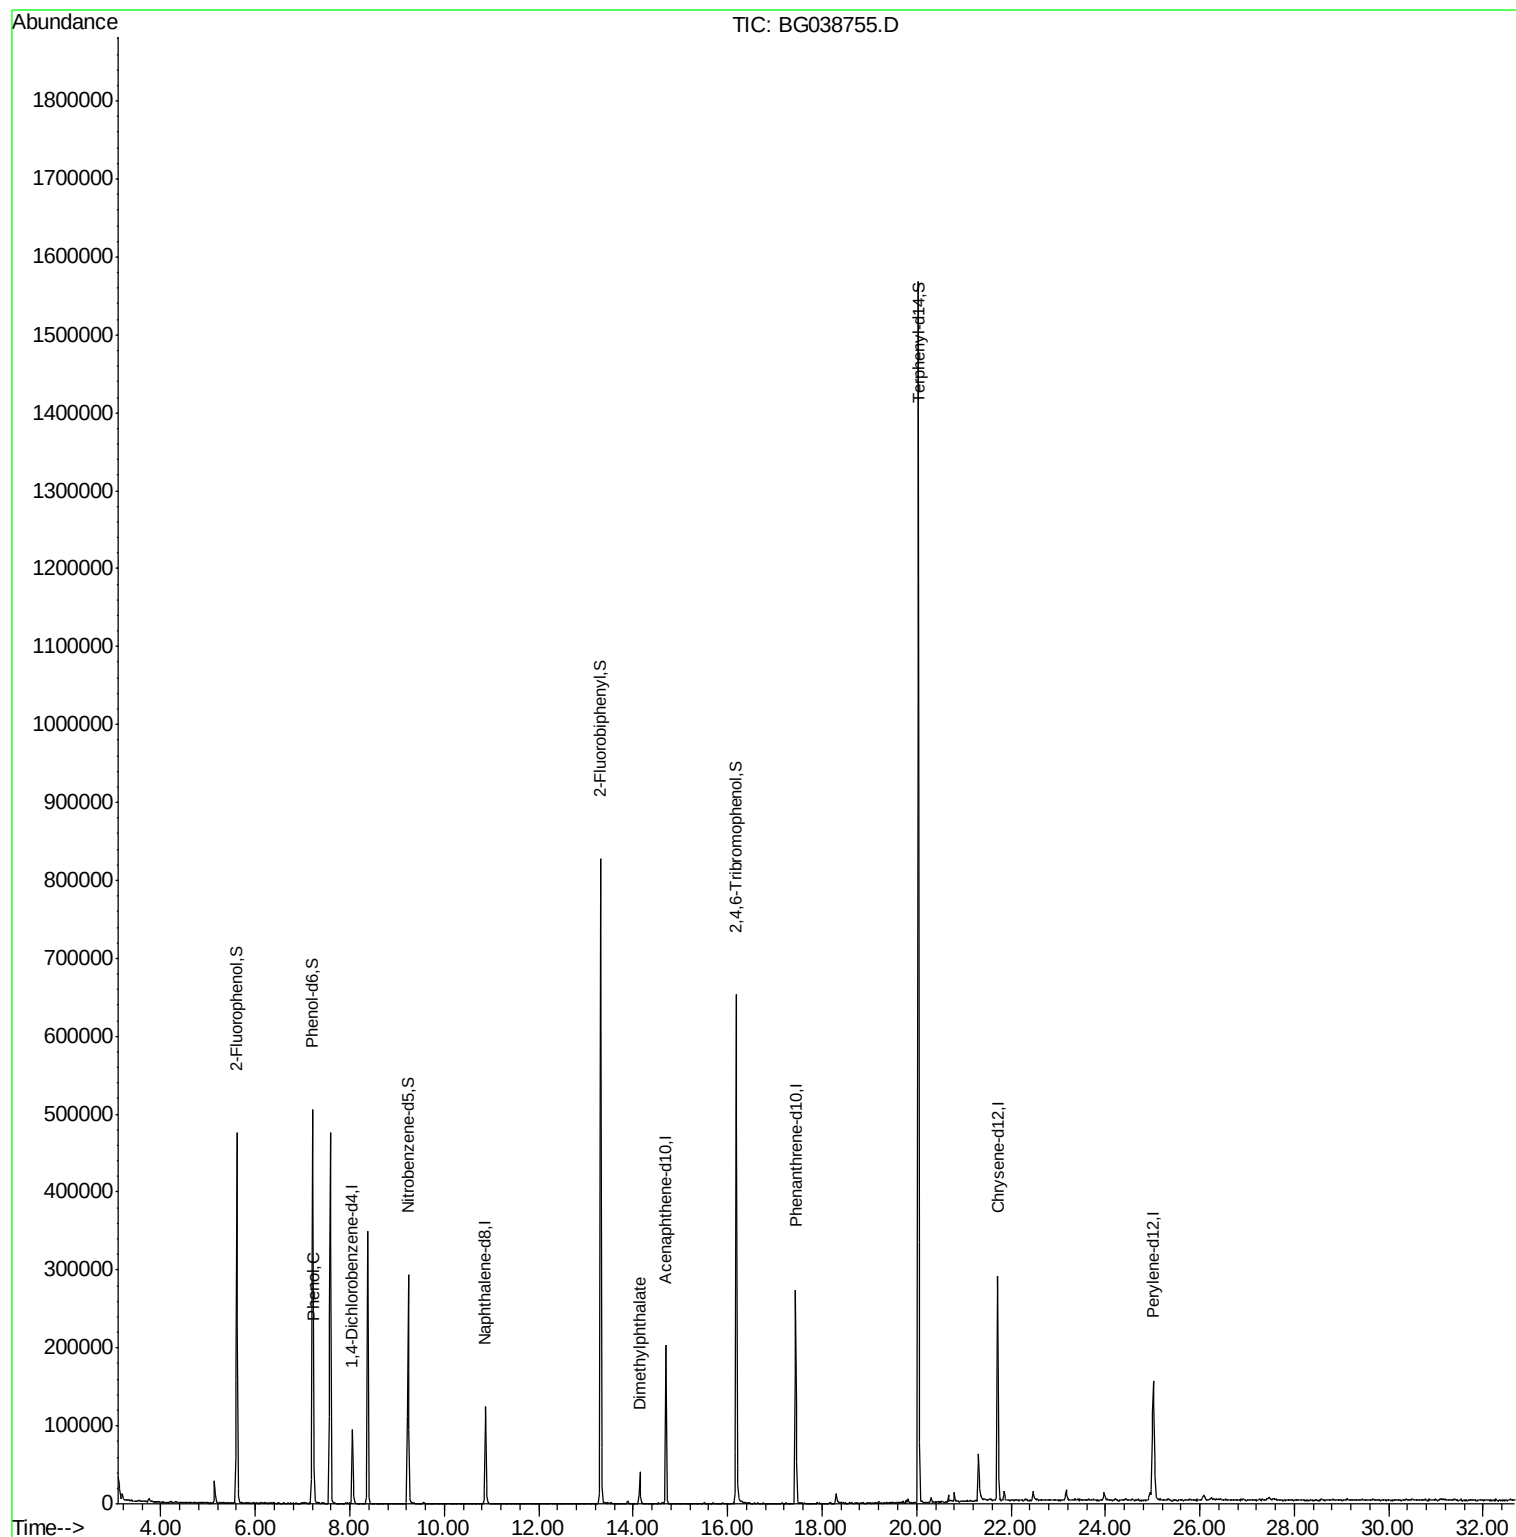

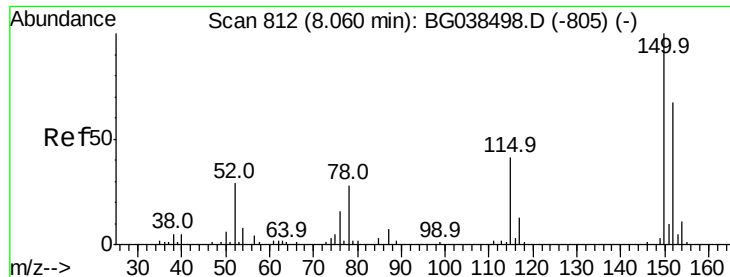


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.06 min Scan# 846
Delta R.T. -0.00 min
Lab File: BG038755.D
Acq: 20 Dec 2018 9:35

Instrument :
BNA_G
ClientSampleId :
EB02_12-14

Tot Ion:152 Resp: 28424
Ion Ratio Lower Upper
152 100
150 161.8 119.5 179.3
115 57.7 49.6 74.4

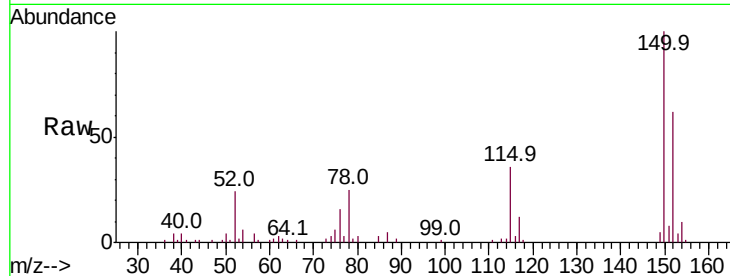


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

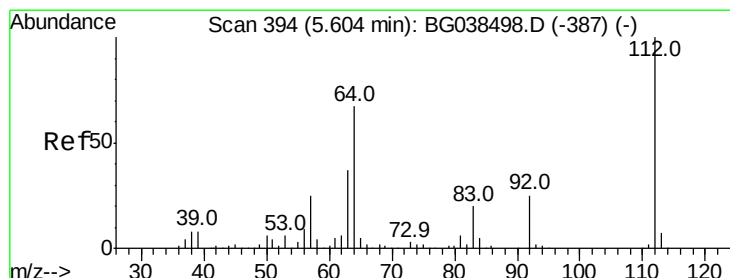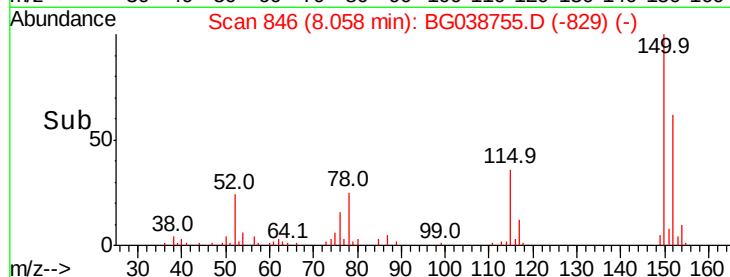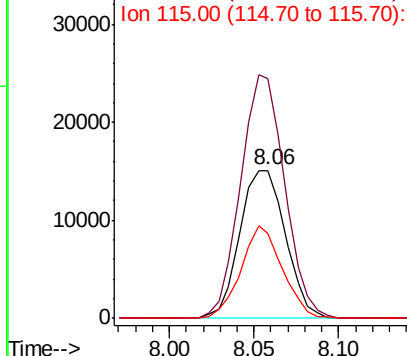



#5


2-Fluorophenol
Concen: 129.018 ng
RT: 5.61 min Scan# 429
Delta R.T. 0.01 min
Lab File: BG038755.D
Acq: 20 Dec 2018 9:35

Tgt Ion:112 Resp: 206761
Ion Ratio Lower Upper
112 100
64 64.8 53.4 80.2
63 36.6 29.3 43.9

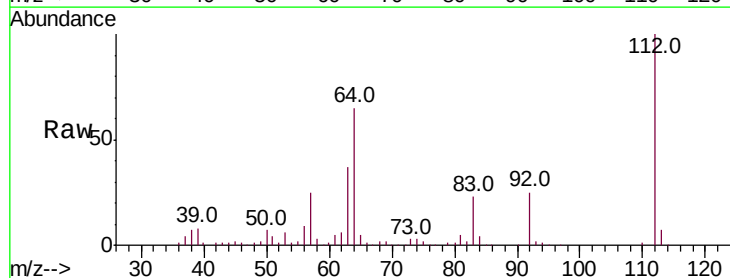

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

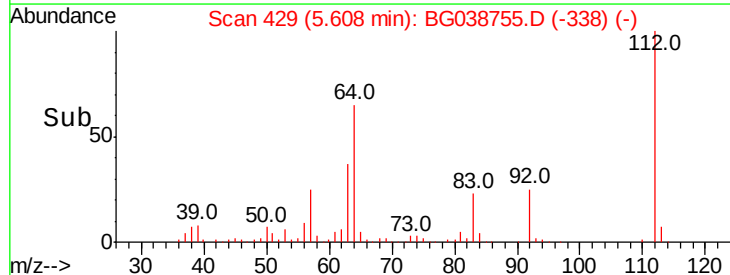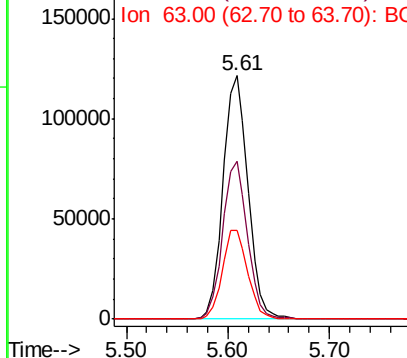

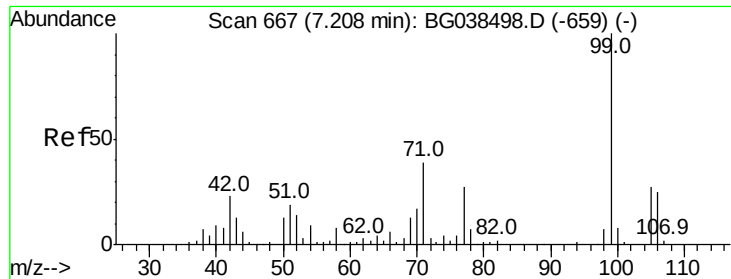

#7

Phenol-d6

Concen: 129.551 ng

RT: 7.21 min Scan# 702

Delta R.T. 0.00 min

Lab File: BG038755.D

Acq: 20 Dec 2018 9:35

Instrument :

BNA_G

ClientSampleId :

EB02_12-14


Tot Ion: 99 Resp: 285014

Ion Ratio Lower Upper




99 100

42 22.8 18.5 27.7

71 40.4 31.1 46.7

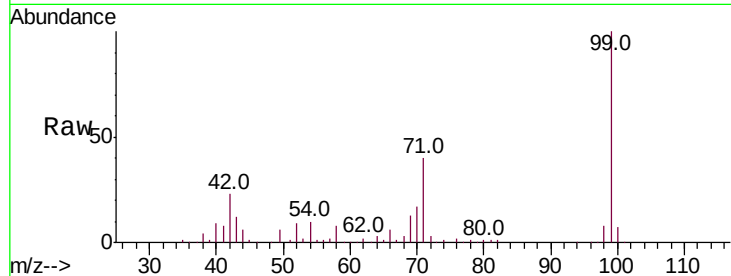

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

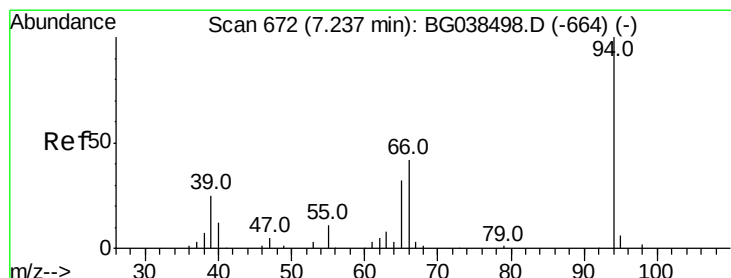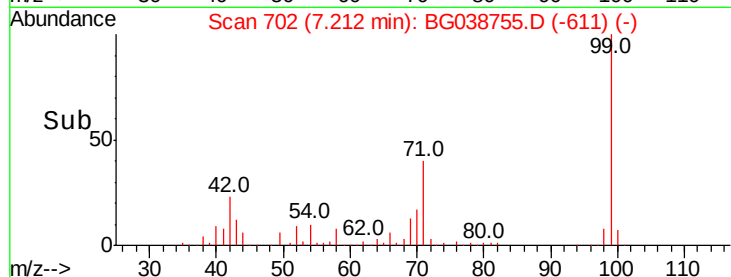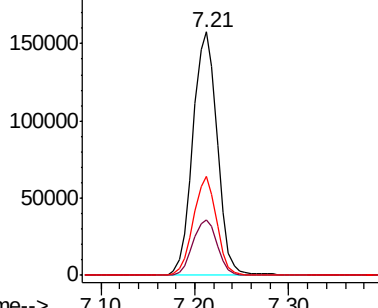

#10

Phenol

Concen: 6.999 ng

RT: 7.24 min Scan# 706

Delta R.T. -0.00 min

Lab File: BG038755.D

Acq: 20 Dec 2018 9:35


Tgt Ion: 94 Resp: 16359

Ion Ratio Lower Upper



94 100


65 35.5 12.6 52.6

66 51.9 24.1 64.1

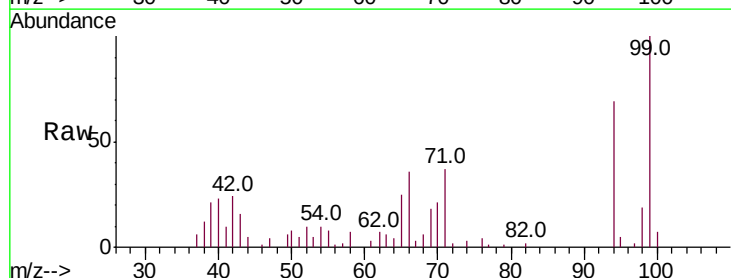

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC



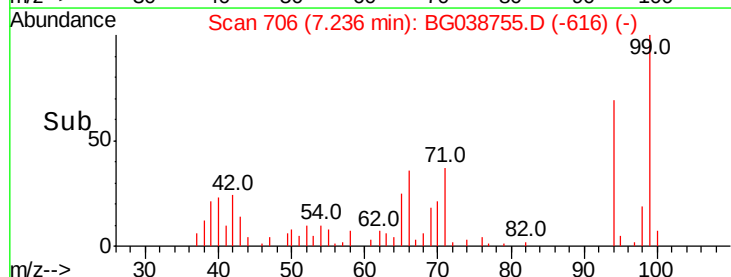
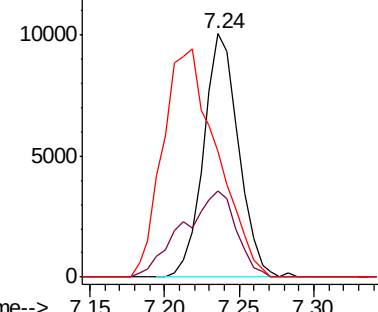


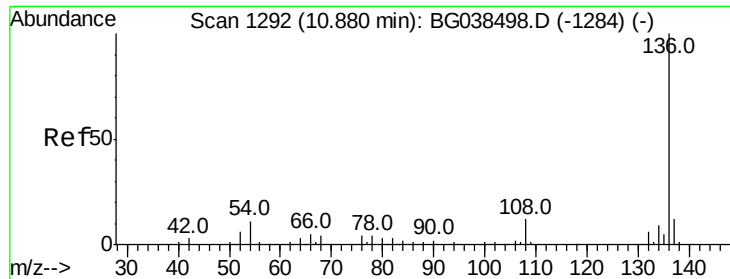

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.87 min Scan# 1325
Delta R.T. -0.01 min
Lab File: BG038755.D
Acq: 20 Dec 2018 9:35




Instrument :
BNA_G
ClientSampleId :
EB02_12-14


Tot Ion:136	Resp:	113311
Ion	Ratio	Lower Upper
136	100	
137	10.6	9.3 13.9
54	10.3	8.5 12.7
68	4.5	3.5 5.3

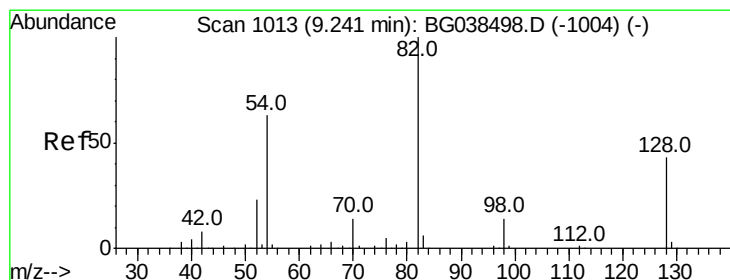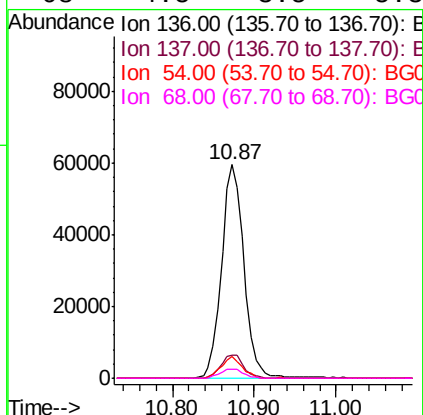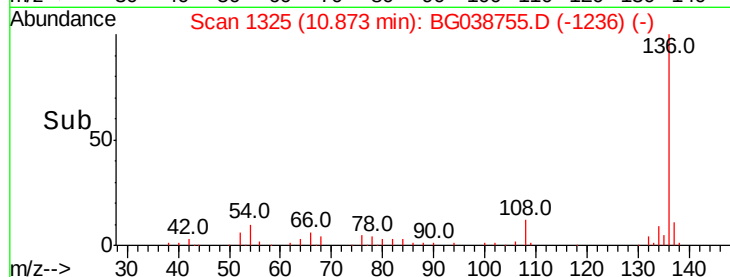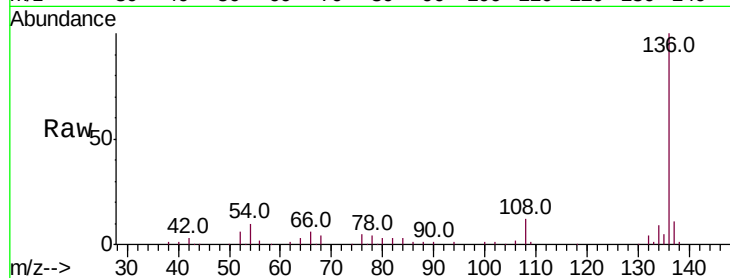

#23
Nitrobenzene-d5
Concen: 78.213 ng
RT: 9.23 min Scan# 1046
Delta R.T. -0.01 min
Lab File: BG038755.D
Acq: 20 Dec 2018 9:35

Tgt Ion: 82	Resp:	173476
Ion	Ratio	Lower Upper
82	100	
128	43.7	34.6 52.0
54	63.9	50.6 76.0

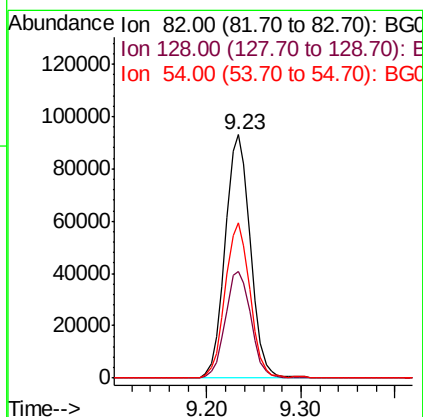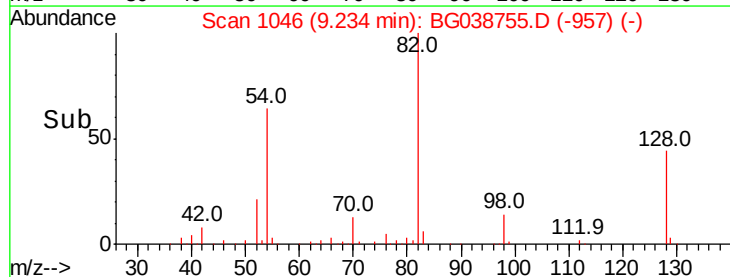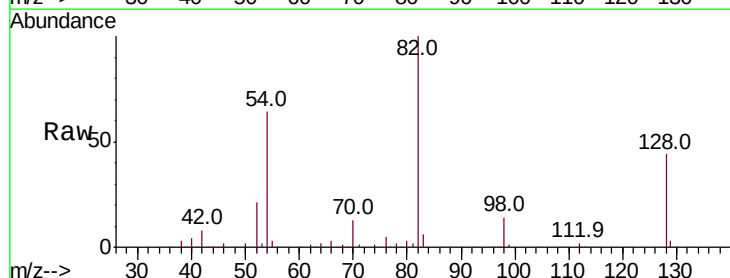

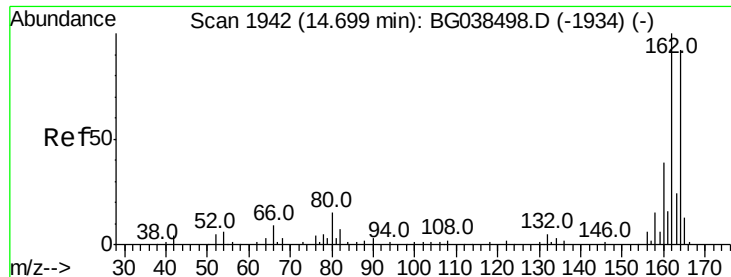

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.69 min Scan# 1975

Delta R.T. -0.01 min

Lab File: BG038755.D

Acq: 20 Dec 2018 9:35

Instrument :

BNA_G

ClientSampleId :

EB02_12-14


Tot Ion:164 Resp: 75234

Ion Ratio Lower Upper

164 100

162 101.6 86.6 130.0




160 45.8 34.2 51.2

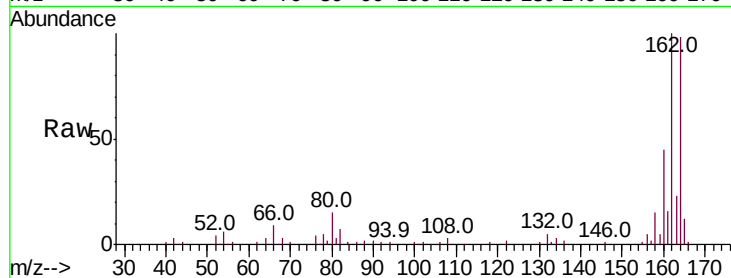

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

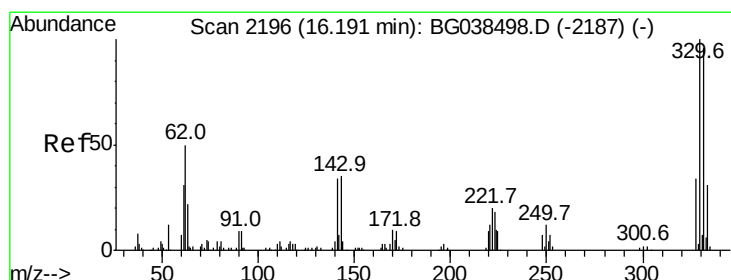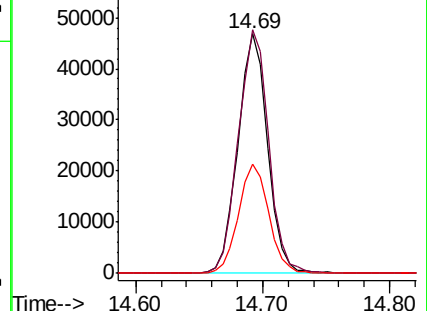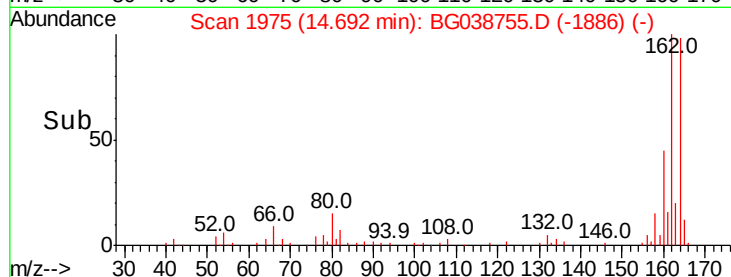

#42

2,4,6-Tribromophenol

Concen: 132.769 ng

RT: 16.18 min Scan# 2229

Delta R.T. -0.01 min

Lab File: BG038755.D

Acq: 20 Dec 2018 9:35


Tgt Ion:330 Resp: 137663

Ion Ratio Lower Upper

330 100

332 94.4 76.9 115.3



141 33.5 28.8 43.2

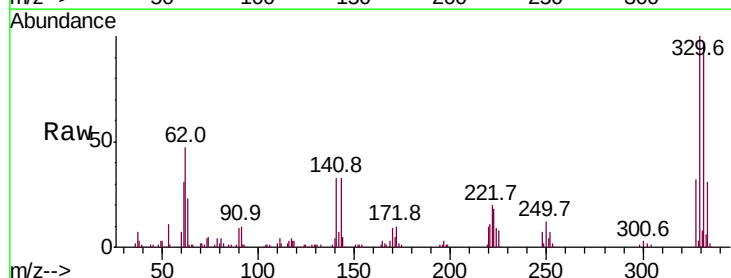


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

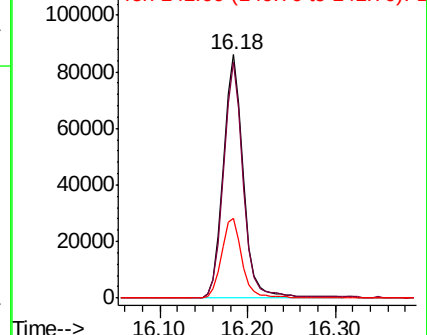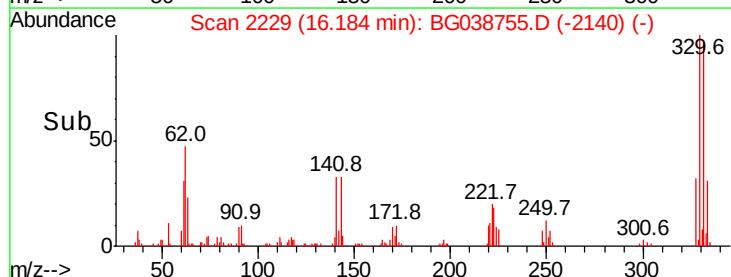


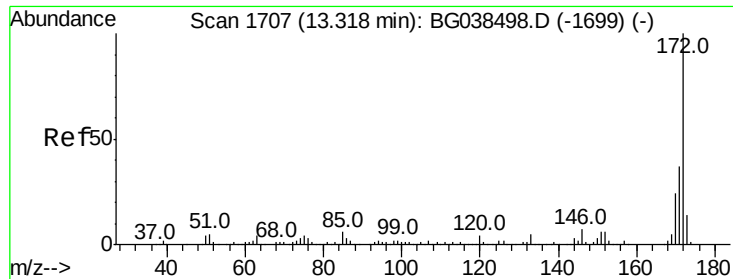




#45
 2-Fluorobiphenyl
 Concen: 82.242 ng
 RT: 13.31 min Scan# 1740
 Delta R.T. -0.01 min
 Lab File: BG038755.D
 Acq: 20 Dec 2018 9:35

Instrument :
 BNA_G
 ClientSampleId :
 EB02_12-14

Tot Ion:172 Resp: 451028
 Ion Ratio Lower Upper
 172 100
 171 37.2 29.8 44.6
 170 24.6 19.5 29.3

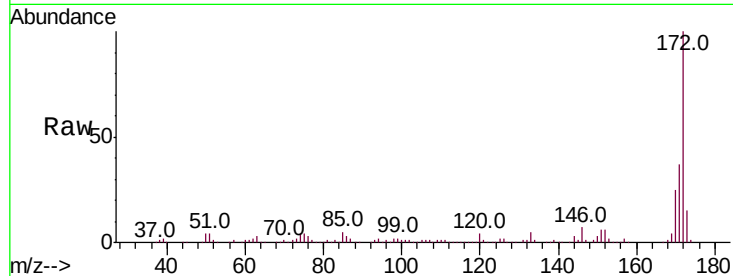


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

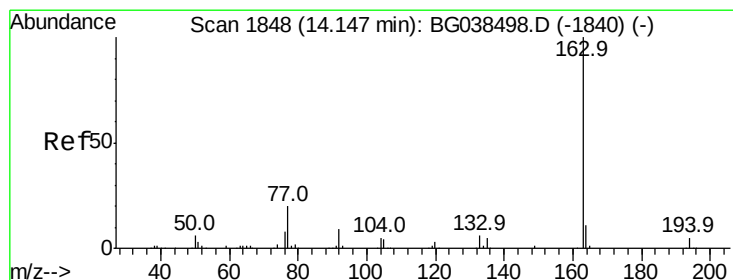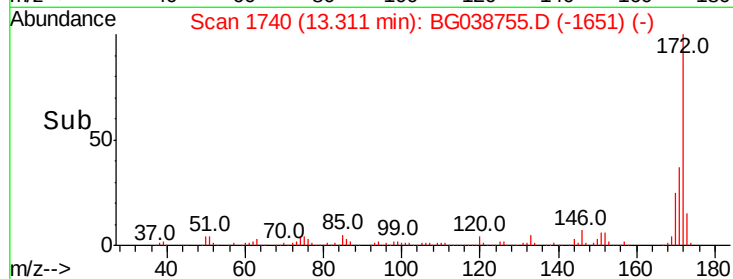
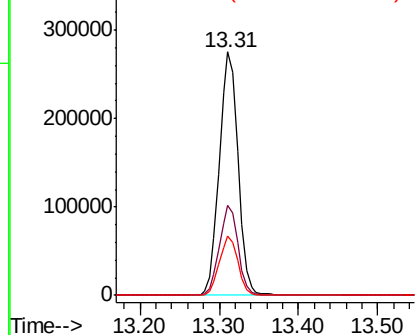



#50
 Dimethylphthalate
 Concen: 5.107 ng
 RT: 14.14 min Scan# 1881
 Delta R.T. -0.01 min
 Lab File: BG038755.D
 Acq: 20 Dec 2018 9:35

Tgt Ion:163 Resp: 31376
 Ion Ratio Lower Upper
 163 100
 194 4.7 3.7 5.5
 164 9.9 8.6 12.8

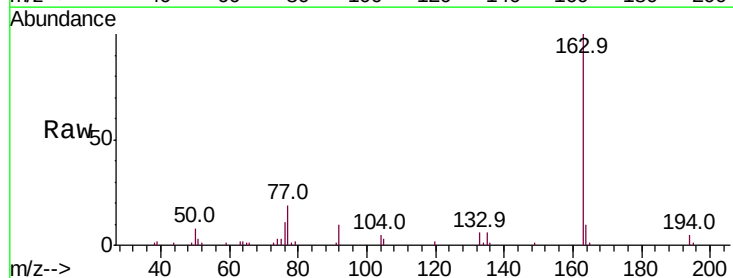

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

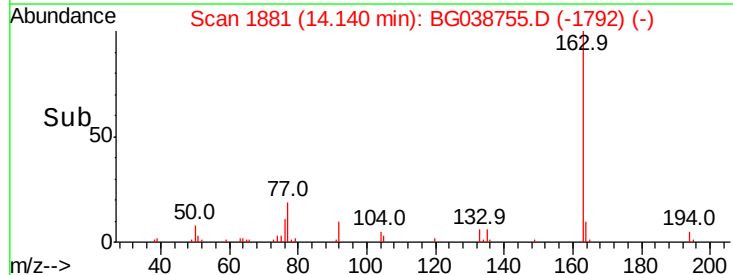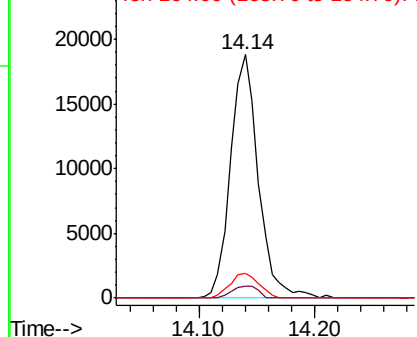


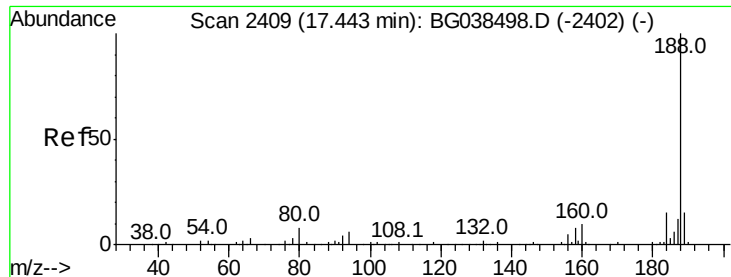




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.44 min Scan# 2443
Delta R.T. -0.00 min
Lab File: BG038755.D
Acq: 20 Dec 2018 9:35

Instrument :
BNA_G
ClientSampleId :
EB02_12-14

Tot Ion:188 Resp: 187088
Ion Ratio Lower Upper
188 100
94 5.8 5.1 7.7
80 6.4 6.1 9.1

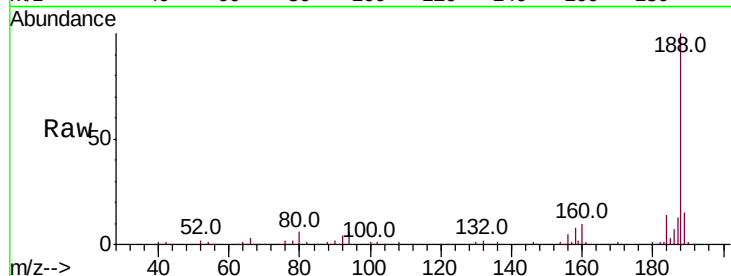


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BG
Ion 80.00 (79.70 to 80.70): BG

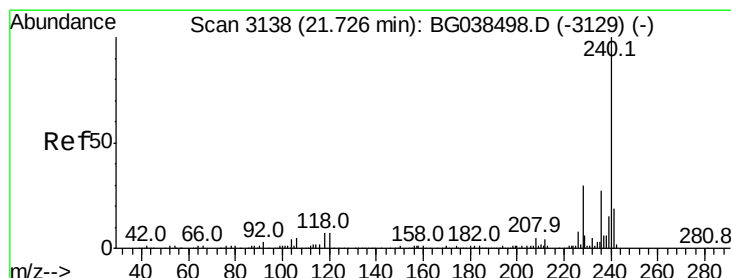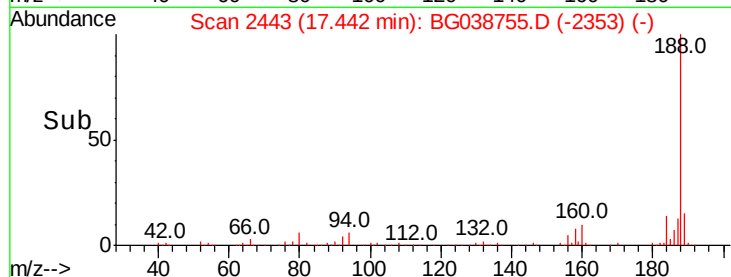
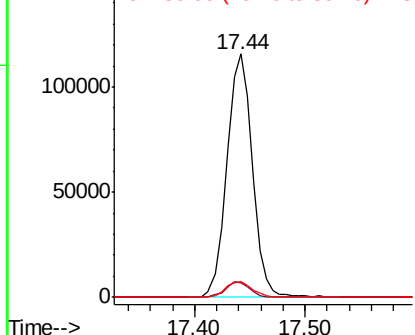



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.72 min Scan# 3171
Delta R.T. -0.01 min
Lab File: BG038755.D
Acq: 20 Dec 2018 9:35

Tgt Ion:240 Resp: 192153
Ion Ratio Lower Upper
240 100
120 5.2 5.3 7.9#
236 26.1 21.4 32.2

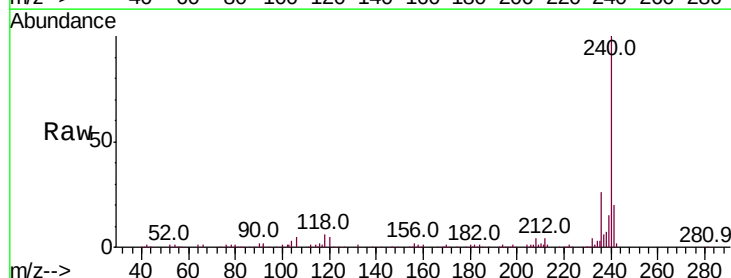

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

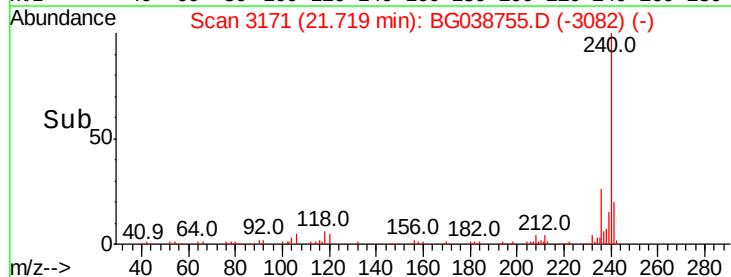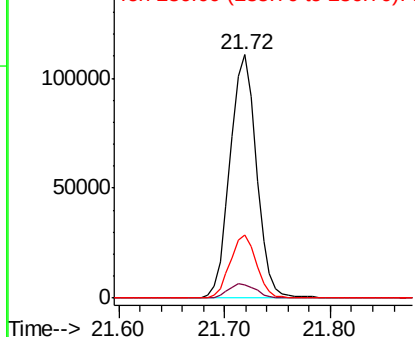

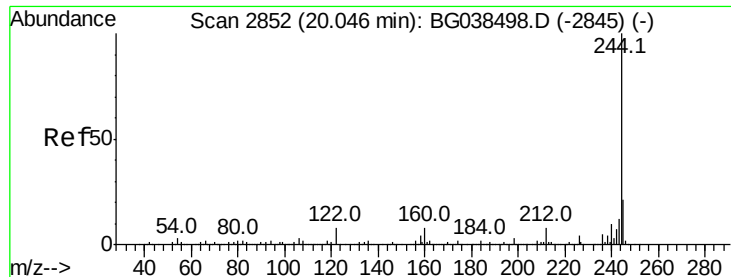

#79

Terphenyl-d14

Concen: 92.137 ng

RT: 20.04 min Scan# 2886

Delta R.T. -0.00 min

Lab File: BG038755.D

Acq: 20 Dec 2018 9:35

Instrument :

BNA_G

ClientSampleId :

EB02_12-14


Tot Ion:244 Resp: 813498

Ion Ratio Lower Upper

244 100

212 7.5 6.2 9.2




122 6.6 6.3 9.5

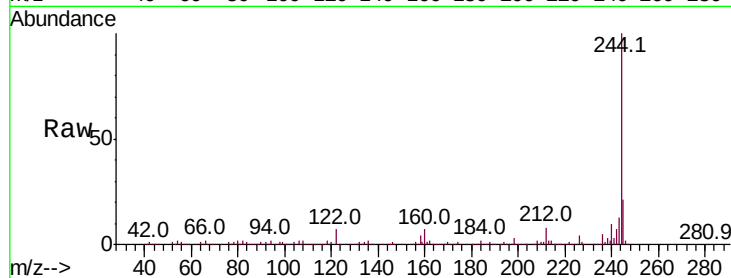

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

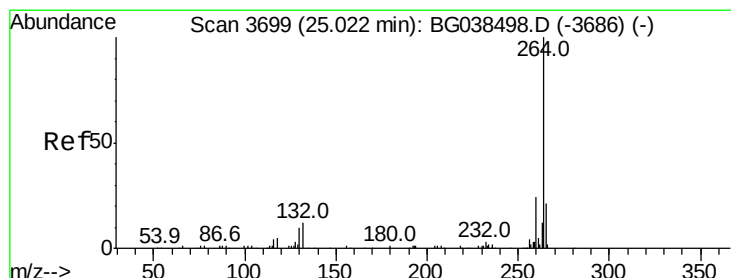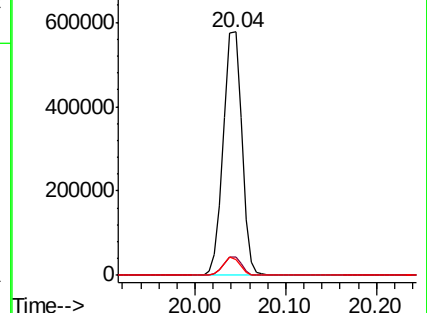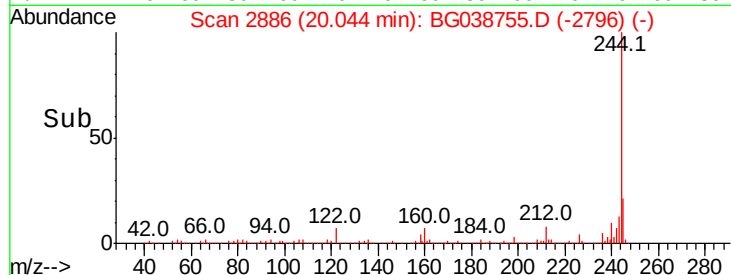

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.02 min Scan# 3732

Delta R.T. -0.01 min

Lab File: BG038755.D

Acq: 20 Dec 2018 9:35


Tgt Ion:264 Resp: 203619

Ion Ratio Lower Upper

264 100

260 22.4 18.9 28.3

265 21.5 17.0 25.4

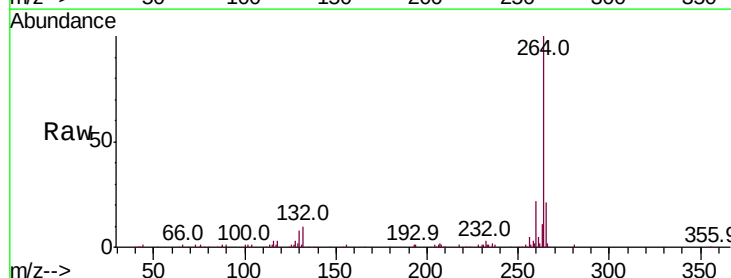

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

