


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121918\
 Data File : BG038745.D
 Acq On : 20 Dec 2018 3:00
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

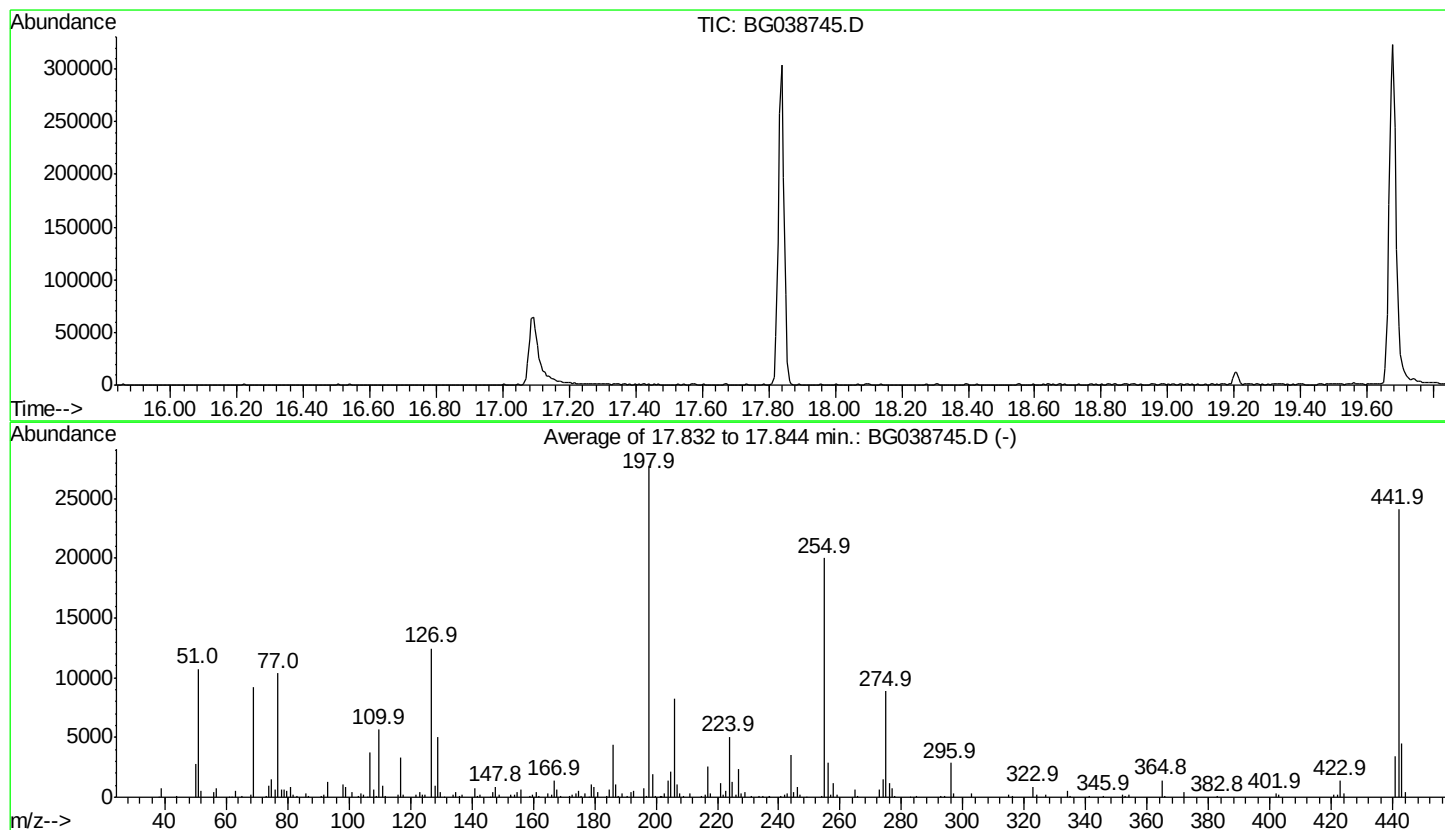

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	10764	PASS
68	69	0.00	2	1.8	169	PASS
69	198	0.00	100	33.1	9183	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.8	12437	PASS
197	198	0.00	2	0.5	126	PASS
198	198	100	100	100.0	27752	PASS
199	198	5	9	7.1	1984	PASS
275	198	10	60	31.9	8866	PASS
365	198	1	100	5.0	1401	PASS
441	198	0.01	100	12.4	3452	PASS
442	198	50	100	86.7	24061	PASS
443	442	15	24	18.7	4506	PASS