
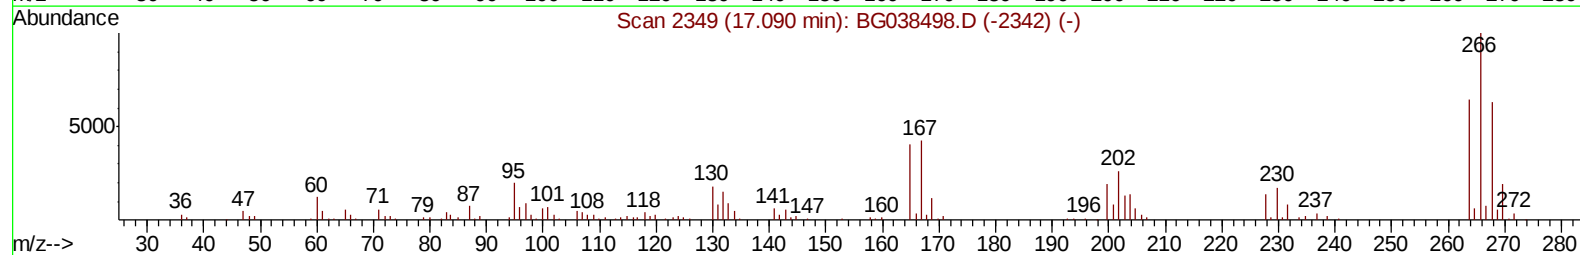
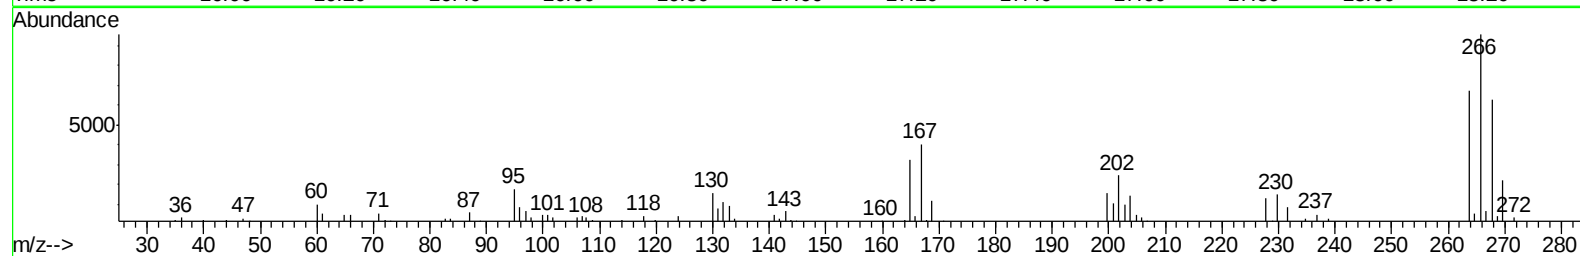


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG122018\
Data File : BG038761.D
Acq On : 20 Dec 2018 14:15
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 21 01:09:33 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

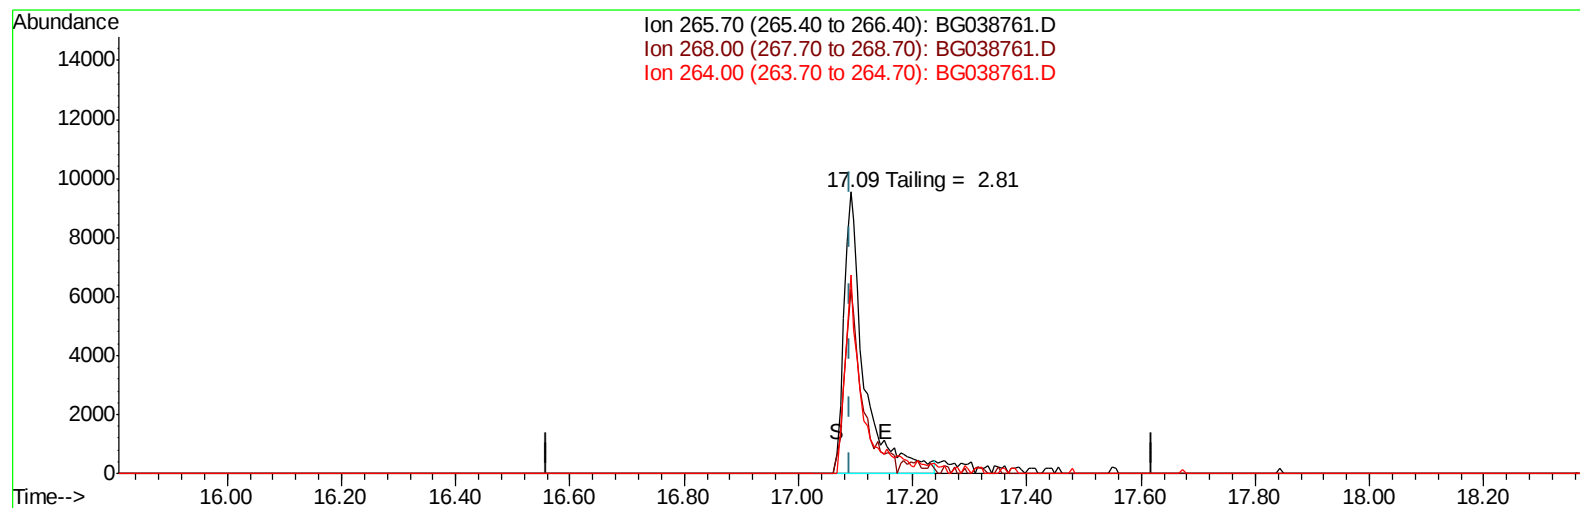

TIC: BG038761.D

(70) Pentachlorophenol (C)




17.091min (+0.001) 25523.37ng

response 22935

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	69.94
264.00	70.90	75.71
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG122018\
 Data File : BG038761.D
 Acq On : 20 Dec 2018 14:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 21 01:09:33 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 12 15:26:27 2018
 Response via : Initial Calibration

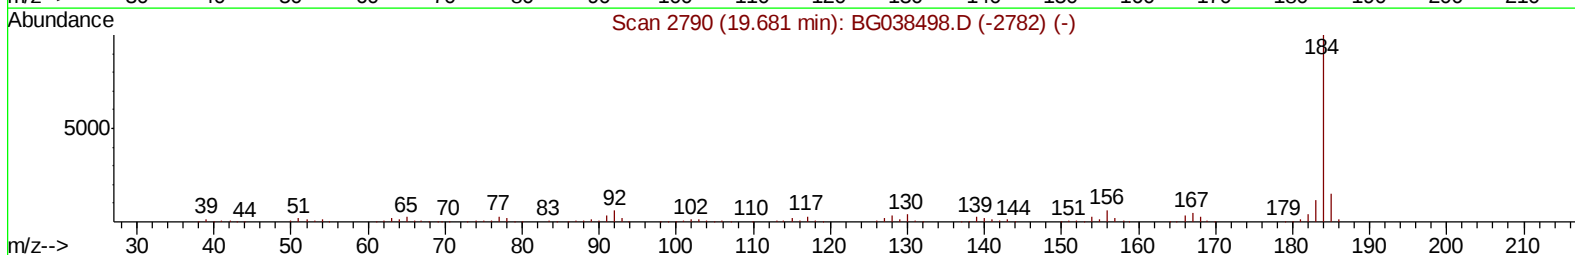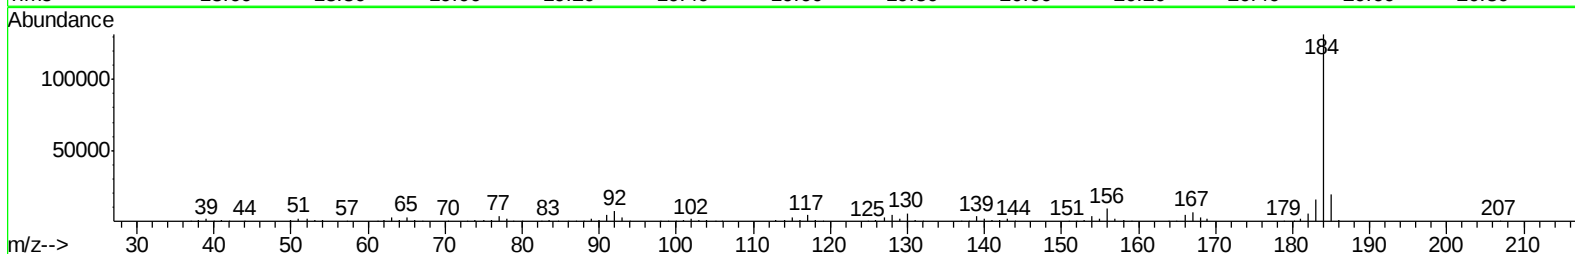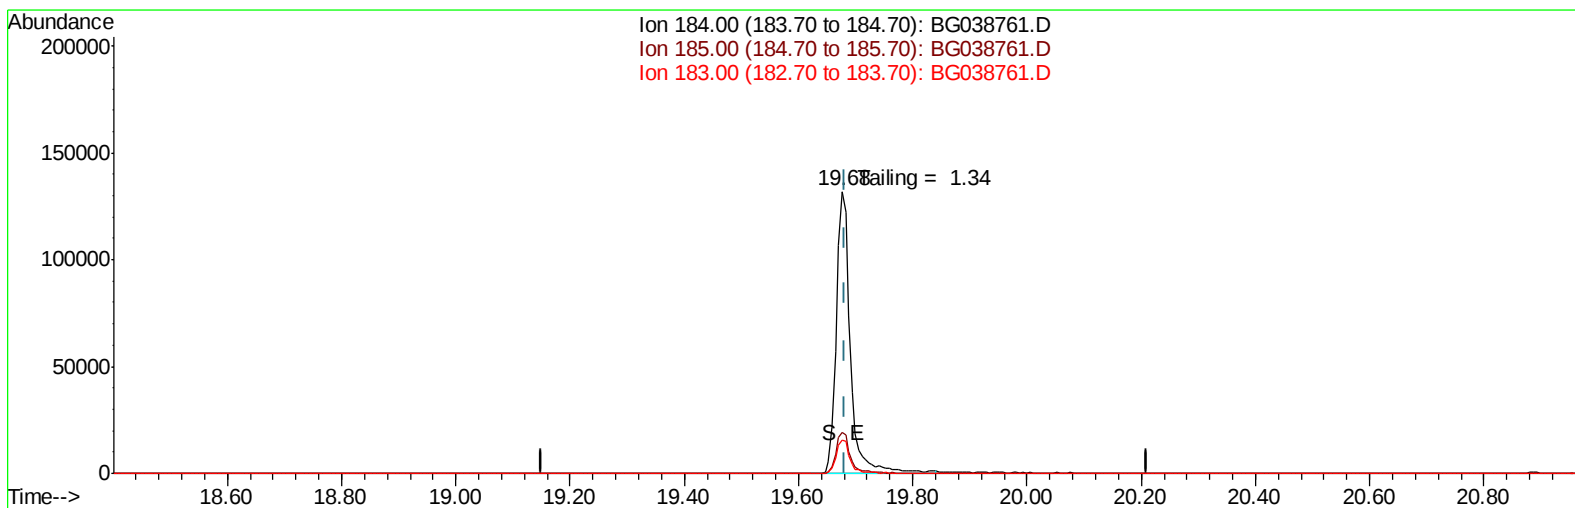

TIC: BG038761.D

(77) Benzidine

19.676min (-0.005) 0.00ng

response 224653

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.68
183.00	12.00	11.98
0.00	0.00	0.00