


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122018\
 Data File : BG038761.D
 Acq On : 20 Dec 2018 14:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

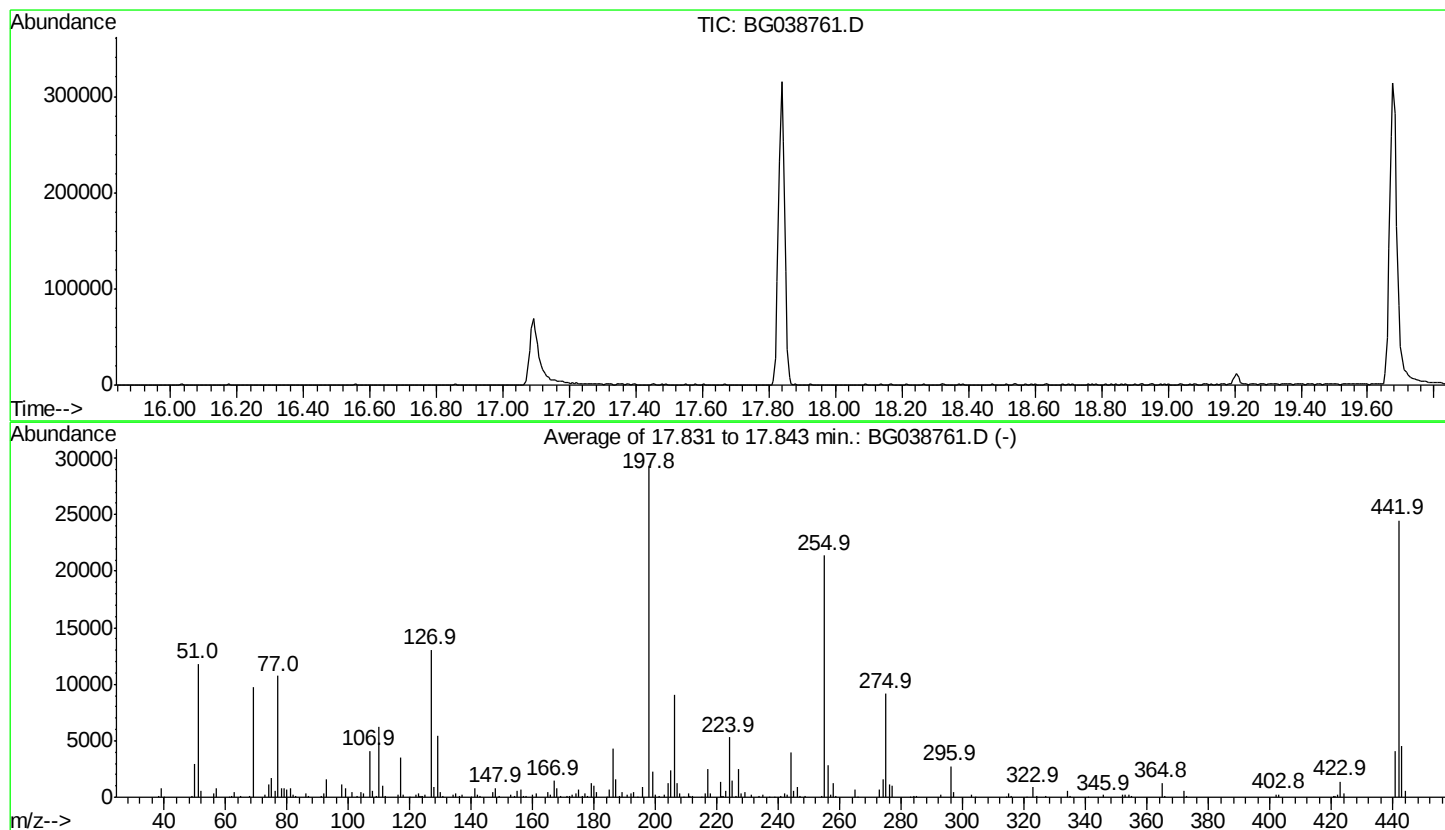

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	11791	PASS
68	69	0.00	2	1.3	128	PASS
69	198	0.00	100	33.2	9752	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.5	13043	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	29338	PASS
199	198	5	9	7.7	2259	PASS
275	198	10	60	31.2	9151	PASS
365	198	1	100	4.3	1255	PASS
441	198	0.01	100	14.1	4132	PASS
442	198	50	100	83.5	24504	PASS
443	442	15	24	18.4	4514	PASS