

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
 Data File : BG051755.D
 Acq On : 22 Dec 2021 17:58
 Operator : CG/JU
 Sample : M5195-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLB6

Quant Time: Dec 22 23:08:28 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 14 14:19:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.270	152	29572	20.000	ng/ul	-0.02
20) Naphthalene-d8	11.107	136	122097	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.908	164	87216	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.657	188	205297	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.975	240	211200	20.000	ng/ul	#-0.01
88) Perylene-d12	25.470	264	205382	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.594	96	4060	5.702	ng/uL	-0.01
4) Pyridine-d5	4.029	84	55119	25.620	ng/ul	-0.02
7) Phenol-d5	7.406	99	73760	27.935	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.577	67	44475	28.334	ng/ul	-0.02
11) 2-Chlorophenol-d4	7.800	132	50747	27.634	ng/ul	-0.01
15) 4-Methylphenol-d8	8.969	113	56828	27.844	ng/ul	-0.01
21) Nitrobenzene-d5	9.439	128	26026	29.074	ng/ul	-0.02
24) 2-Nitrophenol-d4	10.173	143	29464	30.109	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.714	165	57235	26.971	ng/ul	-0.02
31) 4-Chloroaniline-d4	11.231	131	75520	27.029	ng/ul	-0.01
46) Dimethylphthalate-d6	14.297	166	180147	25.806	ng/ul	-0.02
49) Acenaphthylene-d8	14.603	160	231040	26.649	ng/ul	-0.01
54) 4-Nitrophenol-d4	15.072	143	24023	21.162	ng/ul	0.00
60) Fluorene-d10	15.895	176	163447	26.134	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.995	200	20229	18.912	ng/ul	-0.02
73) Anthracene-d10	17.751	188	260155	26.565	ng/ul	-0.01
81) Pyrene-d10	20.030	212	309036	24.312	ng/ul	-0.01
92) Benzo(a)pyrene-d12	25.229	264	289132	26.756	ng/ul	-0.02
Target Compounds						
					Qvalue	
8) Phenol	7.430	94	4640	1.767	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
Data File : BG051755.D
Acq On : 22 Dec 2021 17:58
Operator : CG/JU
Sample : M5195-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLB6

Quant Time: Dec 22 23:08:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 14 14:19:57 2021
Response via : Initial Calibration

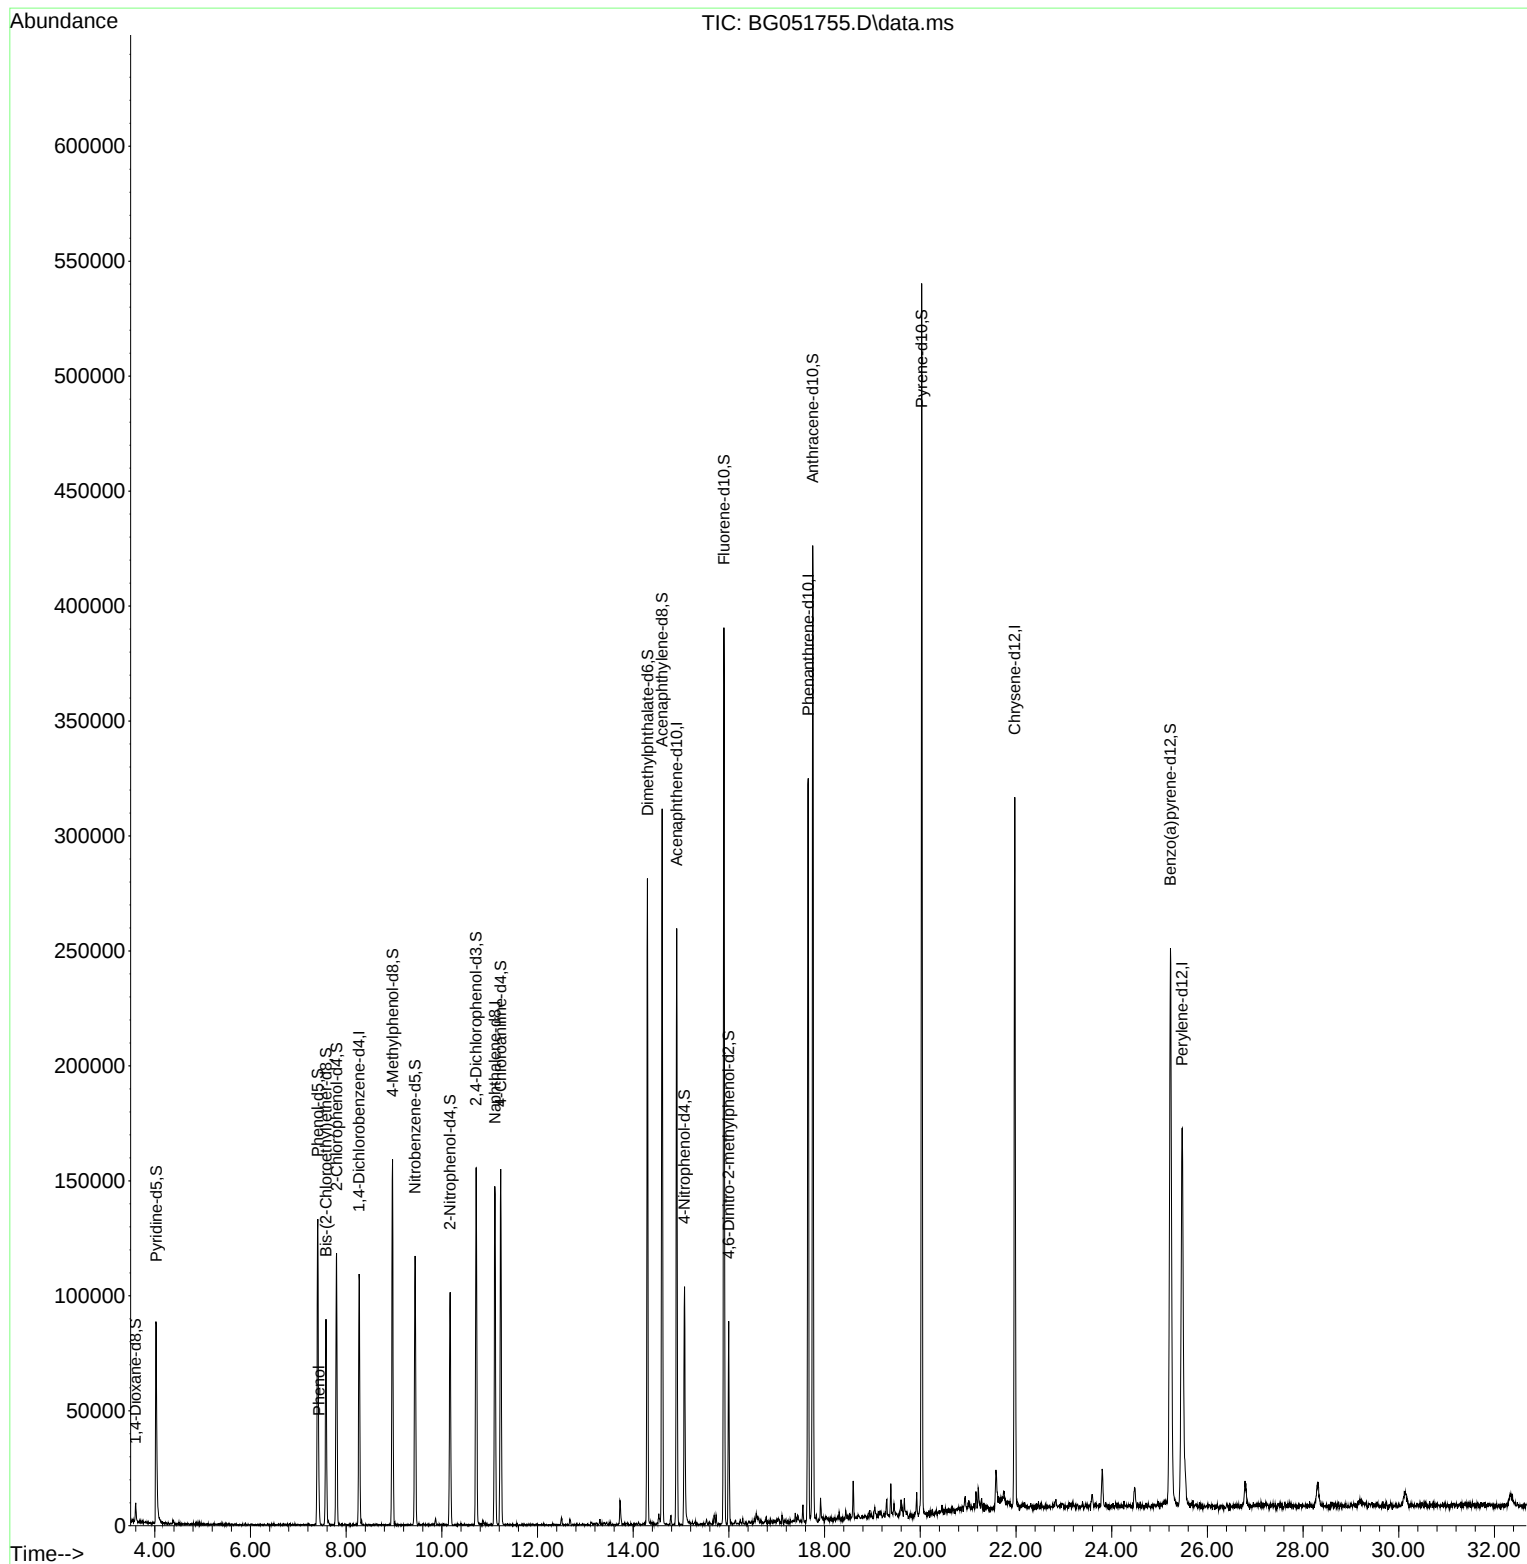

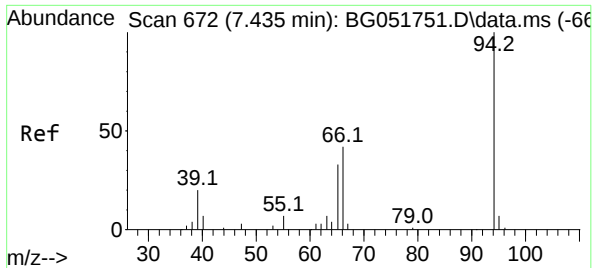

Phenol
 Concen: 1.767 ng/ul
 RT: 7.430 min Scan# 61
 Delta R.T. -0.011 min
 Lab File: BG051755.D
 Acq: 22 Dec 2021 17:58

Instrument :
 BNA_G
 ClientSampleId :
 BGLB6

Tgt Ion: 94 Resp: 4640
 Ion Ratio Lower Upper
 94 100
 65 40.7 25.1 37.7#
 66 51.1 31.6 47.4#

