

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
 Data File : BG051772.D
 Acq On : 23 Dec 2021 6:03
 Operator : CG/JU
 Sample : M5195-15
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLC7

Quant Time: Dec 23 06:41:54 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 14 14:19:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.271	152	38826	20.000	ng/u1	-0.02
20) Naphthalene-d8	11.108	136	155889	20.000	ng/u1	#-0.02
38) Acenaphthene-d10	14.909	164	108987	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.652	188	241625	20.000	ng/u1	#-0.01
79) Chrysene-d12	21.970	240	205413	20.000	ng/u1	#-0.02
88) Perylene-d12	25.471	264	209876	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.601	96	4049	4.331	ng/uL	0.00
4) Pyridine-d5	4.024	84	42861	15.174	ng/u1	-0.02
7) Phenol-d5	7.401	99	86813	25.042	ng/u1	-0.02
9) Bis-(2-Chloroethyl)eth...	7.572	67	51321	24.903	ng/u1	-0.02
11) 2-Chlorophenol-d4	7.795	132	62099	25.756	ng/u1	-0.02
15) 4-Methylphenol-d8	8.964	113	64308	23.999	ng/u1	-0.02
21) Nitrobenzene-d5	9.440	128	32717	28.626	ng/u1	-0.02
24) 2-Nitrophenol-d4	10.174	143	36210	28.982	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.714	165	70412	25.988	ng/u1	-0.02
31) 4-Chloroaniline-d4	11.231	131	69080	19.365	ng/u1	-0.01
46) Dimethylphthalate-d6	14.298	166	220875	25.320	ng/u1	-0.02
49) Acenaphthylene-d8	14.603	160	281118	25.948	ng/u1	-0.01
54) 4-Nitrophenol-d4	15.073	143	32106	22.633	ng/u1	0.00
60) Fluorene-d10	15.896	176	197130	25.223	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.996	200	27921	22.179	ng/u1	-0.02
73) Anthracene-d10	17.752	188	294612	25.560	ng/u1	-0.01
81) Pyrene-d10	20.031	212	328171	26.545	ng/u1	-0.01
92) Benzo(a)pyrene-d12	25.230	264	294153	26.637	ng/u1	-0.02
Target Compounds						
					Qvalue	
8) Phenol	7.431	94	4601	1.335	ng/u1#	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
Data File : BG051772.D
Acq On : 23 Dec 2021 6:03
Operator : CG/JU
Sample : M5195-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLC7

Quant Time: Dec 23 06:41:54 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 14 14:19:57 2021
Response via : Initial Calibration

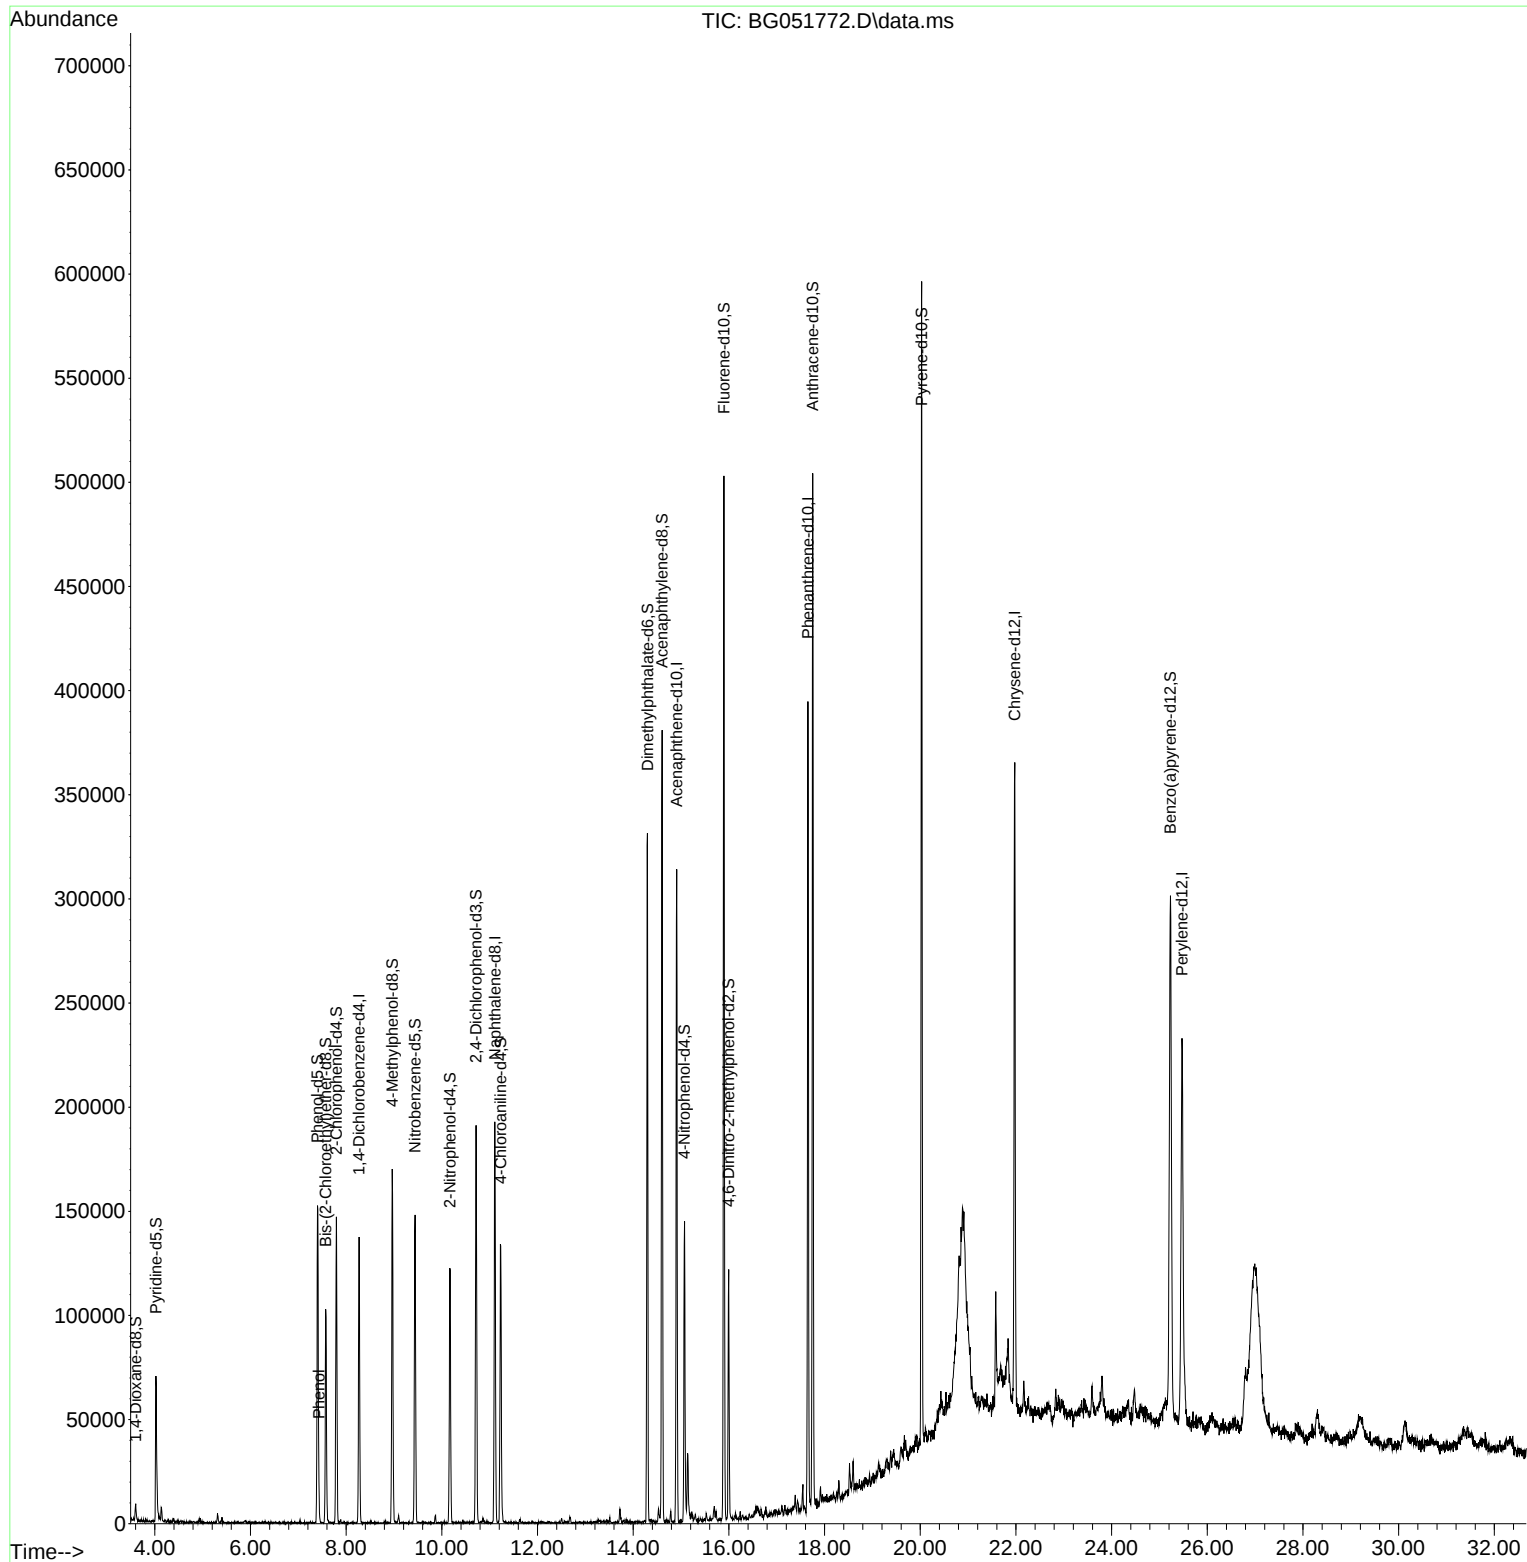

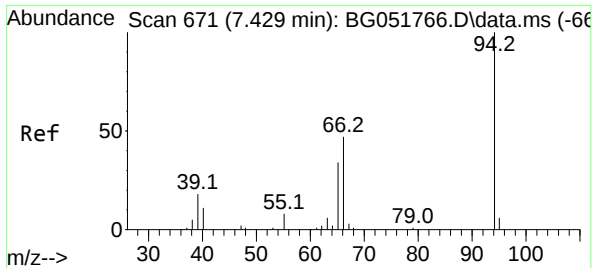

Phenol
 Concen: 1.335 ng/ul
 RT: 7.431 min Scan# 61
 Delta R.T. -0.010 min
 Lab File: BG051772.D
 Acq: 23 Dec 2021 6:03

Instrument :
 BNA_G
 ClientSampleId :
 BGLC7

Tgt Ion: 94	Resp:	4601
Ion	Ratio	Lower Upper
94	100	
65	28.2	25.1 37.7
66	51.7	31.6 47.4#

