

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
 Data File : BG051756.D
 Acq On : 22 Dec 2021 18:39
 Operator : CG/JU
 Sample : M5195-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051756.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.600	14	19	24	rBV2	8977	12904	1.42%	0.126%
2	3.752	42	45	48	rBV4	1283	1492	0.16%	0.015%
3	4.023	87	91	103	rBV	107910	188169	20.78%	1.837%
4	4.387	149	153	156	rVB	2002	2606	0.29%	0.025%
5	5.103	271	275	277	rVB	1003	1273	0.14%	0.012%
6	7.406	659	667	679	rBV	157526	290153	32.04%	2.832%
7	7.577	690	696	703	rBV	105980	175467	19.37%	1.713%
8	7.794	727	733	745	rVB	135450	240107	26.51%	2.344%
9	8.041	772	775	778	rBV	886	1244	0.14%	0.012%
10	8.270	808	814	821	rBV	122633	211721	23.38%	2.066%
11	8.323	821	823	827	rVB2	2450	1985	0.22%	0.019%
12	8.969	924	933	940	rBV	182881	320309	35.37%	3.126%
13	9.439	1006	1013	1021	rVB	145141	260027	28.71%	2.538%
14	9.868	1082	1086	1091	rVB3	3013	4051	0.45%	0.040%
15	10.173	1131	1138	1145	rBV	119267	214035	23.63%	2.089%
16	10.714	1223	1230	1240	rBV	184280	334001	36.88%	3.260%
17	10.860	1249	1255	1260	rBV3	3647	6523	0.72%	0.064%
18	11.107	1289	1297	1308	rBV	171122	312019	34.45%	3.045%
19	11.230	1311	1318	1326	rBV	177452	320814	35.42%	3.131%
20	12.499	1526	1534	1540	rBV4	4371	6746	0.74%	0.066%
21	12.681	1559	1565	1569	rVB4	2660	4495	0.50%	0.044%
22	13.122	1636	1640	1642	rBV	1122	1293	0.14%	0.013%
23	13.298	1667	1670	1673	rVB2	2472	3208	0.35%	0.031%
24	13.392	1681	1686	1689	rBV2	1742	2765	0.31%	0.027%
25	13.439	1692	1694	1698	rVB2	1608	1952	0.22%	0.019%
26	13.727	1738	1743	1750	rVV2	12279	20111	2.22%	0.196%
27	13.809	1752	1757	1761	rVB2	1304	1666	0.18%	0.016%
28	14.297	1833	1840	1847	rBV	332310	488732	53.96%	4.770%
29	14.526	1877	1879	1885	rBV3	5154	8022	0.89%	0.078%
30	14.602	1885	1892	1901	rVB	374462	596407	65.85%	5.821%
31	14.784	1919	1923	1932	rVB3	5555	7394	0.82%	0.072%
32	14.908	1937	1944	1951	rVB	294269	455147	50.26%	4.442%
33	15.072	1964	1972	1984	rBV	132304	219848	24.27%	2.146%
34	15.296	2008	2010	2013	rVB2	2214	2052	0.23%	0.020%
35	15.395	2025	2027	2030	rVB4	1563	1455	0.16%	0.014%
36	15.478	2036	2041	2042	rBV5	5017	6857	0.76%	0.067%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
 Data File : BG051756.D
 Acq On : 22 Dec 2021 18:39
 Operator : CG/JU
 Sample : M5195-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	15.695	2074	2078	2081	rBV3	4218	6105	0.67%	0.060%
38	15.736	2081	2085	2088	rVB3	3873	4448	0.49%	0.043%
39	15.895	2106	2112	2119	rBV	455630	720213	79.52%	7.030%
40	15.995	2124	2129	2137	rVB2	106462	155562	17.18%	1.518%
41	16.141	2152	2154	2158	rVB4	2661	2648	0.29%	0.026%
42	16.235	2167	2170	2172	rVV4	2551	2269	0.25%	0.022%
43	16.288	2175	2179	2182	rBV3	2534	3138	0.35%	0.031%
44	16.418	2195	2201	2204	rBV3	2311	3438	0.38%	0.034%
45	16.529	2216	2220	2222	rBV4	3299	3482	0.38%	0.034%
46	16.564	2223	2226	2229	rBV3	3681	5314	0.59%	0.052%
47	16.776	2259	2262	2266	rVB3	2967	3629	0.40%	0.035%
48	16.882	2278	2280	2286	rVB3	2168	2849	0.31%	0.028%
49	16.940	2286	2290	2292	rBV4	2371	3136	0.35%	0.031%
50	16.999	2296	2300	2303	rBV4	2245	3019	0.33%	0.029%
51	17.034	2304	2306	2307	rBV	2408	1452	0.16%	0.014%
52	17.111	2315	2319	2322	rBV4	4852	5270	0.58%	0.051%
53	17.387	2364	2366	2370	rVB5	4325	4302	0.48%	0.042%
54	17.440	2371	2375	2378	rVB5	4702	5698	0.63%	0.056%
55	17.545	2390	2393	2399	rVB5	8923	11077	1.22%	0.108%
56	17.657	2405	2412	2418	rBV	371890	567692	62.68%	5.541%
57	17.757	2422	2429	2438	rVV	492890	785947	86.78%	7.671%
58	17.822	2438	2440	2444	rVB3	3560	4303	0.48%	0.042%
59	17.916	2452	2456	2461	rBV	6092	9628	1.06%	0.094%
60	18.303	2520	2522	2526	rVB5	4766	5594	0.62%	0.055%
61	18.526	2556	2560	2564	rBV4	15147	21244	2.35%	0.207%
62	18.597	2568	2572	2576	rVB	19534	24582	2.71%	0.240%
63	19.055	2645	2650	2653	rBV7	5037	9634	1.06%	0.094%
64	19.302	2689	2692	2695	rVB3	7062	8346	0.92%	0.081%
65	19.384	2703	2706	2709	rBV2	9939	12093	1.34%	0.118%
66	19.666	2752	2754	2760	rVB2	8915	10818	1.19%	0.106%
67	20.030	2810	2816	2823	rVB	629786	905662	100.00%	8.840%
68	21.575	3075	3079	3089	rBV3	51189	103877	11.47%	1.014%
69	21.975	3140	3147	3159	rVB	352942	609352	67.28%	5.947%
70	22.498	3234	3236	3240	rBV4	3097	4103	0.45%	0.040%
71	23.473	3400	3402	3404	rBV2	2842	2311	0.26%	0.023%
72	23.584	3419	3421	3423	rBV3	4451	4171	0.46%	0.041%
73	24.418	3562	3563	3564	rBV	2823	1394	0.15%	0.014%
74	25.229	3691	3701	3716	rVB2	276645	847530	93.58%	8.272%
75	25.329	3716	3718	3720	rBV3	3165	1662	0.18%	0.016%
76	25.470	3732	3742	3759	rBV2	185544	604067	66.70%	5.896%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
Data File : BG051756.D
Acq On : 22 Dec 2021 18:39
Operator : CG/JU
Sample : M5195-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLB7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Title : SVOA CALIBRATION

77	26.792	3963	3967	3973	rVB7	7678	16694	1.84%	0.163%
78	27.620	4107	4108	4111	rBV2	3533	2343	0.26%	0.023%
79	27.749	4128	4130	4131	rBV2	3103	2136	0.24%	0.021%
80	28.842	4314	4316	4317	rBV2	2960	1789	0.20%	0.017%
81	31.932	4840	4842	4844	rBV2	4081	2685	0.30%	0.026%
82	32.096	4868	4870	4872	rBV3	2458	1760	0.19%	0.017%



Sum of corrected areas: 10245516

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
Data File : BG051756.D
Acq On : 22 Dec 2021 18:39
Operator : CG/JU
Sample : M5195-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

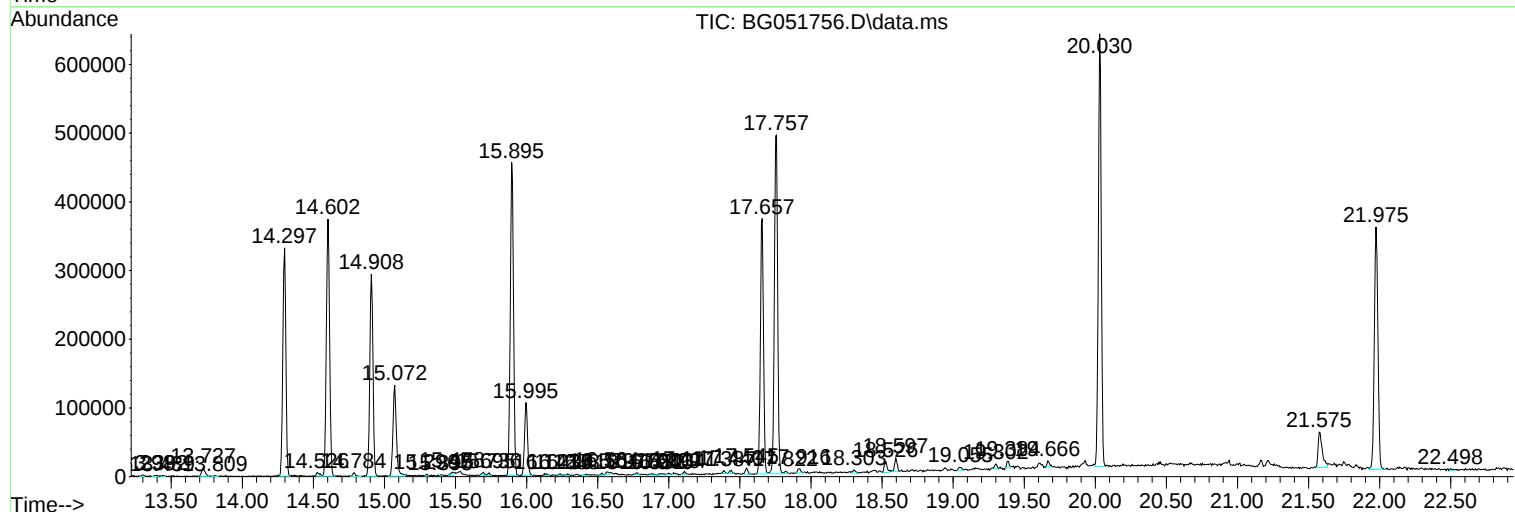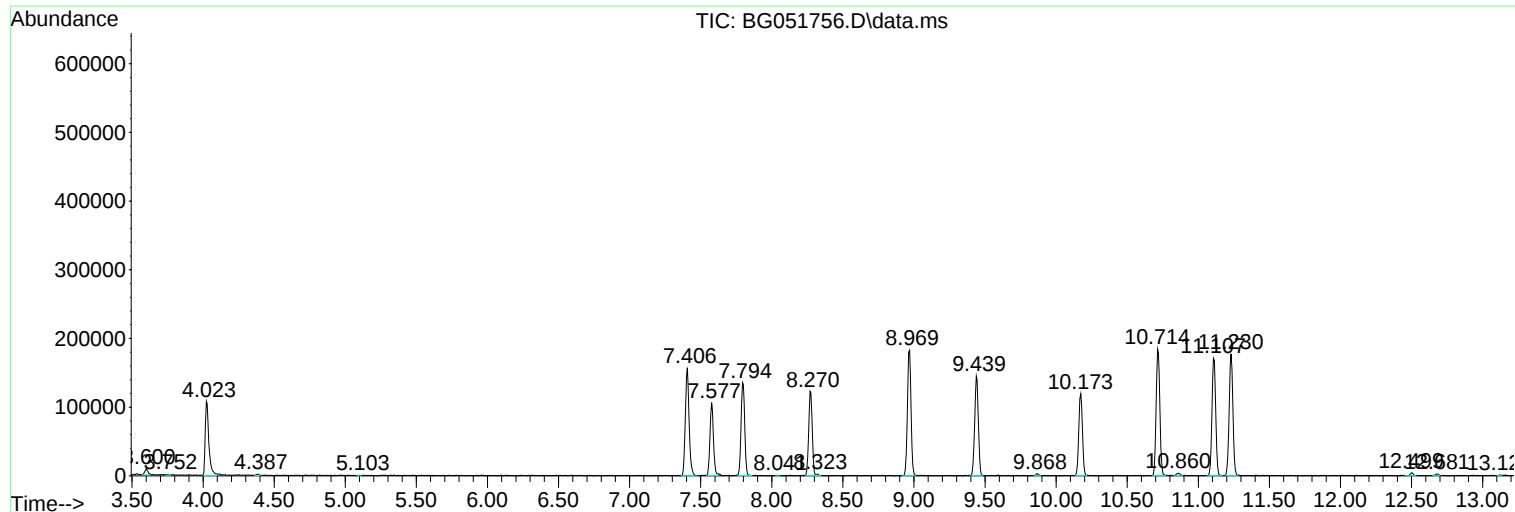

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
Data File : BG051756.D
Acq On : 22 Dec 2021 18:39
Operator : CG/JU
Sample : M5195-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLB7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Trichloroacetic acid, penta... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.575	3.41 ng/ul	103877	Chrysene-d12	21.975

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	94
2		1-Hexacosene	364	C26H52	018835-33-1	91
3		Bromoacetic acid, octadecyl ester	390	C20H39BrO2	018992-03-5	91
4		Cyclopentadecane	210	C15H30	000295-48-7	91
5		1-Tetracosene	336	C24H48	010192-32-2	91

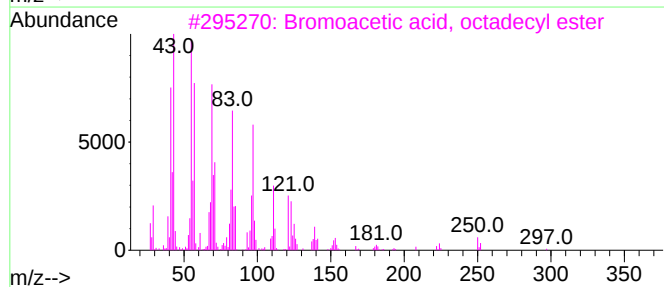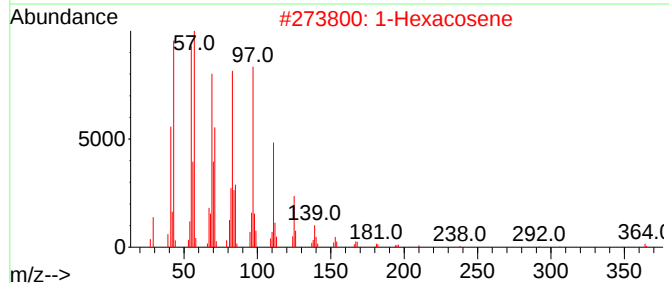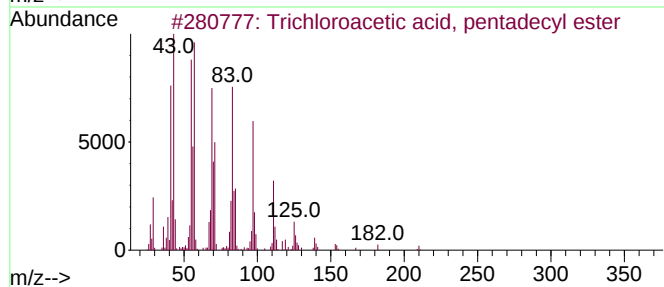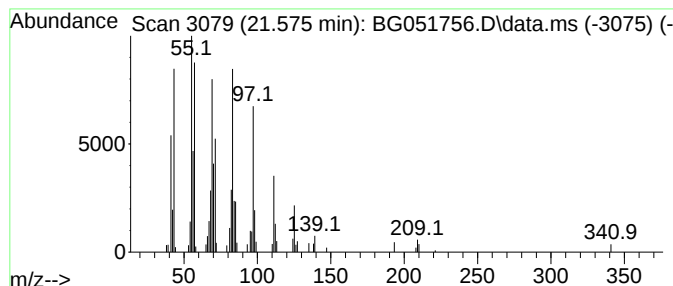

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
Data File : BG051756.D
Acq On : 22 Dec 2021 18:39
Operator : CG/JU
Sample : M5195-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Trichloroacetic...	21.575	3.4	ng/ul	103877	5	21.975	609352	20.0