

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
 Data File : BG051761.D
 Acq On : 22 Dec 2021 22:01
 Operator : CG/JU
 Sample : M5195-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051761.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.601	14	19	23	rBV3	8108	11565	1.22%	0.107%
2	4.024	86	91	101	rBV	110520	190304	20.04%	1.769%
3	4.382	149	152	154	rBV	2043	2274	0.24%	0.021%
4	4.629	190	194	200	rVB2	1498	2069	0.22%	0.019%
5	7.408	659	667	680	rVB	164012	306073	32.23%	2.845%
6	7.578	689	696	703	rBV	110556	182716	19.24%	1.698%
7	7.795	726	733	740	rBV	149143	257571	27.13%	2.394%
8	8.271	805	814	821	rBV2	127756	217808	22.94%	2.024%
9	8.964	926	932	940	rBV	195220	340702	35.88%	3.166%
10	9.053	943	947	951	rVB	990	1282	0.14%	0.012%
11	9.440	1004	1013	1022	rBV2	150381	275508	29.01%	2.560%
12	9.599	1033	1040	1043	rBV2	2235	3215	0.34%	0.030%
13	9.869	1082	1086	1091	rBV3	2842	3743	0.39%	0.035%
14	10.175	1129	1138	1145	rBV	129054	234022	24.65%	2.175%
15	10.715	1222	1230	1239	rBV	197637	354426	37.33%	3.294%
16	10.862	1249	1255	1260	rVB3	8122	14245	1.50%	0.132%
17	11.109	1289	1297	1304	rBV	177456	320310	33.73%	2.977%
18	11.232	1310	1318	1330	rVB	186920	342208	36.04%	3.180%
19	12.501	1531	1534	1537	rBV2	1807	2430	0.26%	0.023%
20	12.683	1558	1565	1568	rVB2	3746	5841	0.62%	0.054%
21	13.300	1665	1670	1674	rVB2	1513	1872	0.20%	0.017%
22	13.511	1702	1706	1710	rBV3	1747	3030	0.32%	0.028%
23	13.729	1738	1743	1747	rBV4	5693	9485	1.00%	0.088%
24	13.846	1761	1763	1767	rBV2	918	1313	0.14%	0.012%
25	14.292	1832	1839	1847	rBV	348013	527118	55.51%	4.899%
26	14.527	1875	1879	1885	rBV5	7639	12288	1.29%	0.114%
27	14.604	1885	1892	1898	rVV	408585	634579	66.83%	5.897%
28	14.780	1919	1922	1926	rVB3	3726	4480	0.47%	0.042%
29	14.909	1936	1944	1952	rVB	300707	468703	49.36%	4.356%
30	15.074	1965	1972	1981	rBV2	148500	247852	26.10%	2.303%
31	15.291	2005	2009	2013	rBV4	1219	2221	0.23%	0.021%
32	15.467	2035	2039	2041	rVB	1140	1380	0.15%	0.013%
33	15.532	2044	2050	2053	rVV3	3251	4379	0.46%	0.041%
34	15.691	2071	2077	2082	rBV5	6491	12771	1.34%	0.119%
35	15.732	2082	2084	2087	rVB3	2472	3217	0.34%	0.030%
36	15.896	2105	2112	2119	rVB	522013	779011	82.04%	7.240%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
 Data File : BG051761.D
 Acq On : 22 Dec 2021 22:01
 Operator : CG/JU
 Sample : M5195-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	15.996	2121	2129	2141	rVV2	123965	184201	19.40%	1.712%
38	16.137	2151	2153	2157	rVB3	2520	2800	0.29%	0.026%
39	16.237	2167	2170	2175	rVB5	3418	4619	0.49%	0.043%
40	16.284	2175	2178	2182	rBV3	1941	2998	0.32%	0.028%

41	16.349	2185	2189	2191	rBV3	3553	3972	0.42%	0.037%
42	16.425	2198	2202	2206	rBV4	2328	3751	0.40%	0.035%
43	16.525	2218	2219	2223	rBV4	2302	2477	0.26%	0.023%
44	16.566	2223	2226	2228	rBV2	3357	4473	0.47%	0.042%
45	16.677	2239	2245	2248	rVB4	2715	4283	0.45%	0.040%

46	16.713	2248	2251	2253	rBV2	1461	1568	0.17%	0.015%
47	16.771	2257	2261	2265	rVB5	2890	3835	0.40%	0.036%
48	16.877	2276	2279	2280	rBV2	1223	1397	0.15%	0.013%
49	16.942	2284	2290	2293	rBV4	2704	4040	0.43%	0.038%
50	17.006	2299	2301	2302	rVB2	1911	1343	0.14%	0.012%

51	17.036	2304	2306	2308	rBV3	1971	1656	0.17%	0.015%
52	17.112	2315	2319	2324	rVB3	4505	6301	0.66%	0.059%
53	17.165	2326	2328	2333	rBV4	1867	3013	0.32%	0.028%
54	17.353	2357	2360	2362	rBV3	1079	1545	0.16%	0.014%
55	17.388	2362	2366	2371	rVV4	5652	8048	0.85%	0.075%

56	17.435	2371	2374	2379	rVB4	4543	7694	0.81%	0.072%
57	17.482	2379	2382	2383	rBV3	1835	1705	0.18%	0.016%
58	17.506	2383	2386	2388	rBV3	1899	1481	0.16%	0.014%
59	17.541	2389	2392	2399	rVB3	8955	12081	1.27%	0.112%
60	17.611	2401	2404	2405	rBV3	1380	1387	0.15%	0.013%

61	17.653	2405	2411	2418	rBV	377519	580696	61.15%	5.397%
62	17.752	2422	2428	2435	rVB	563661	836176	88.06%	7.771%
63	17.823	2437	2440	2443	rVB3	3641	3481	0.37%	0.032%
64	17.917	2451	2456	2459	rBV	9506	14272	1.50%	0.133%
65	18.011	2470	2472	2473	rBV2	2287	1444	0.15%	0.013%

66	18.246	2510	2512	2518	rBV6	1561	3025	0.32%	0.028%
67	18.305	2518	2522	2526	rVV6	5935	7919	0.83%	0.074%
68	18.358	2530	2531	2535	rVB4	1712	1404	0.15%	0.013%
69	18.440	2544	2545	2548	rVB2	2344	1976	0.21%	0.018%
70	18.522	2556	2559	2565	rVB5	5655	9422	0.99%	0.088%

71	18.598	2568	2572	2576	rVB	21404	27593	2.91%	0.256%
72	18.822	2607	2610	2615	rBV7	2435	4390	0.46%	0.041%
73	18.945	2627	2631	2635	rBV6	6851	7815	0.82%	0.073%
74	19.051	2646	2649	2652	rBV4	3157	4007	0.42%	0.037%
75	19.133	2659	2663	2666	rBV4	6766	9640	1.02%	0.090%

76	19.297	2689	2691	2696	rVB3	4555	3876	0.41%	0.036%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
 Data File : BG051761.D
 Acq On : 22 Dec 2021 22:01
 Operator : CG/JU
 Sample : M5195-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLC3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	19.386	2703	2706	2709	rVB4	6334	7849	0.83%	0.073%
78	19.444	2714	2716	2717	rBV2	2952	1593	0.17%	0.015%
79	19.597	2738	2742	2745	rBV6	8074	10987	1.16%	0.102%
80	19.668	2750	2754	2757	rVV3	11854	16256	1.71%	0.151%
81	19.697	2757	2759	2763	rVB4	8108	8367	0.88%	0.078%
82	19.873	2785	2789	2790	rBV3	3076	4312	0.45%	0.040%
83	19.973	2804	2806	2807	rBV2	2603	1492	0.16%	0.014%
84	20.032	2809	2816	2822	rVV	659521	949563	100.00%	8.825%
85	21.166	3005	3009	3012	rBV5	11286	17539	1.85%	0.163%
86	21.577	3075	3079	3085	rVB3	31077	46636	4.91%	0.433%
87	21.976	3140	3147	3154	rVB2	339729	598951	63.08%	5.566%
88	24.479	3567	3573	3580	rVB7	10274	25039	2.64%	0.233%
89	25.231	3692	3701	3718	rVB2	297797	887391	93.45%	8.247%
90	25.471	3732	3742	3759	rVB2	186673	614366	64.70%	5.710%




Sum of corrected areas: 10760156

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
Data File : BG051761.D
Acq On : 22 Dec 2021 22:01
Operator : CG/JU
Sample : M5195-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

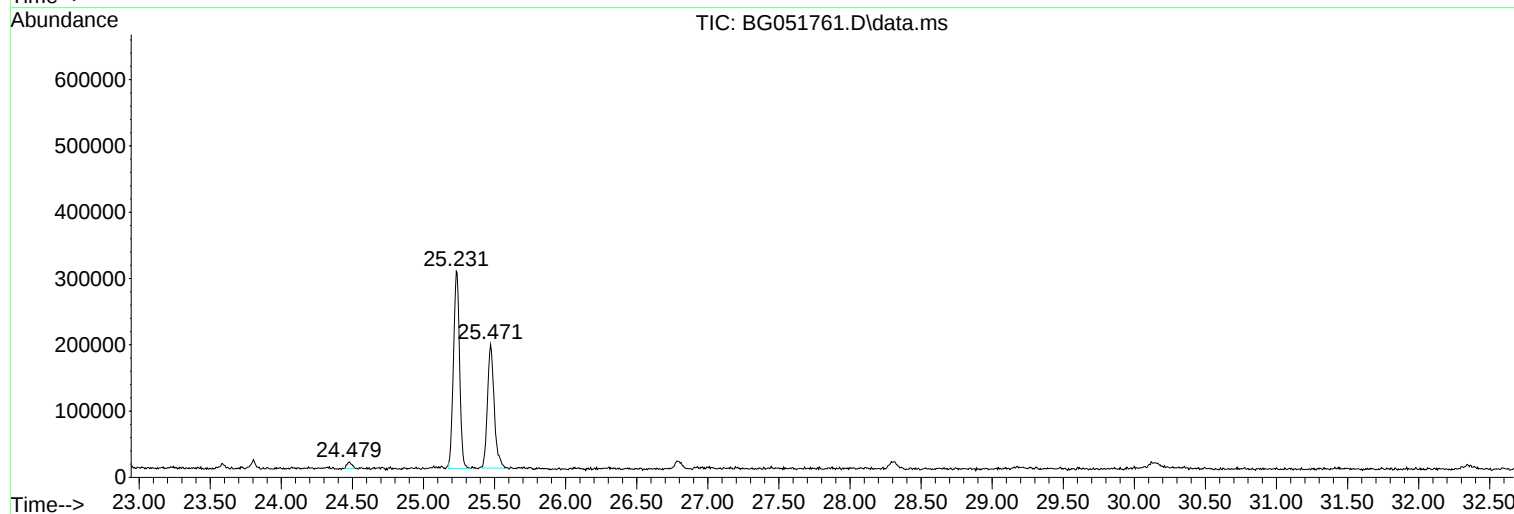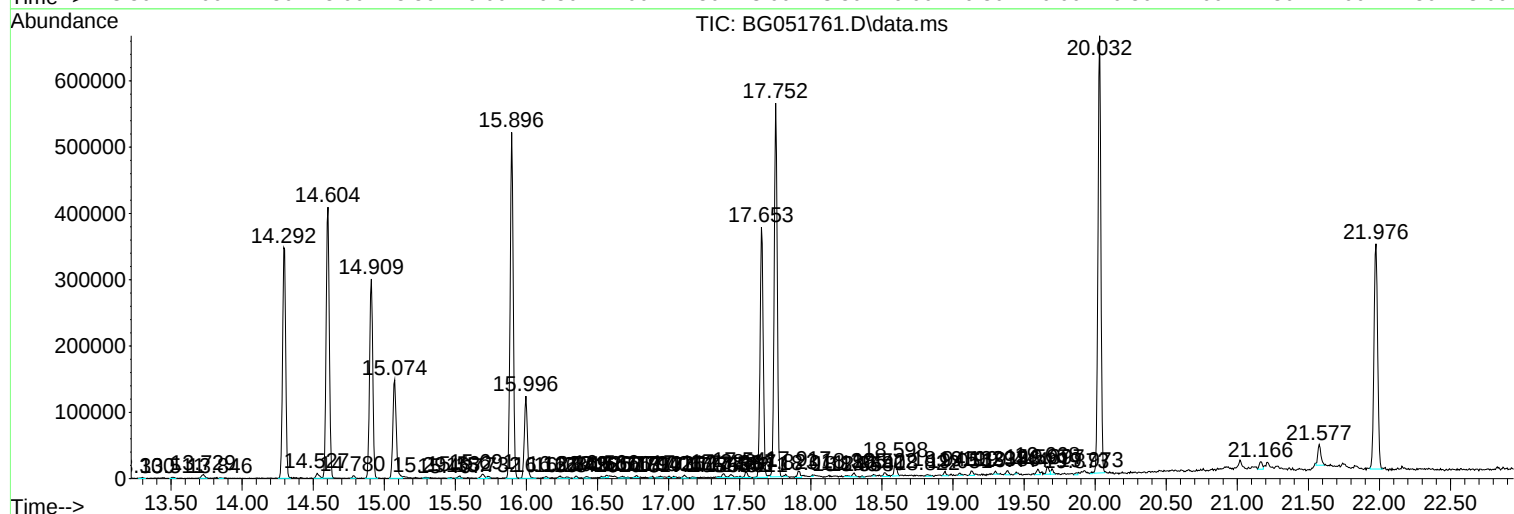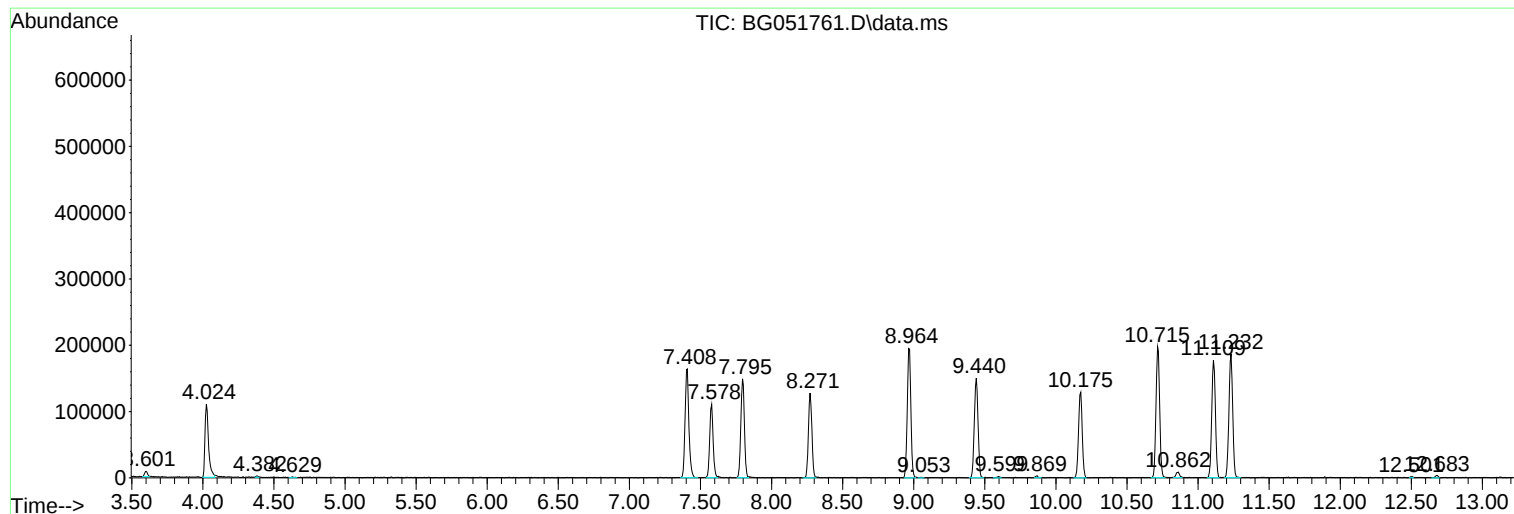

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
Data File : BG051761.D
Acq On : 22 Dec 2021 22:01
Operator : CG/JU
Sample : M5195-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
Data File : BG051761.D
Acq On : 22 Dec 2021 22:01
Operator : CG/JU
Sample : M5195-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc