

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
 Data File : BG051762.D
 Acq On : 22 Dec 2021 22:42
 Operator : CG/JU
 Sample : M5195-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLC1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051762.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.600	15	19	24	rBV	7887	12108	1.29%	0.126%
2	4.387	148	153	156	rVB2	2452	3308	0.35%	0.034%
3	7.407	660	667	677	rVB	146796	265377	28.27%	2.752%
4	7.577	689	696	703	rBV	101028	175108	18.66%	1.816%
5	7.794	726	733	743	rVB	132733	230680	24.58%	2.392%
6	8.270	806	814	821	rBV	111531	192374	20.50%	1.995%
7	8.963	925	932	941	rBV	157719	279339	29.76%	2.897%
8	9.439	1003	1013	1020	rVB	144396	256329	27.31%	2.658%
9	9.598	1037	1040	1045	rBV2	1242	1897	0.20%	0.020%
10	9.862	1077	1085	1089	rBV3	3711	5224	0.56%	0.054%
11	10.173	1130	1138	1145	rBV	103023	187798	20.01%	1.947%
12	10.714	1223	1230	1241	rBV	175444	315762	33.64%	3.274%
13	11.107	1290	1297	1304	rVB	157985	282270	30.07%	2.927%
14	11.225	1311	1317	1328	rVB	127327	238957	25.46%	2.478%
15	12.500	1530	1534	1539	rBV4	2235	3364	0.36%	0.035%
16	12.682	1558	1565	1570	rBV2	2195	3865	0.41%	0.040%
17	13.269	1661	1665	1668	rBV	815	1384	0.15%	0.014%
18	13.299	1668	1670	1676	rVB2	1931	2488	0.27%	0.026%
19	13.510	1704	1706	1709	rBV	1552	1893	0.20%	0.020%
20	13.722	1738	1742	1751	rVB3	6855	11827	1.26%	0.123%
21	14.297	1834	1840	1847	rBV	336469	491165	52.33%	5.093%
22	14.421	1859	1861	1865	rBV2	947	1427	0.15%	0.015%
23	14.532	1874	1880	1885	rBV4	6443	11294	1.20%	0.117%
24	14.603	1885	1892	1899	rVB	372226	602732	64.22%	6.250%
25	14.785	1919	1923	1929	rVB2	5092	6805	0.73%	0.071%
26	14.908	1937	1944	1952	rBV	272441	420522	44.80%	4.361%
27	15.073	1964	1972	1984	rBV2	91541	159571	17.00%	1.655%
28	15.296	2007	2010	2016	rVB3	4203	5356	0.57%	0.056%
29	15.525	2046	2049	2055	rVB	3515	4818	0.51%	0.050%
30	15.689	2073	2077	2081	rBV3	6257	11497	1.22%	0.119%
31	15.736	2081	2085	2088	rVB2	4090	5740	0.61%	0.060%
32	15.895	2105	2112	2122	rVB	487932	739879	78.83%	7.673%
33	15.995	2124	2129	2137	rBV2	33781	50138	5.34%	0.520%
34	16.136	2149	2153	2158	rVB4	2710	4379	0.47%	0.045%
35	16.236	2167	2170	2175	rVB4	2716	3860	0.41%	0.040%
36	16.283	2175	2178	2185	rVB2	3373	4206	0.45%	0.044%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
 Data File : BG051762.D
 Acq On : 22 Dec 2021 22:42
 Operator : CG/JU
 Sample : M5195-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLC1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	16.418	2198	2201	2204	rBV3	2515	3945	0.42%	0.041%
38	16.529	2215	2220	2223	rBV5	3113	4326	0.46%	0.045%
39	16.565	2223	2226	2228	rBV4	4604	4346	0.46%	0.045%
40	16.676	2242	2245	2249	rVB2	4098	4300	0.46%	0.045%
41	16.776	2257	2262	2266	rVB4	4182	6362	0.68%	0.066%
42	16.876	2278	2279	2284	rVB2	3053	2130	0.23%	0.022%
43	16.923	2284	2287	2288	rBV	1609	1292	0.14%	0.013%
44	16.947	2288	2291	2296	rBV4	1712	3411	0.36%	0.035%
45	17.035	2303	2306	2307	rBV3	2617	1980	0.21%	0.021%
46	17.117	2315	2320	2323	rBV4	4116	6491	0.69%	0.067%
47	17.182	2326	2331	2335	rVB5	3341	4585	0.49%	0.048%
48	17.340	2356	2358	2361	rBV4	1960	2165	0.23%	0.022%
49	17.387	2361	2366	2370	rVV5	6740	10064	1.07%	0.104%
50	17.434	2372	2374	2380	rVB4	4022	5891	0.63%	0.061%
51	17.546	2389	2393	2398	rBV3	12342	16199	1.73%	0.168%
52	17.651	2403	2411	2418	rBV	333021	535167	57.02%	5.550%
53	17.751	2421	2428	2435	rVB2	510461	808525	86.14%	8.384%
54	17.857	2445	2446	2449	rBV2	1878	2024	0.22%	0.021%
55	17.886	2449	2451	2453	rBV2	1681	1752	0.19%	0.018%
56	17.916	2453	2456	2460	rVV3	8294	10629	1.13%	0.110%
57	18.121	2488	2491	2492	rBV2	1772	1736	0.18%	0.018%
58	18.151	2494	2496	2499	rVB4	1760	1672	0.18%	0.017%
59	18.186	2499	2502	2504	rBV4	1909	2264	0.24%	0.023%
60	18.304	2518	2522	2527	rVB4	7537	11773	1.25%	0.122%
61	18.362	2529	2532	2536	rBV5	2172	3890	0.41%	0.040%
62	18.445	2544	2546	2549	rVB4	4476	4004	0.43%	0.042%
63	18.480	2549	2552	2557	rBV6	2735	3335	0.36%	0.035%
64	18.533	2557	2561	2562	rVB4	2695	2569	0.27%	0.027%
65	18.597	2565	2572	2576	rBV	18362	24206	2.58%	0.251%
66	18.815	2607	2609	2611	rBV3	2118	2486	0.26%	0.026%
67	19.044	2647	2648	2652	rVB3	3675	3357	0.36%	0.035%
68	19.132	2657	2663	2668	rBV4	10248	17219	1.83%	0.179%
69	19.296	2689	2691	2696	rVB4	6147	7846	0.84%	0.081%
70	19.384	2702	2706	2710	rBV2	9731	13779	1.47%	0.143%
71	19.449	2715	2717	2722	rVB5	4207	4725	0.50%	0.049%
72	19.596	2738	2742	2745	rBV4	7216	11979	1.28%	0.124%
73	19.661	2751	2753	2757	rBV3	5984	7208	0.77%	0.075%
74	19.696	2757	2759	2764	rVB3	9658	9610	1.02%	0.100%
75	19.919	2792	2797	2801	rVB5	6339	10888	1.16%	0.113%
76	20.031	2810	2816	2824	rVB	664876	938594	100.00%	9.733%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
 Data File : BG051762.D
 Acq On : 22 Dec 2021 22:42
 Operator : CG/JU
 Sample : M5195-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLC1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	21.164	3006	3009	3012	rVB4	7059	7455	0.79%	0.077%
78	21.576	3074	3079	3090	rBV3	48144	90013	9.59%	0.933%
79	21.975	3140	3147	3154	rVB	327248	562378	59.92%	5.832%
80	22.568	3246	3248	3249	rBV2	4199	2283	0.24%	0.024%
81	23.802	3454	3458	3465	rVB2	19773	39351	4.19%	0.408%
82	24.472	3568	3572	3580	rVB10	9821	22477	2.39%	0.233%
83	25.229	3690	3701	3717	rBV3	282612	854205	91.01%	8.858%
84	25.476	3732	3743	3757	rBV2	170515	544843	58.05%	5.650%
85	26.275	3875	3879	3880	rBV4	3901	4818	0.51%	0.050%
86	26.310	3884	3885	3886	rBV	3612	1948	0.21%	0.020%




Sum of corrected areas: 9643236

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
Data File : BG051762.D
Acq On : 22 Dec 2021 22:42
Operator : CG/JU
Sample : M5195-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLC1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

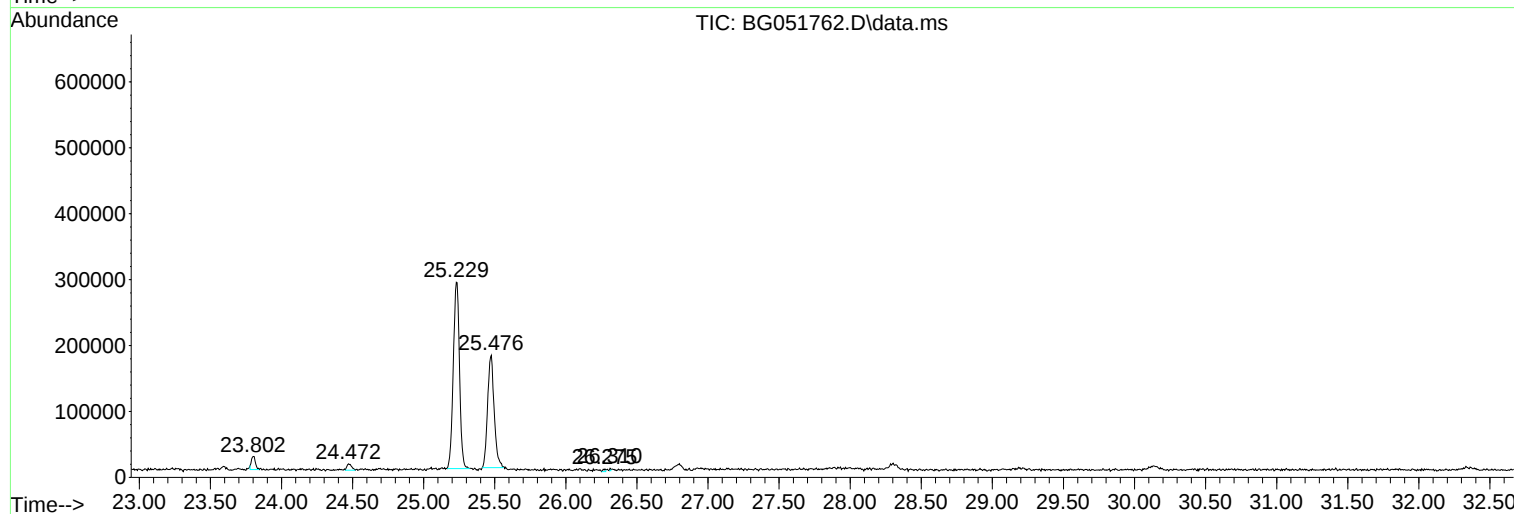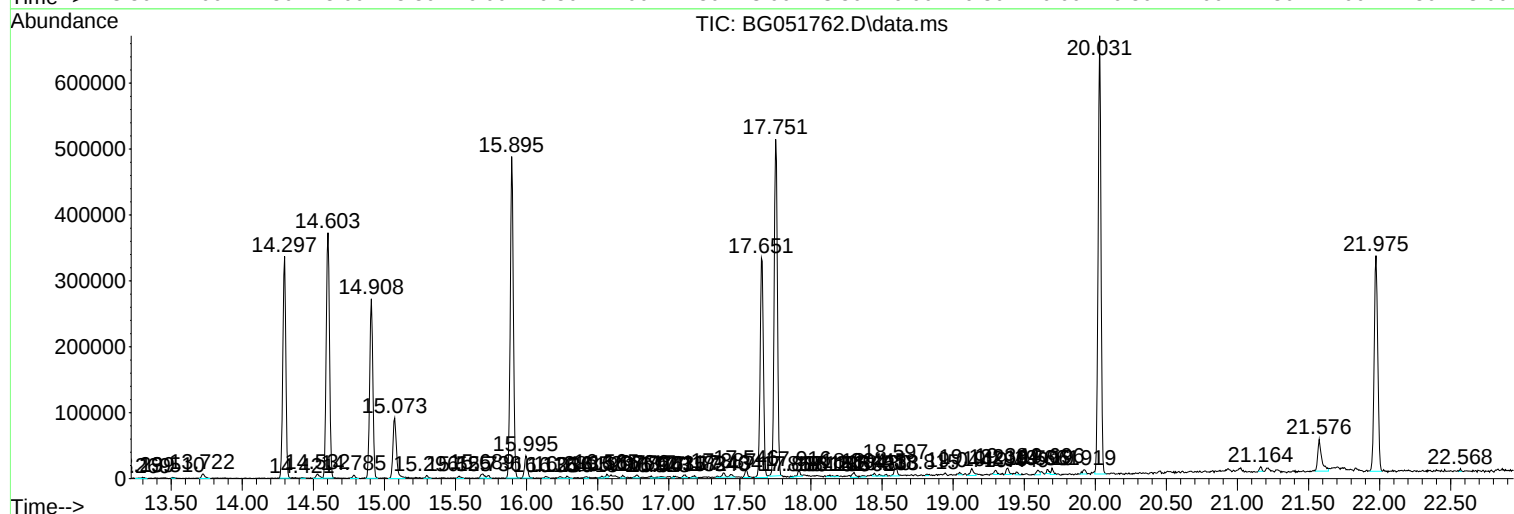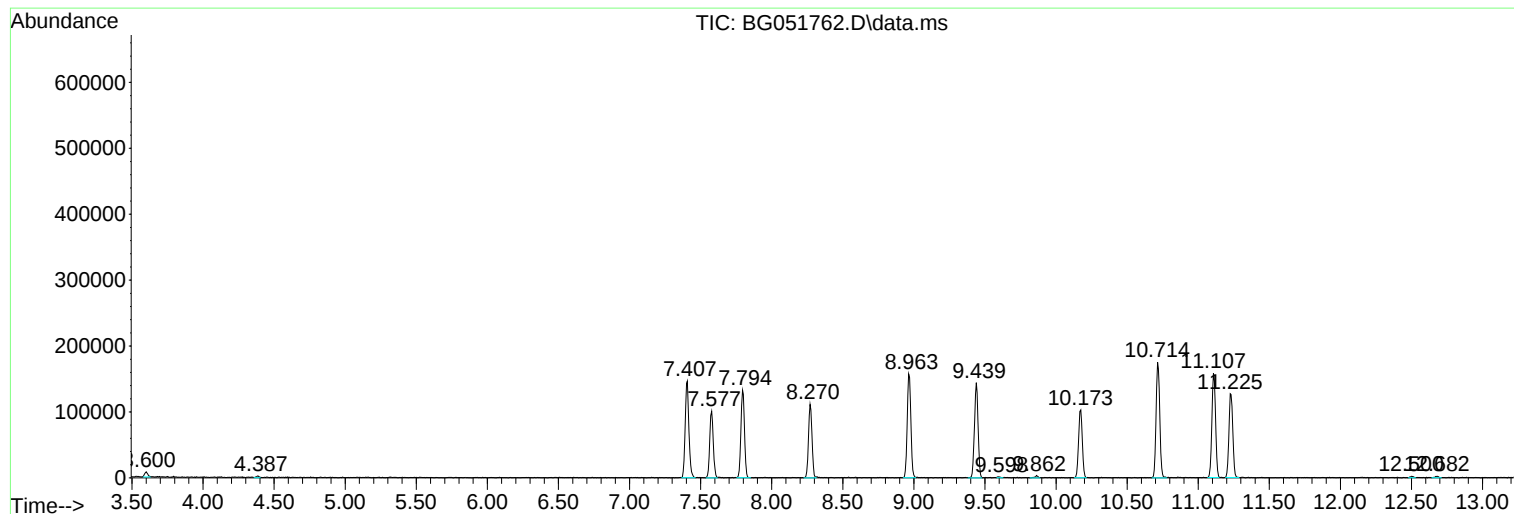

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
Data File : BG051762.D
Acq On : 22 Dec 2021 22:42
Operator : CG/JU
Sample : M5195-09
Misc :
ALS Vial : 13 Sample Multiplier: 1










Instrument :
BNA_G
ClientSampleId :
BGLC1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
21.576	3.20 ng/ul	90013	Chrysene-d12	21.975	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Eicosene, (E)-	280	C20H40	074685-33-9	96
2	9-Eicosene, (E)-	280	C20H40	074685-29-3	94
3	Cycloeicosane	280	C20H40	000296-56-0	93
4	1-Hexacosene	364	C26H52	018835-33-1	93
5	Eicosyl methyl ether	312	C21H44O	1000406-29-4	90

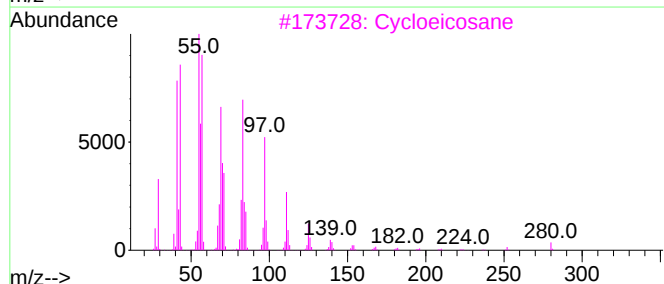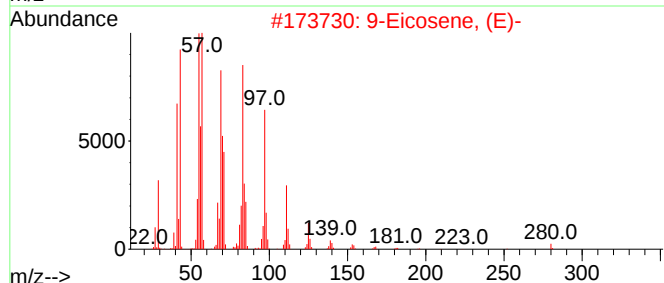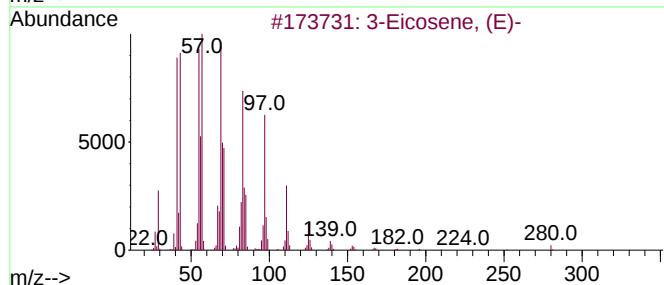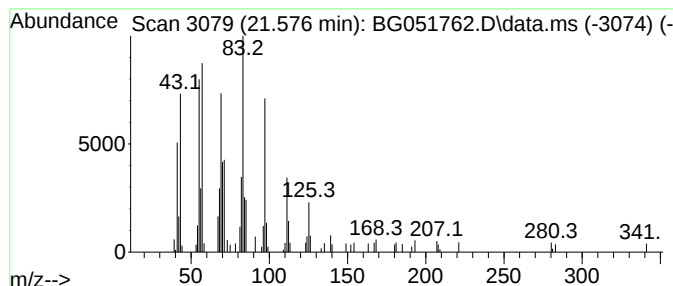

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122221\
Data File : BG051762.D
Acq On : 22 Dec 2021 22:42
Operator : CG/JU
Sample : M5195-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLC1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.576	3.2	ng/u1	90013	5	21.975	562378	20.0