

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122422\
 Data File : BG056120.D
 Acq On : 25 Dec 2022 12:45
 Operator : CG/JU
 Sample : N6017-19
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Dec 25 22:37:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG122422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 24 22:54:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.346	152	42478	20.000	ng/ul	0.00
20) Naphthalene-d8	11.178	136	184092	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.951	164	147975	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.688	188	359133	20.000	ng/ul	0.00
79) Chrysene-d12	21.995	240	342430	20.000	ng/ul	0.00
88) Perylene-d12	25.462	264	373185	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.646	96	5854	5.769	ng/uL	0.00
4) Pyridine-d5	4.081	84	87454	26.432	ng/ul	0.00
7) Phenol-d5	7.477	99	145575	37.781	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.653	67	56230	37.026	ng/ul	0.00
11) 2-Chlorophenol-d4	7.871	132	92748	40.727	ng/ul	0.00
15) 4-Methylphenol-d8	9.034	113	114704	39.555	ng/ul	0.00
21) Nitrobenzene-d5	9.516	128	51191	38.179	ng/ul	0.00
24) 2-Nitrophenol-d4	10.244	143	69883	39.892	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.785	165	143067	36.751	ng/ul	0.00
31) 4-Chloroaniline-d4	11.302	131	116013	26.348	ng/ul	0.00
46) Dimethylphthalate-d6	14.345	166	445338	38.885	ng/ul	0.00
49) Acenaphthylene-d8	14.651	160	508682	39.330	ng/ul	0.00
54) 4-Nitrophenol-d4	15.115	143	64441	37.380	ng/ul	0.00
60) Fluorene-d10	15.938	176	415995	36.799	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.037	200	90034	38.999	ng/ul	0.00
73) Anthracene-d10	17.788	188	656063	39.532	ng/ul	0.00
81) Pyrene-d10	20.056	212	781552	41.327	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.221	264	761356	40.139	ng/ul	0.00
Target Compounds						
17) N-Nitroso-di-n-propyla...	9.034	70	2751	1.355	ng/ul#	1
83) Butylbenzylphthalate	20.973	149	101695	21.302	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122422\
Data File : BG056120.D
Acq On : 25 Dec 2022 12:45
Operator : CG/JU
Sample : N6017-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Dec 25 22:37:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG122422.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 24 22:54:38 2022
Response via : Initial Calibration

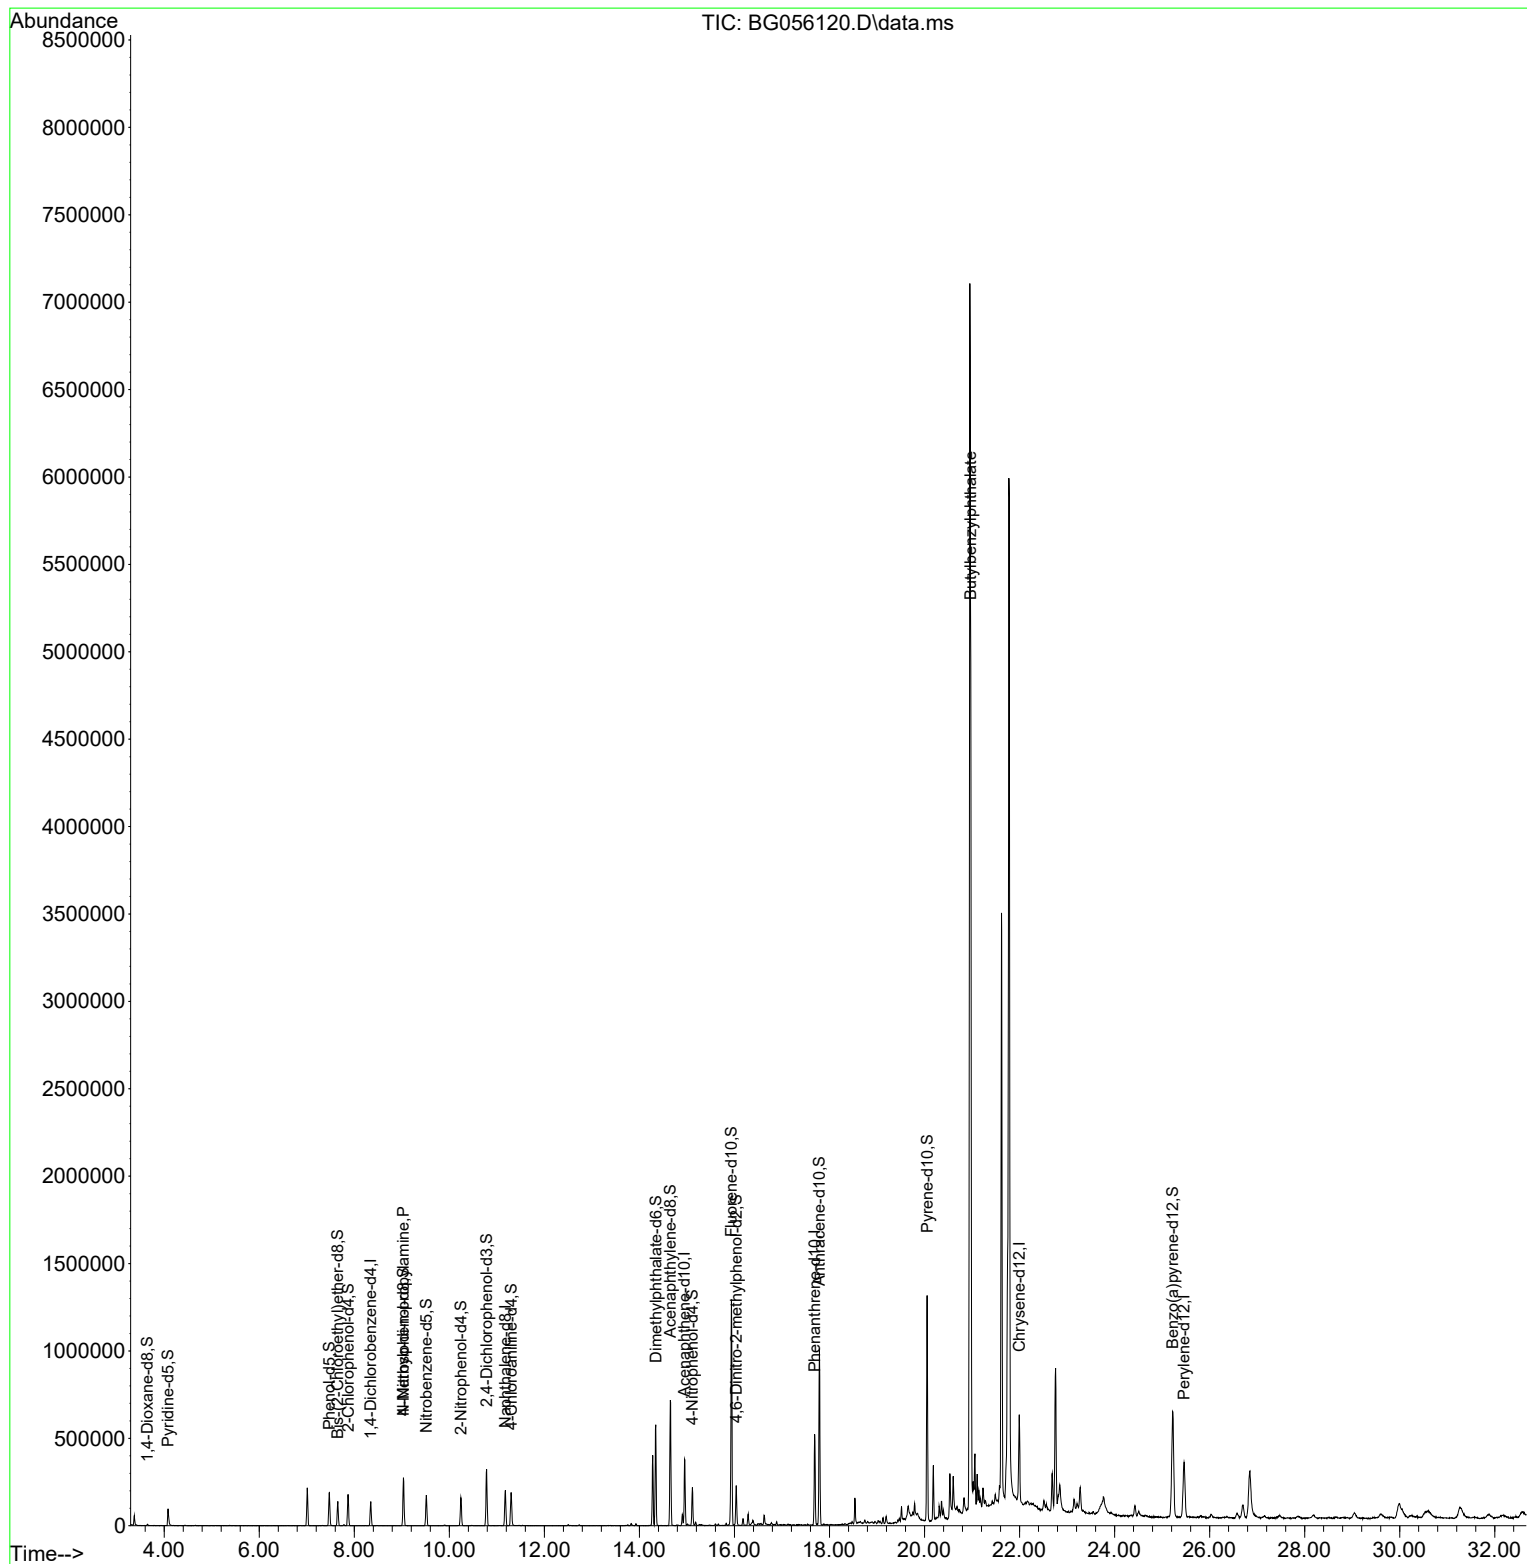




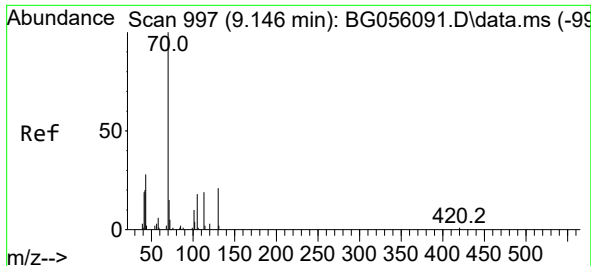


#17
N-Nitroso-di-n-propylamine
Concen: 1.355 ng/ul
RT: 9.034 min Scan# 91
Delta R.T. -0.112 min
Lab File: BG056120.D
Acq: 25 Dec 2022 12:45

Instrument :
BNA_G
ClientSampleId :

Tgt Ion: 70 Resp: 2751

Ion	Ratio	Lower	Upper
70	100		
42	143.6	16.1	24.1#
101	0.0	8.4	12.6#
130	0.0	16.8	25.2#

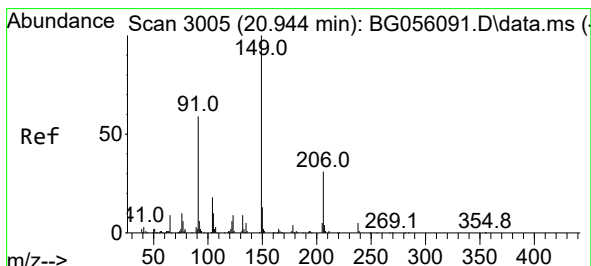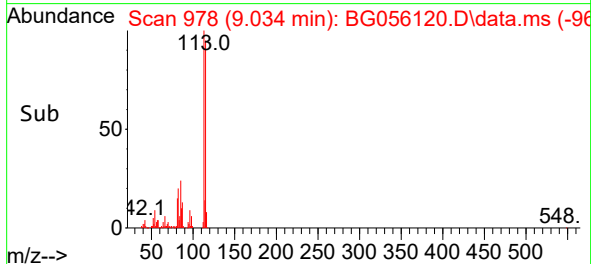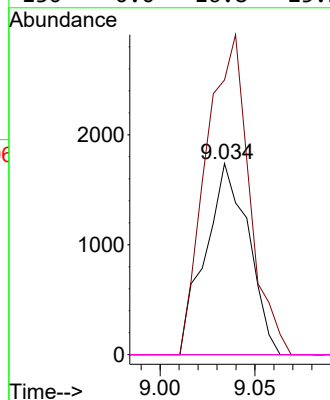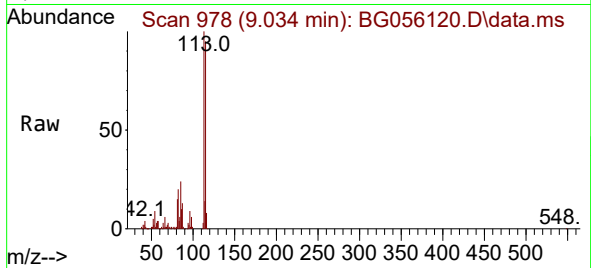

#83
Butylbenzylphthalate
Concen: 21.302 ng/ul
RT: 20.973 min Scan# 3010
Delta R.T. 0.029 min
Lab File: BG056120.D
Acq: 25 Dec 2022 12:45

Tgt Ion: 149 Resp: 101695

Ion	Ratio	Lower	Upper
149	100		
91	43.9	46.9	70.3#
206	0.8	24.6	36.8#

