

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122422\
 Data File : BG056123.D
 Acq On : 25 Dec 2022 16:12
 Operator : CG/JU
 Sample : N6017-21
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Dec 25 22:38:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG122422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 24 22:54:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.342	152	39213	20.000	ng/ul	0.00
20) Naphthalene-d8	11.180	136	161979	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.952	164	135179	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.690	188	327205	20.000	ng/ul	0.00
79) Chrysene-d12	21.991	240	323222	20.000	ng/ul	0.00
88) Perylene-d12	25.464	264	333034	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.648	96	3445	3.677	ng/uL	0.00
4) Pyridine-d5	4.094	84	211	0.069	ng/ul	0.00
7) Phenol-d5	7.473	99	74129	20.840	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.649	67	56143	40.047	ng/ul	0.00
11) 2-Chlorophenol-d4	7.867	132	51317	24.410	ng/ul	0.00
15) 4-Methylphenol-d8	9.036	113	65983	24.648	ng/ul	0.00
21) Nitrobenzene-d5	9.518	128	49472	41.934	ng/ul	0.00
24) 2-Nitrophenol-d4	10.246	143	66841	43.364	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.781	165	75491	22.040	ng/ul	0.00
31) 4-Chloroaniline-d4	11.298	131	58630	15.133	ng/ul	0.00
46) Dimethylphthalate-d6	14.341	166	434511	41.531	ng/ul	0.00
49) Acenaphthylene-d8	14.653	160	267801	22.666	ng/ul	0.00
54) 4-Nitrophenol-d4	15.117	143	35789	22.725	ng/ul	0.00
60) Fluorene-d10	15.939	176	320180	31.004	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.039	200	82240	39.099	ng/ul	0.00
73) Anthracene-d10	17.790	188	319482	21.129	ng/ul	0.00
81) Pyrene-d10	20.052	212	364540	20.422	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.217	264	380530	22.480	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	9.177	105	8721	1.967	ng/ul	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122422\
Data File : BG056123.D
Acq On : 25 Dec 2022 16:12
Operator : CG/JU
Sample : N6017-21
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :


Quant Time: Dec 25 22:38:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG122422.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 24 22:54:38 2022
Response via : Initial Calibration

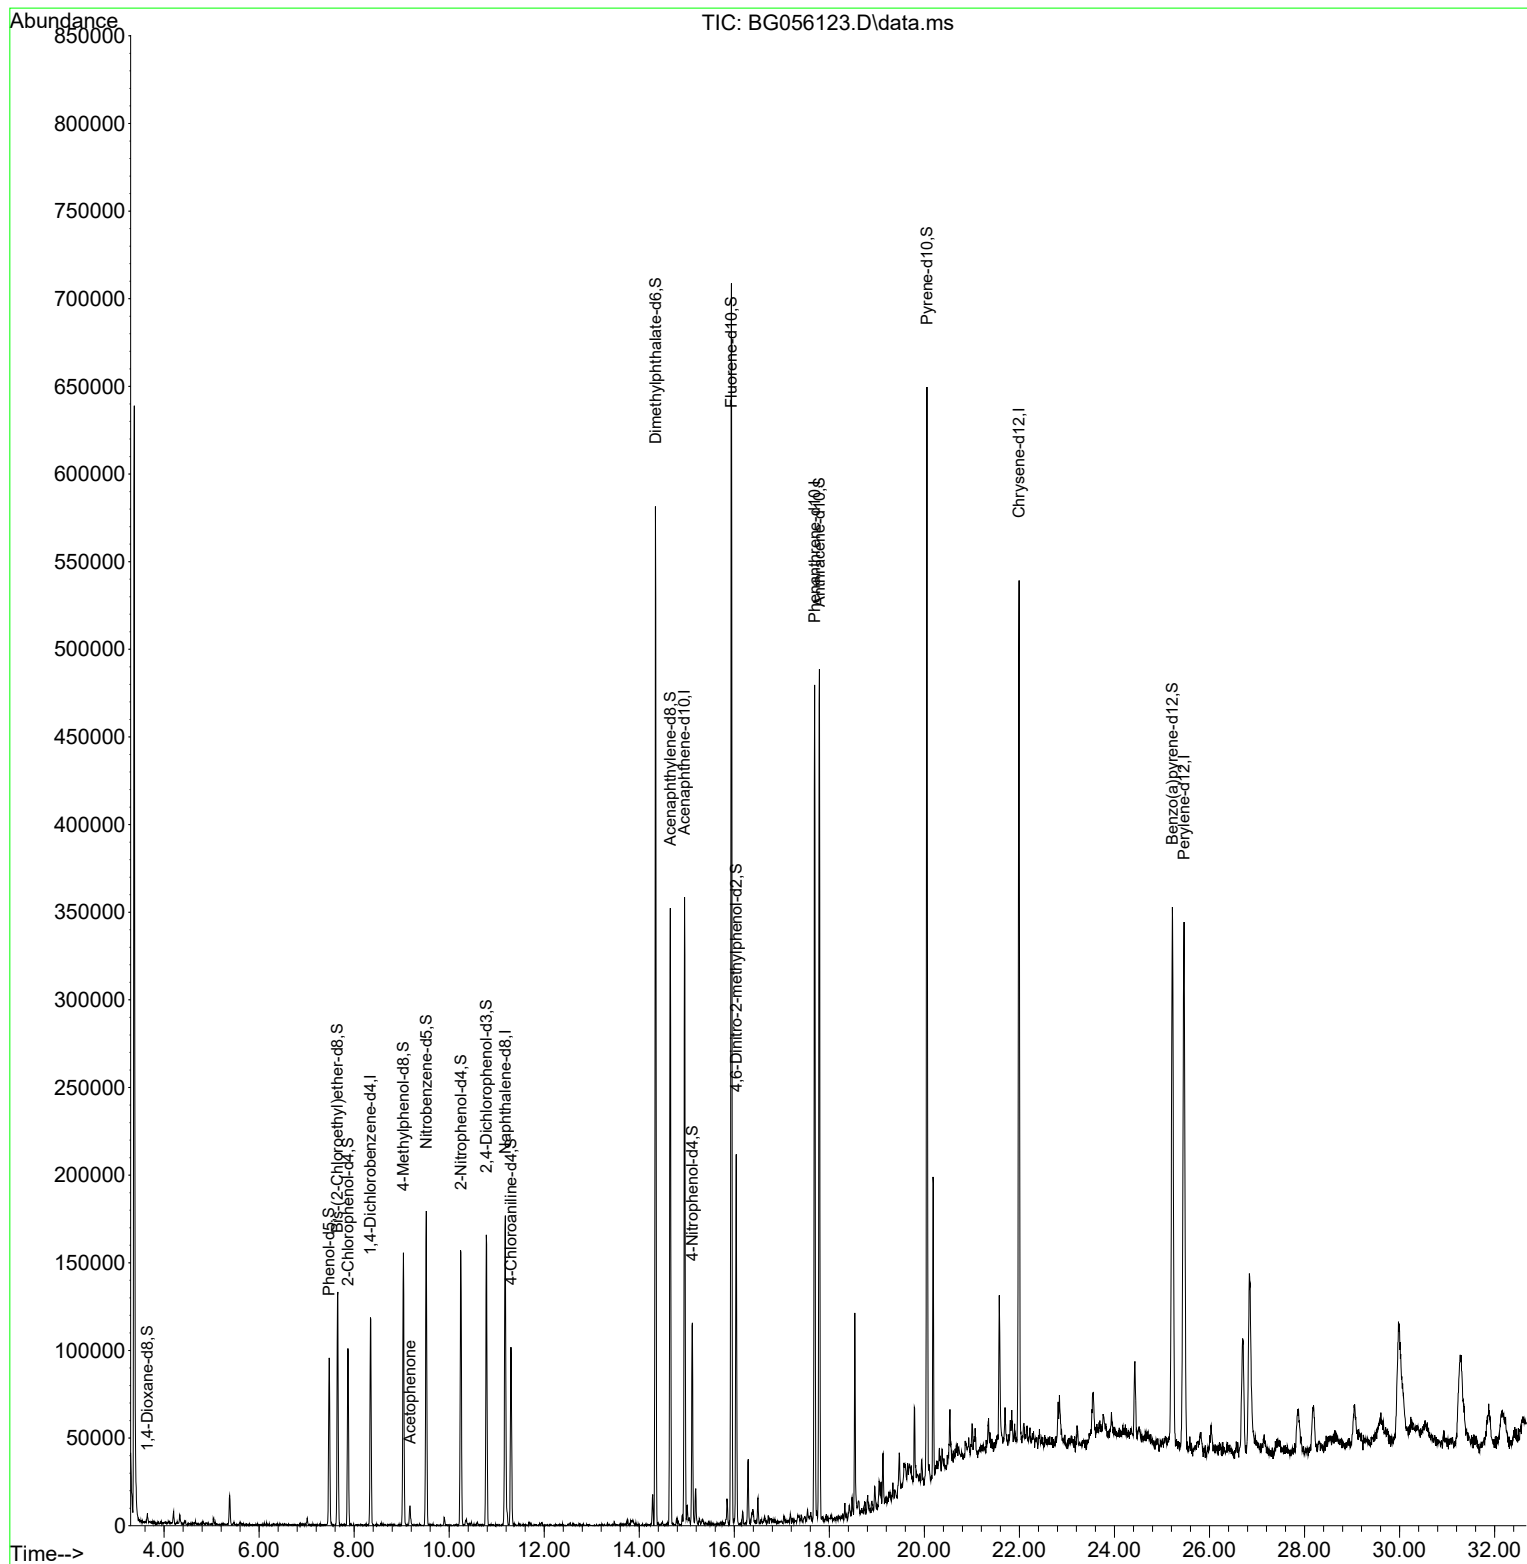

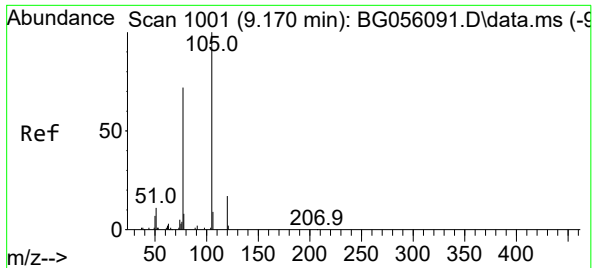

#16
 Acetophenone
 Concen: 1.967 ng/ul
 RT: 9.177 min Scan# 10
 Delta R.T. 0.007 min
 Lab File: BG056123.D
 Acq: 25 Dec 2022 16:12

Instrument :
 BNA_G
 ClientSampleId :

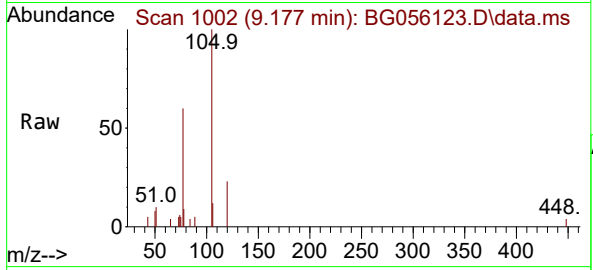

Tgt Ion:	105	Resp:	8721
Ion	Ratio	Lower	Upper
105	100		
77	59.8	59.0	88.4
51	9.7	9.6	14.4

