




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122422\
 Data File : BG056120.D
 Acq On : 25 Dec 2022 12:45
 Operator : CG/JU
 Sample : N0017-19
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBYG5

Manual IntegrationsAPPROVED

Quant Time: Dec 25 22:37:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG122422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 24 22:54:38 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/26/2022
 Supervised By :Sohil Jodhani 12/26/2022

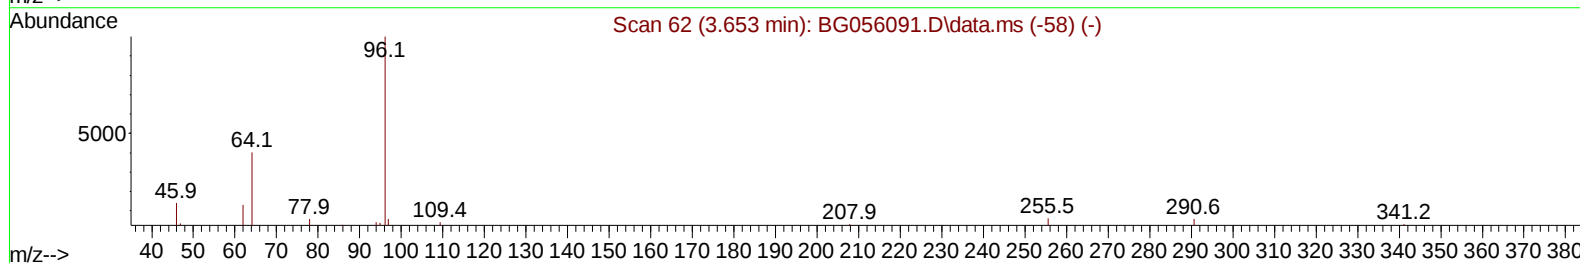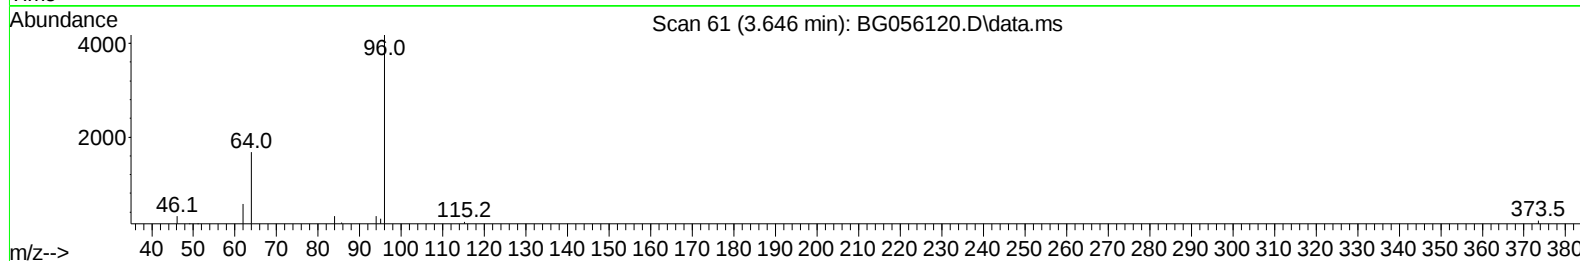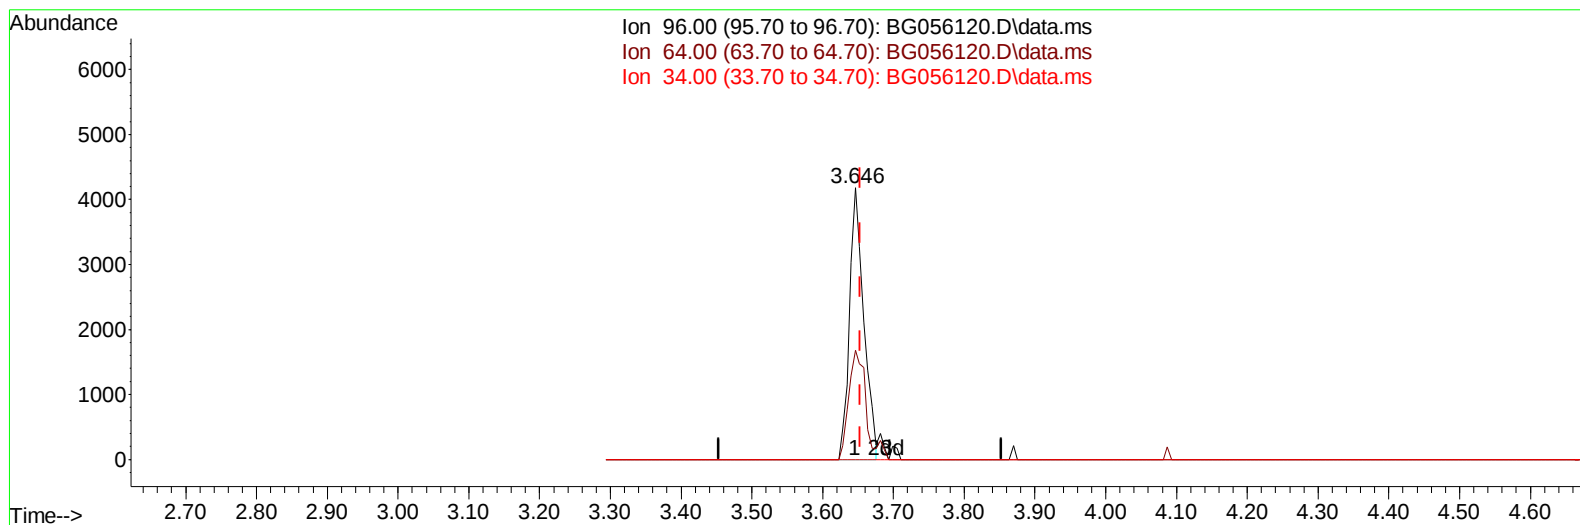

TIC: BG056120.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.646min (-0.007) 5.77 ng/uL

response 5854

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.20	40.16
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122422\
 Data File : BG056120.D
 Acq On : 25 Dec 2022 12:45
 Operator : CG/JU
 Sample : N6017-19
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBYG5

Manual IntegrationsAPPROVED

Quant Time: Dec 25 22:37:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG122422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 24 22:54:38 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/26/2022
 Supervised By :Sohil Jodhani 12/26/2022

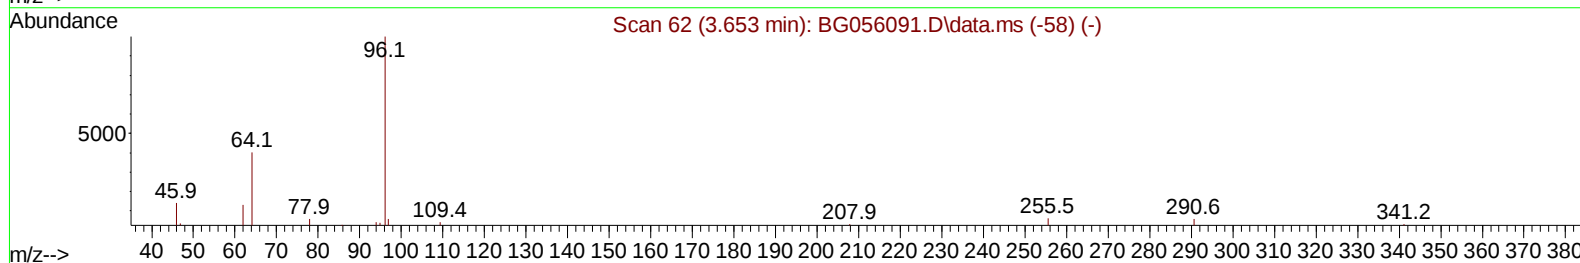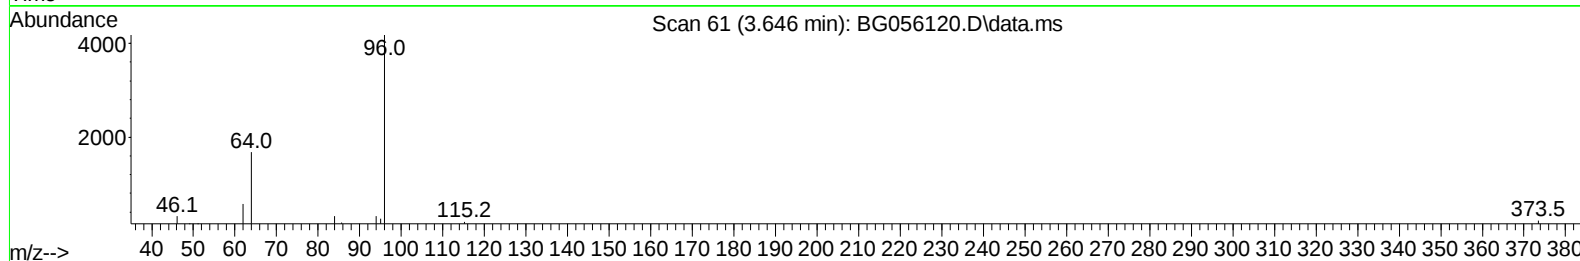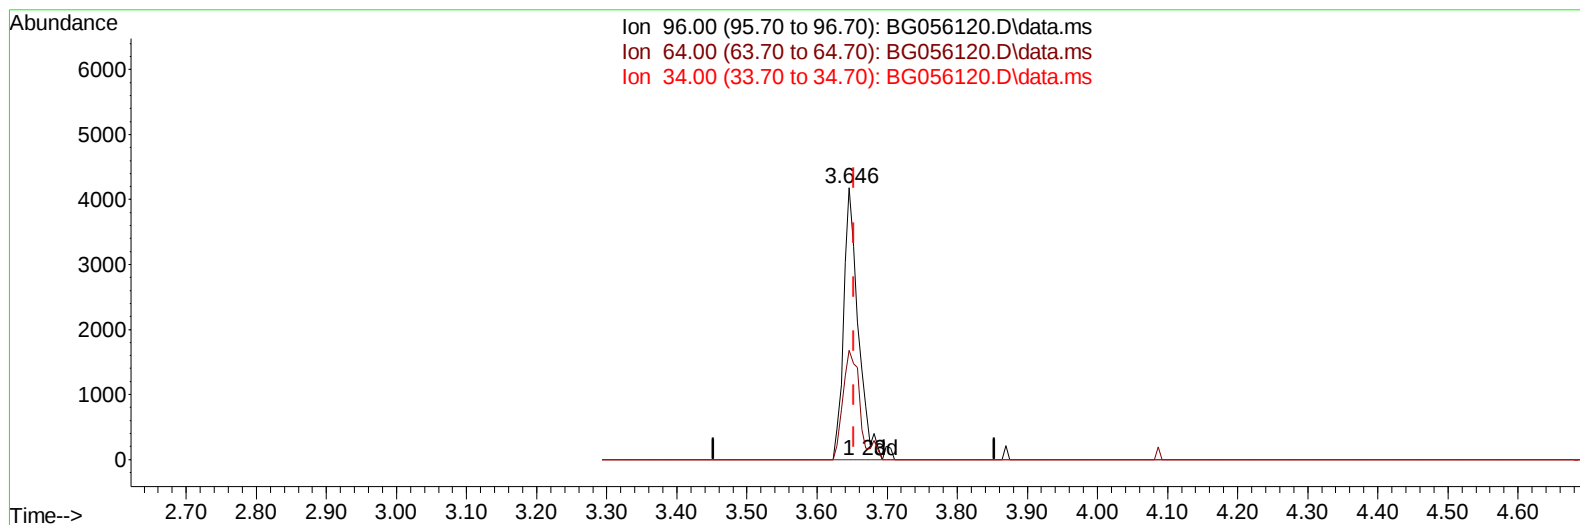

TIC: BG056120.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.646min (-0.007) 5.97 ng/uL m

response 6063

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.20	40.16
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122422\
 Data File : BG056120.D
 Acq On : 25 Dec 2022 12:45
 Operator : CG/JU
 Sample : N6017-19
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBYG5

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/26/2022
 Supervised By :Sohil Jodhani 12/26/2022

Quant Time: Dec 25 22:37:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG122422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 24 22:54:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.346	152	42478	20.000	ng/ul	0.00
20) Naphthalene-d8	11.178	136	184092	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.951	164	147975	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.688	188	359133	20.000	ng/ul	0.00
79) Chrysene-d12	21.995	240	342430	20.000	ng/ul	0.00
88) Perylene-d12	25.462	264	373185	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.646	96	6063m	5.975	ng/uL	0.00
4) Pyridine-d5	4.081	84	87454	26.432	ng/ul	0.00
7) Phenol-d5	7.477	99	145575	37.781	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.653	67	56230	37.026	ng/ul	0.00
11) 2-Chlorophenol-d4	7.871	132	92748	40.727	ng/ul	0.00
15) 4-Methylphenol-d8	9.034	113	114704	39.555	ng/ul	0.00
21) Nitrobenzene-d5	9.516	128	51191	38.179	ng/ul	0.00
24) 2-Nitrophenol-d4	10.244	143	69883	39.892	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.785	165	143067	36.751	ng/ul	0.00
31) 4-Chloroaniline-d4	11.302	131	116013	26.348	ng/ul	0.00
46) Dimethylphthalate-d6	14.345	166	445338	38.885	ng/ul	0.00
49) Acenaphthylene-d8	14.651	160	508682	39.330	ng/ul	0.00
54) 4-Nitrophenol-d4	15.115	143	64441	37.380	ng/ul	0.00
60) Fluorene-d10	15.938	176	415995	36.799	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.037	200	90034	38.999	ng/ul	0.00
73) Anthracene-d10	17.788	188	656063	39.532	ng/ul	0.00
81) Pyrene-d10	20.056	212	781552	41.327	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.221	264	761356	40.139	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122422\
Data File : BG056120.D
Acq On : 25 Dec 2022 12:45
Operator : CG/JU
Sample : N6017-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBYG5

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/26/2022
Supervised By :Sohil Jodhani 12/26/2022

Quant Time: Dec 25 22:37:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG122422.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 24 22:54:38 2022
Response via : Initial Calibration

