

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122422\
 Data File : BG056114.D
 Acq On : 25 Dec 2022 8:40
 Operator : CG/JU
 Sample : PB149812BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK812

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG122422.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	9	14	18	rBV2	9762	14061	0.94%	0.102%
2	3.646	58	61	67	rVV2	6091	9285	0.62%	0.067%
3	4.081	131	135	148	rBV2	87254	148750	9.95%	1.077%
4	4.440	193	196	200	rVB3	2292	3024	0.20%	0.022%
5	7.471	705	712	720	rBV	134307	230077	15.38%	1.665%
6	7.653	736	743	749	rBV	105226	170924	11.43%	1.237%
7	7.871	772	780	786	rBV	130644	225304	15.06%	1.631%
8	8.347	854	861	868	rVB	125053	213065	14.25%	1.542%
9	9.034	970	978	988	rBV	194199	333293	22.28%	2.412%
10	9.516	1050	1060	1067	rBV	127003	223140	14.92%	1.615%
11	10.244	1176	1184	1193	rBV	110621	199114	13.31%	1.441%
12	10.785	1268	1276	1284	rBB	215094	384438	25.70%	2.782%
13	11.179	1335	1343	1351	rBB	180085	326111	21.80%	2.360%
14	11.302	1356	1364	1372	rBV	184608	337460	22.56%	2.442%
15	12.736	1602	1608	1614	rBB2	4279	7068	0.47%	0.051%
16	14.340	1875	1881	1889	rVB	443432	642845	42.98%	4.652%
17	14.651	1927	1934	1941	rBV2	504550	799105	53.43%	5.783%
18	14.957	1978	1986	1993	rVB	382629	616936	41.25%	4.465%
19	15.115	2005	2013	2019	rBV	161338	257874	17.24%	1.866%
20	15.344	2048	2052	2058	rBV	1191	1600	0.11%	0.012%
21	15.938	2145	2153	2160	rBB	729232	1090273	72.90%	7.890%
22	16.038	2164	2170	2177	rBV	174392	254892	17.04%	1.845%
23	16.173	2189	2193	2197	rBV	2427	4286	0.29%	0.031%
24	17.689	2444	2451	2460	rBV	572711	830950	55.56%	6.014%
25	17.789	2461	2468	2475	rVV	784227	1212173	81.05%	8.773%
26	17.947	2491	2495	2497	rBV2	1420	1725	0.12%	0.012%
27	18.059	2512	2514	2517	rVB	1654	1714	0.11%	0.012%
28	18.329	2551	2560	2562	rBV2	1564	3053	0.20%	0.022%
29	18.635	2609	2612	2615	rVB3	1178	1500	0.10%	0.011%
30	18.670	2615	2618	2621	rBV2	1667	1743	0.12%	0.013%
31	18.993	2670	2673	2675	rBV3	1775	2101	0.14%	0.015%
32	19.158	2699	2701	2705	rVB3	1700	1643	0.11%	0.012%
33	19.622	2776	2780	2784	rVB2	12398	17696	1.18%	0.128%
34	19.686	2787	2791	2796	rBV2	11036	19398	1.30%	0.140%
35	19.745	2799	2801	2803	rBV3	2203	1803	0.12%	0.013%
36	19.892	2824	2826	2829	rVV3	1893	1852	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122422\
 Data File : BG056114.D
 Acq On : 25 Dec 2022 8:40
 Operator : CG/JU
 Sample : PB149812BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK812

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG122422.M
 Title : SVOA CALIBRATION

37	19.933	2831	2833	2838	rBV4	5214	7860	0.53%	0.057%
38	20.010	2844	2846	2847	rBV2	2099	1693	0.11%	0.012%
39	20.051	2847	2853	2861	rVV	1026971	1495602	100.00%	10.824%
40	20.133	2866	2867	2869	rBV2	2612	1830	0.12%	0.013%
41	20.162	2871	2872	2874	rBV2	2485	2046	0.14%	0.015%
42	20.256	2886	2888	2891	rBV3	2751	3494	0.23%	0.025%
43	20.403	2911	2913	2914	rBV2	3244	2334	0.16%	0.017%
44	20.709	2960	2965	2967	rBV5	3526	6105	0.41%	0.044%
45	20.762	2973	2974	2977	rVB3	3458	2431	0.16%	0.018%
46	20.826	2983	2985	2986	rBV2	4198	2470	0.17%	0.018%
47	20.867	2990	2992	2993	rVV2	3057	2360	0.16%	0.017%
48	20.903	2996	2998	3001	rBV4	3400	3977	0.27%	0.029%
49	20.973	3009	3010	3014	rBV4	5833	7921	0.53%	0.057%
50	21.085	3028	3029	3031	rBV2	3478	2736	0.18%	0.020%
51	21.990	3175	3183	3191	rBV	551366	967176	64.67%	7.000%
52	22.471	3263	3265	3267	rBV2	3784	2914	0.19%	0.021%
53	22.841	3326	3328	3331	rBV4	4526	4657	0.31%	0.034%
54	22.971	3348	3350	3351	rBV2	4449	2569	0.17%	0.019%
55	23.041	3360	3362	3363	rBV2	3832	2443	0.16%	0.018%
56	23.294	3404	3405	3406	rVB	4894	1725	0.12%	0.012%
57	23.353	3413	3415	3417	rVB3	5317	2804	0.19%	0.020%
58	23.605	3456	3458	3459	rVB2	5834	3464	0.23%	0.025%
59	23.864	3501	3502	3504	rBV2	4992	3740	0.25%	0.027%
60	24.257	3567	3569	3570	rVB2	4636	2552	0.17%	0.018%
61	24.422	3595	3597	3604	rVB7	12271	23395	1.56%	0.169%
62	25.057	3703	3705	3706	rVB2	4422	2002	0.13%	0.014%
63	25.221	3721	3733	3746	rVB2	492262	1480697	99.00%	10.716%
64	25.456	3762	3773	3787	rVB2	330009	1003740	67.11%	7.264%
65	25.550	3787	3789	3791	rVB3	6607	4168	0.28%	0.030%
66	25.568	3791	3792	3793	rBV	5344	3153	0.21%	0.023%
67	26.108	3882	3884	3885	rBV2	4464	3506	0.23%	0.025%
68	26.696	3976	3984	3995	rVB9	18273	64458	4.31%	0.466%
69	26.772	3995	3997	3999	rVB3	3728	2103	0.14%	0.015%
70	27.759	4163	4165	4166	rBV2	4099	2496	0.17%	0.018%
71	27.859	4180	4182	4183	rVB2	4963	2634	0.18%	0.019%
72	27.947	4195	4197	4200	rBV5	4594	5631	0.38%	0.041%
73	28.194	4229	4239	4245	rBV5	14224	41092	2.75%	0.297%
74	28.617	4309	4311	4313	rVB3	4792	2921	0.20%	0.021%
75	29.963	4536	4540	4541	rBV3	5957	9402	0.63%	0.068%
76	30.327	4600	4602	4607	rBV4	4244	6719	0.45%	0.049%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122422\
 Data File : BG056114.D
 Acq On : 25 Dec 2022 8:40
 Operator : CG/JU
 Sample : PB149812BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK812

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG122422.M
 Title : SVOA CALIBRATION

77	30.438	4619	4621	4625	rBV5	4482	4646	0.31%	0.034%
78	30.703	4664	4666	4670	rBV5	4458	5627	0.38%	0.041%
79	31.079	4728	4730	4731	rVB2	4499	2503	0.17%	0.018%
80	31.126	4736	4738	4739	rBV2	3654	1886	0.13%	0.014%
81	31.596	4816	4818	4819	rBV2	4120	1971	0.13%	0.014%
82	31.854	4860	4862	4863	rBV2	3862	2918	0.20%	0.021%
83	31.872	4863	4865	4866	rBV2	4627	2629	0.18%	0.019%
84	32.131	4907	4909	4912	rBV4	5941	7707	0.52%	0.056%
85	32.324	4940	4942	4944	rBV3	4801	2566	0.17%	0.019%




Sum of corrected areas: 13817749

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122422\
Data File : BG056114.D
Acq On : 25 Dec 2022 8:40
Operator : CG/JU
Sample : PB149812BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK812

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG122422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

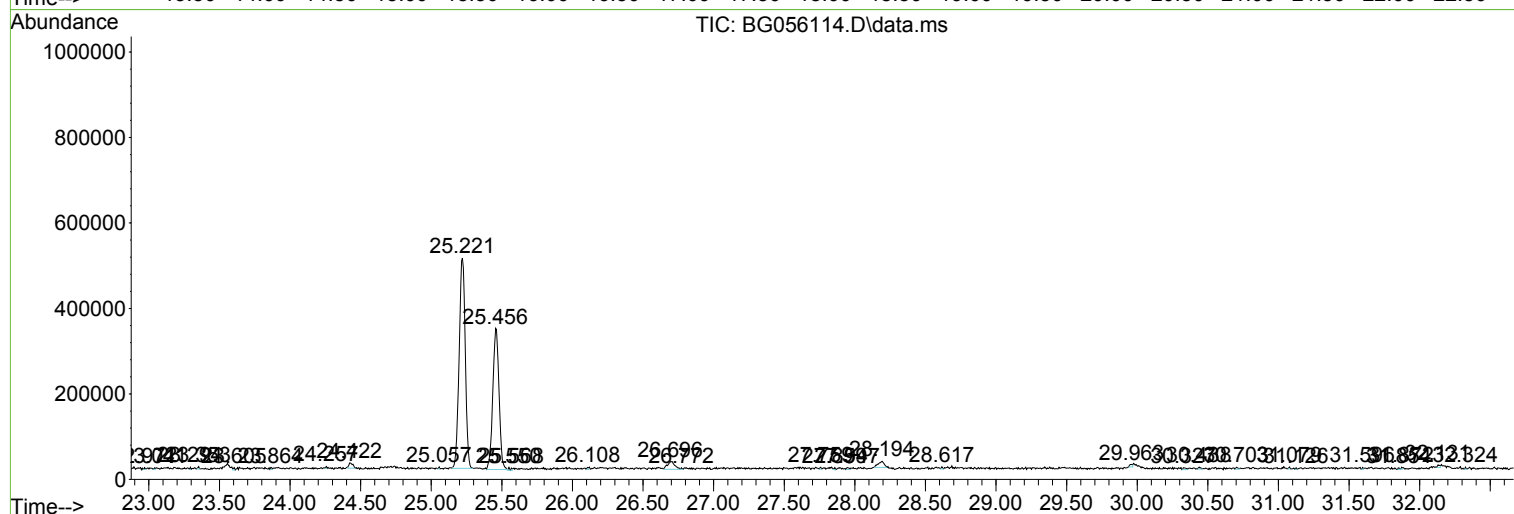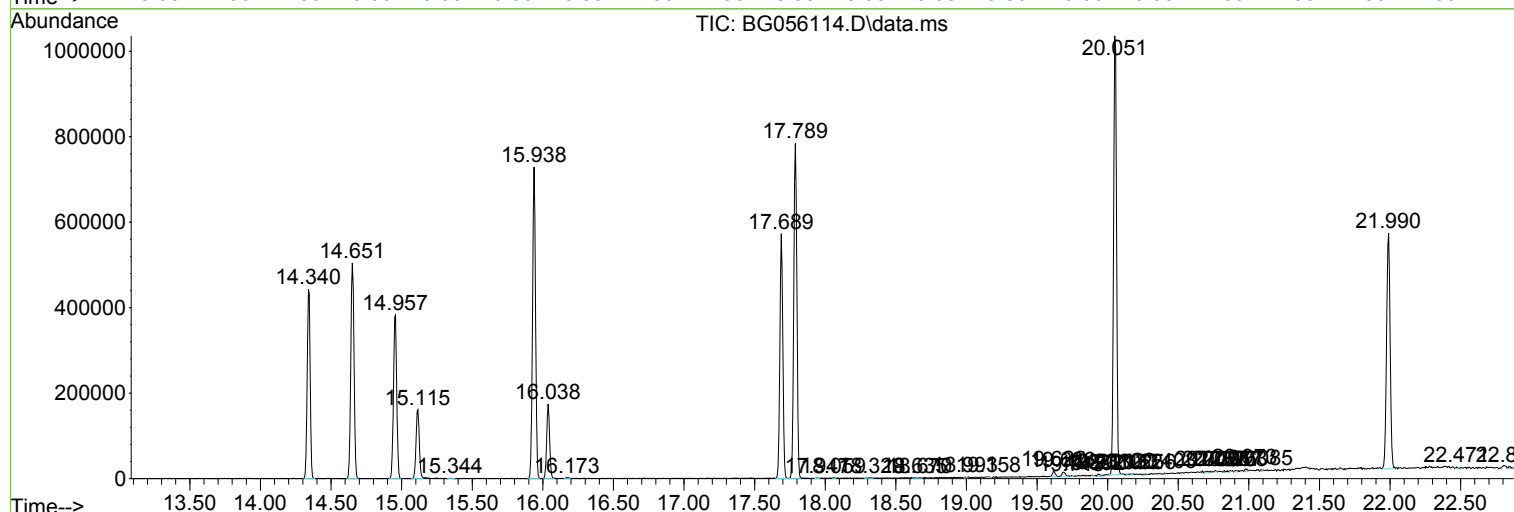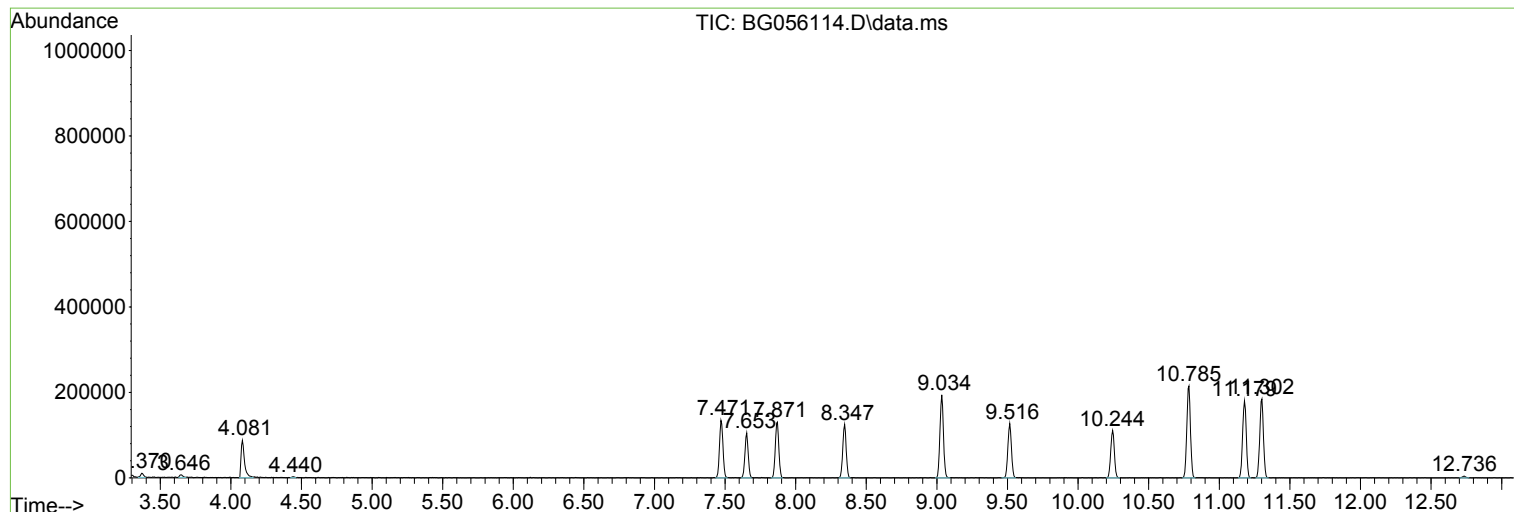

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122422\
Data File : BG056114.D
Acq On : 25 Dec 2022 8:40
Operator : CG/JU
Sample : PB149812BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK812

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG122422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122422\
Data File : BG056114.D
Acq On : 25 Dec 2022 8:40
Operator : CG/JU
Sample : PB149812BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK812

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG122422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc