
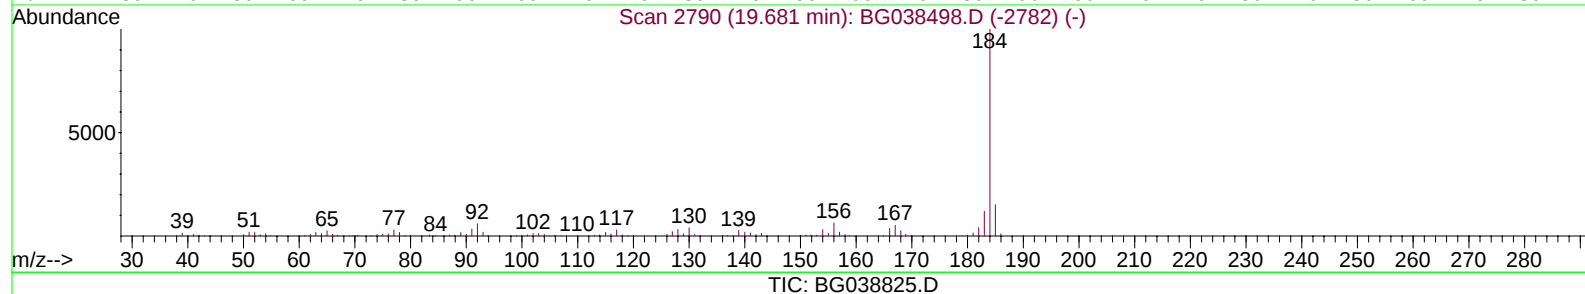
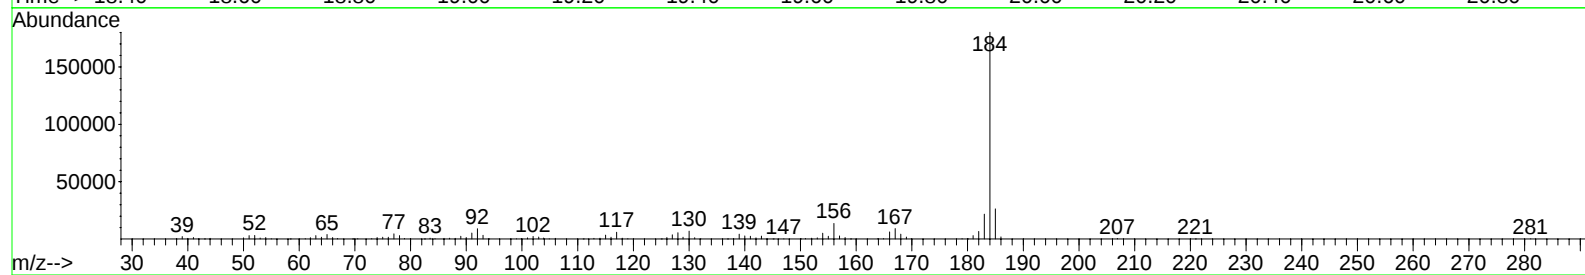


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG122618\
 Data File : BG038825.D
 Acq On : 26 Dec 2018 11:42
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 17:56:23 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 12 15:26:27 2018
 Response via : Initial Calibration

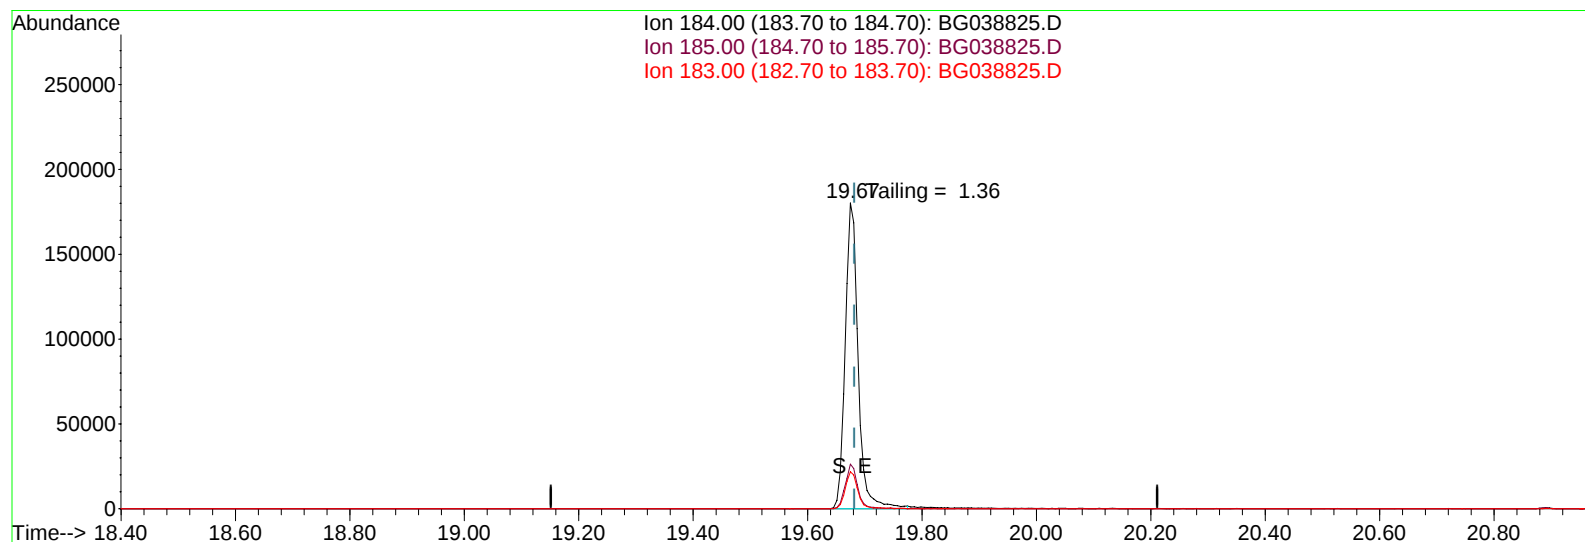

(77) Benzidine




19.675min (-0.007) 0.00ng

response 284178

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.60
183.00	12.00	12.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG122618\
Data File : BG038825.D
Acq On : 26 Dec 2018 11:42
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 17:56:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

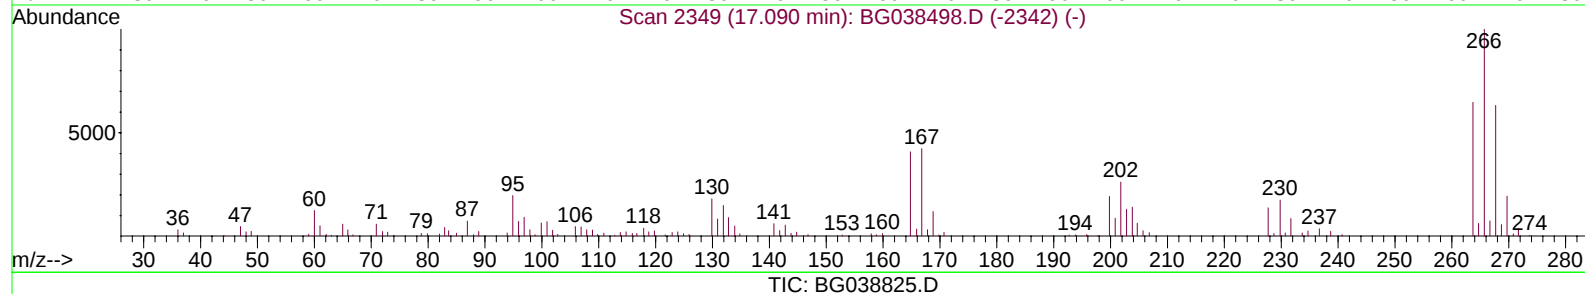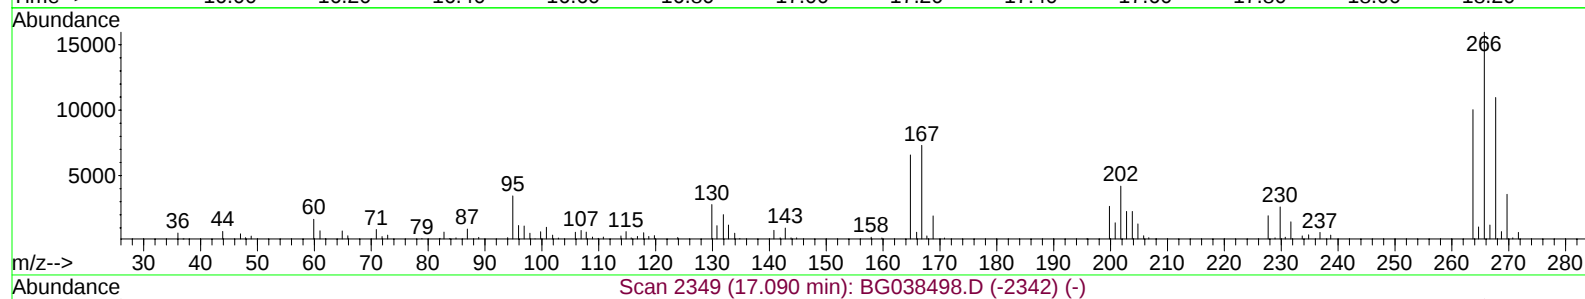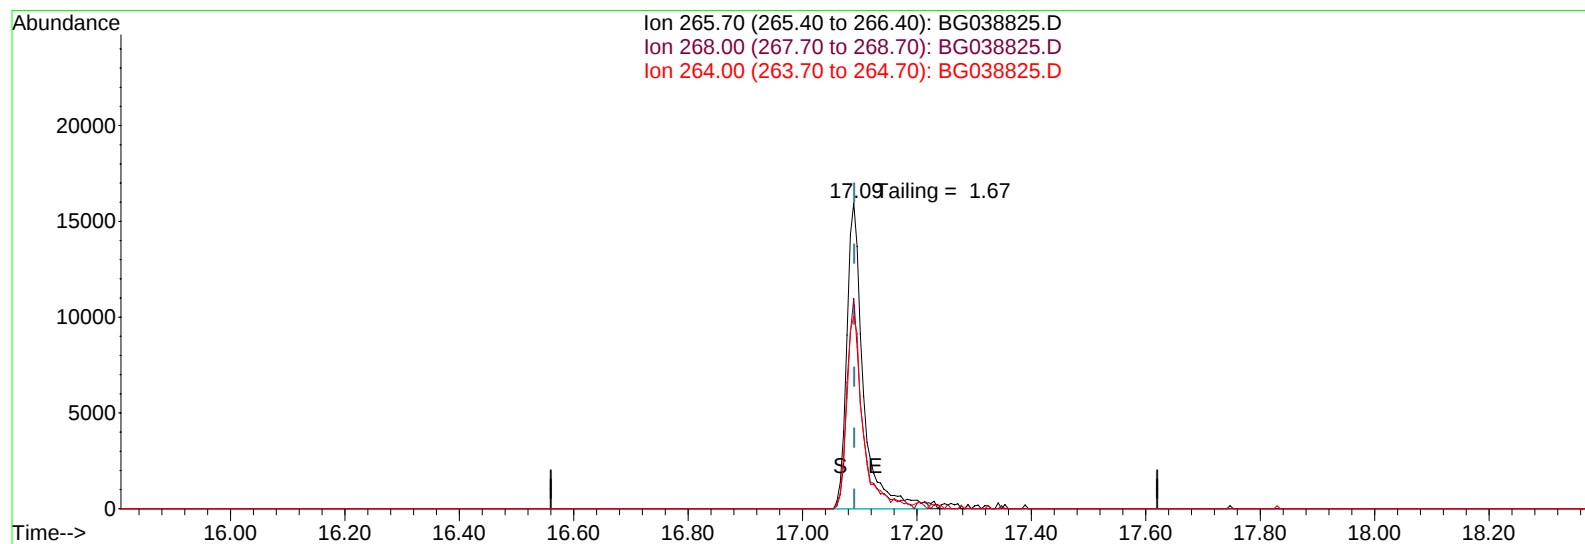

(70) Pentachlorophenol (C)

17.089min (-0.001) 28405.60ng

response 32757

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	73.26
264.00	70.90	69.59
0.00	0.00	0.00