


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG122618\
 Data File : BG038825.D
 Acq On : 26 Dec 2018 11:42
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

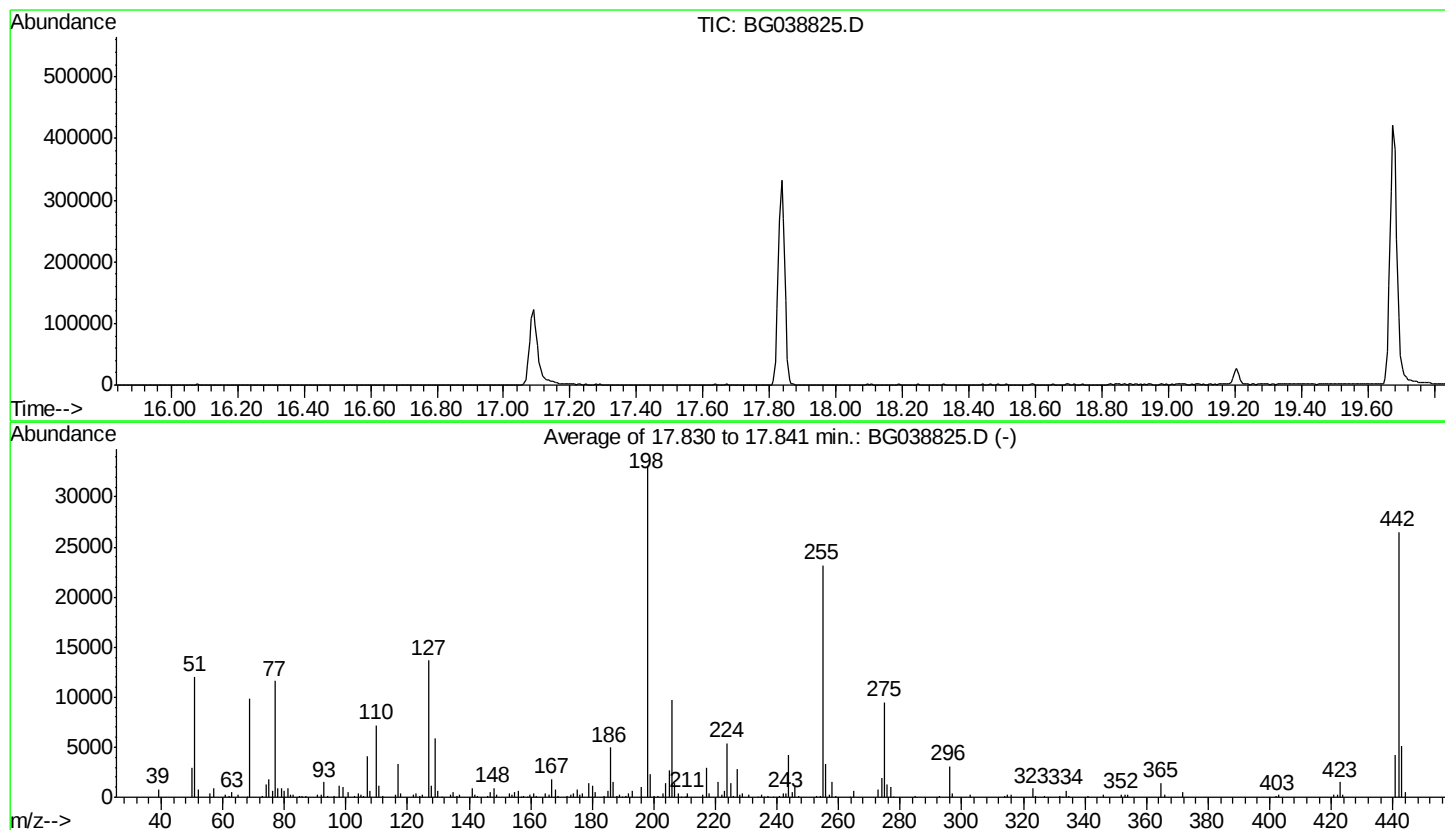

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	12087	PASS
68	69	0.00	2	0.7	64	PASS
69	198	0.00	100	29.5	9786	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.2	13660	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	33122	PASS
199	198	5	9	7.0	2316	PASS
275	198	10	60	28.8	9524	PASS
365	198	1	100	4.3	1428	PASS
441	198	0.01	100	12.9	4272	PASS
442	198	50	100	80.0	26490	PASS
443	442	15	24	19.4	5148	PASS