

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
 Data File : BG051800.D
 Acq On : 27 Dec 2021 13:18
 Operator : CG/JU
 Sample : M5201-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P035-TW001-A-01

Quant Time: Dec 27 14:49:56 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 23 13:37:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.272	152	32197	20.000	ng/u1	-0.02
20) Naphthalene-d8	11.109	136	133250	20.000	ng/u1	-0.02
38) Acenaphthene-d10	14.904	164	93609	20.000	ng/u1	-0.02
64) Phenanthrene-d10	17.653	188	210278	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.971	240	199753	20.000	ng/u1	#-0.02
88) Perylene-d12	25.472	264	190587	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.602	96	3849	4.965	ng/uL	0.00
4) Pyridine-d5	4.025	84	26907	11.487	ng/u1	-0.02
7) Phenol-d5	7.402	99	17791	6.189	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.573	67	59747	34.961	ng/u1	-0.02
11) 2-Chlorophenol-d4	7.796	132	53271	26.644	ng/u1	-0.02
15) 4-Methylphenol-d8	8.965	113	28624	12.881	ng/u1	-0.02
21) Nitrobenzene-d5	9.441	128	35941	36.790	ng/u1	-0.02
24) 2-Nitrophenol-d4	10.169	143	37373	34.995	ng/u1	-0.02
28) 2,4-Dichlorophenol-d3	10.721	165	67124	28.984	ng/u1	0.00
31) 4-Chloroaniline-d4	11.232	131	26624	8.731	ng/u1	0.00
46) Dimethylphthalate-d6	14.293	166	245589	32.778	ng/u1	-0.02
49) Acenaphthylene-d8	14.598	160	89117	9.577	ng/u1	-0.02
54) 4-Nitrophenol-d4	15.080	143	7729	6.344	ng/u1	0.00
60) Fluorene-d10	15.897	176	227711	33.922	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.997	200	33626	30.693	ng/u1	-0.02
73) Anthracene-d10	17.753	188	284886	28.401	ng/u1	0.00
81) Pyrene-d10	20.026	212	459767	38.243	ng/u1	-0.02
92) Benzo(a)pyrene-d12	25.225	264	46827	4.670	ng/u1	-0.03
Target Compounds						
78) Di-n-butylphthalate	18.587	149	13097	1.112	ng/u1#	Qvalue 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
Data File : BG051800.D
Acq On : 27 Dec 2021 13:18
Operator : CG/JU
Sample : M5201-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P035-TW001-A-01


Quant Time: Dec 27 14:49:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 23 13:37:07 2021
Response via : Initial Calibration

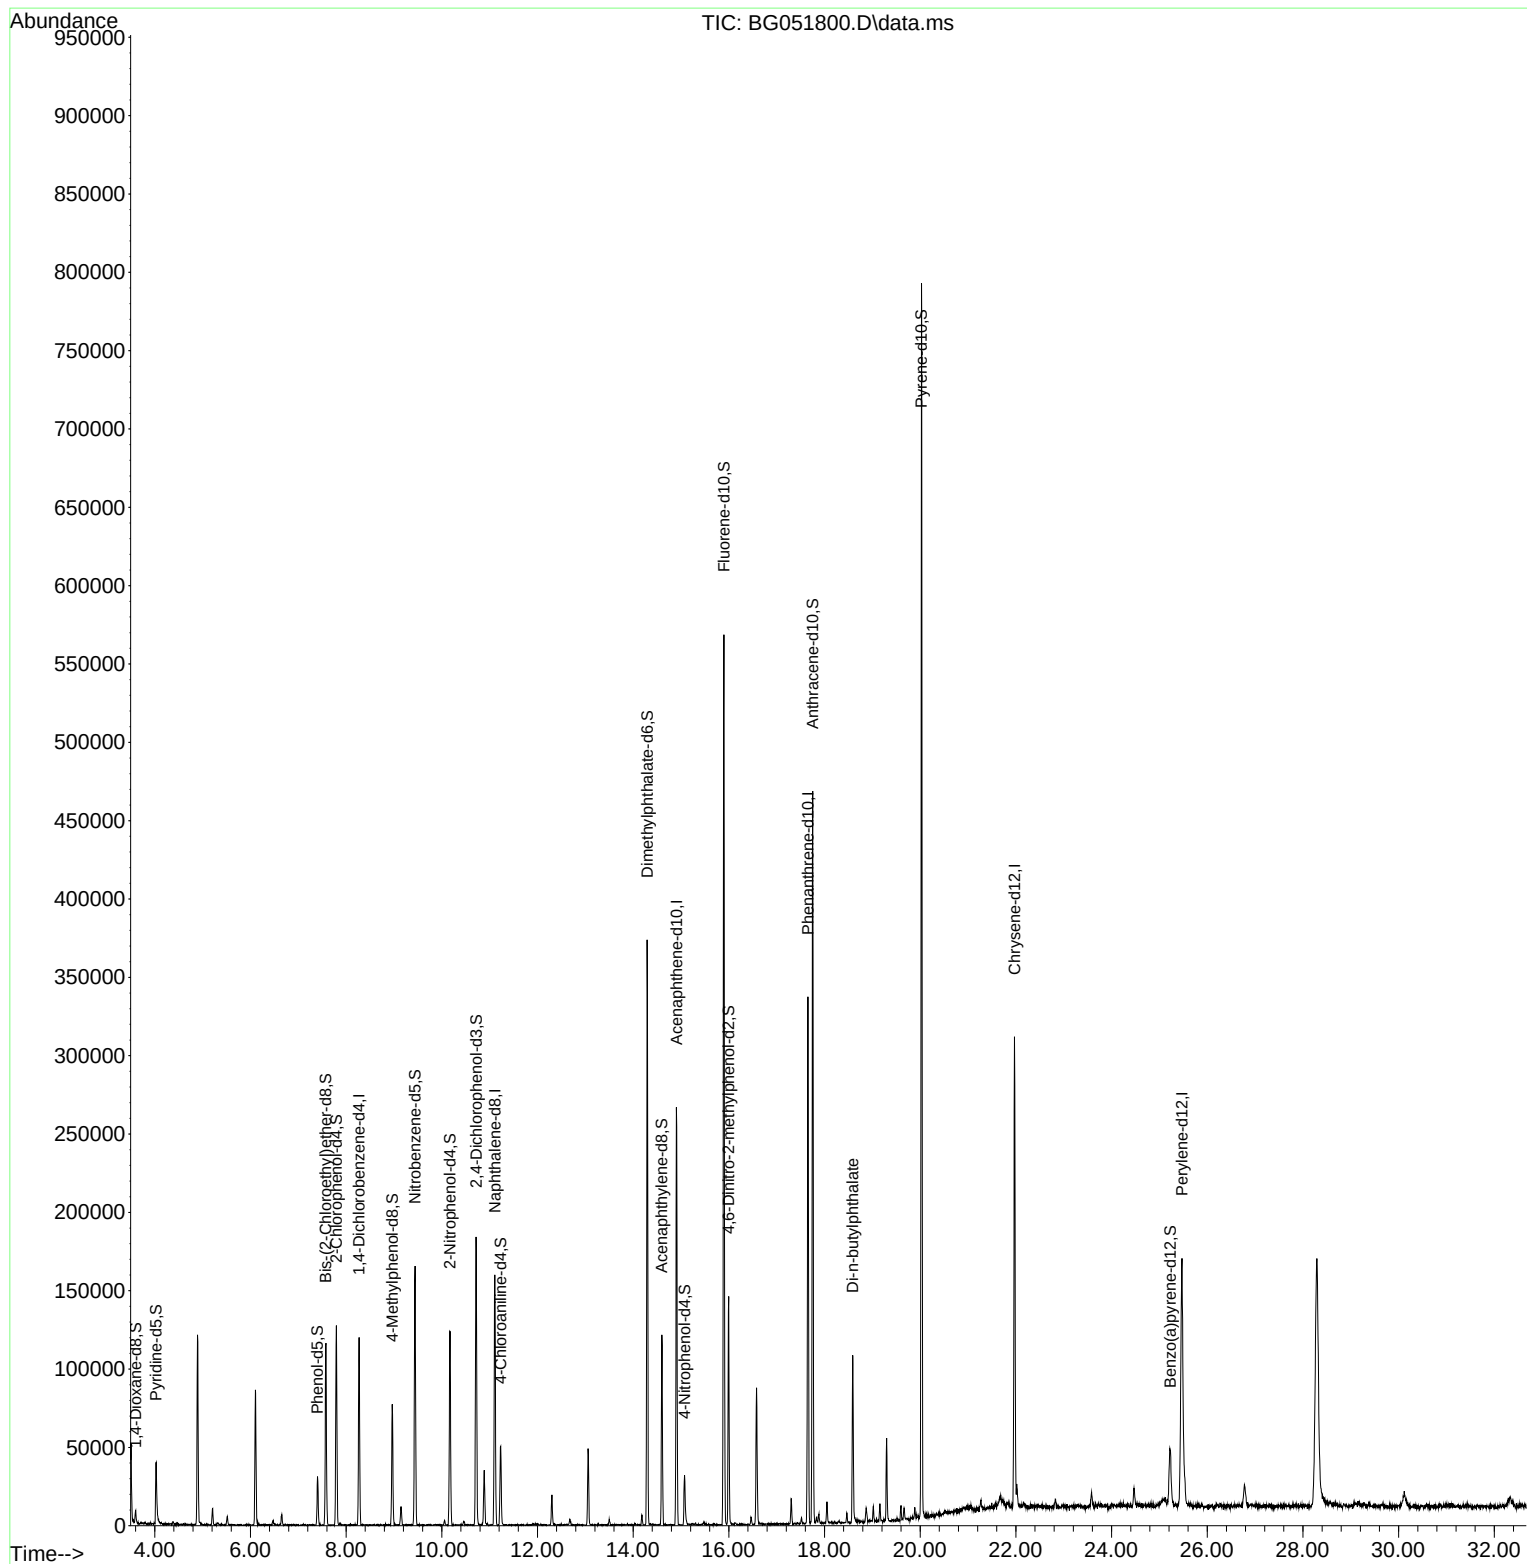

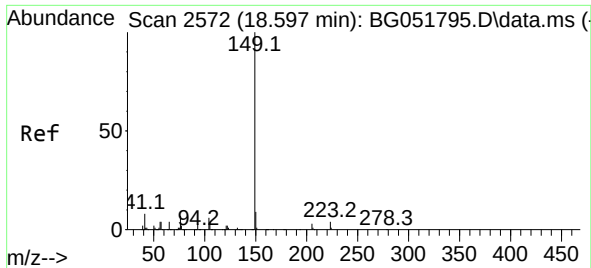

#78
 Di-n-butylphthalate
 Concen: 1.112 ng/ul
 RT: 18.587 min Scan# 21
 Delta R.T. -0.027 min
 Lab File: BG051800.D
 Acq: 27 Dec 2021 13:18

Instrument :
 BNA_G
 ClientSampleId :
 P035-TW001-A-01

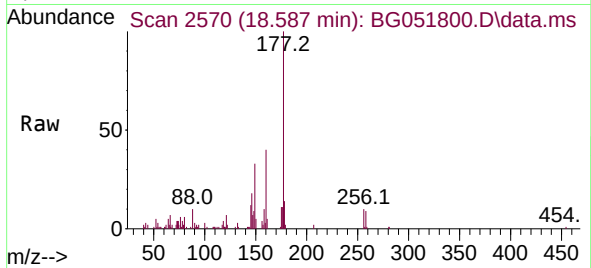

Tgt Ion:149 Resp: 13097
 Ion Ratio Lower Upper
 149 100
 150 15.7 7.5 11.3#
 104 0.0 5.0 7.6#

