

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
 Data File : BG051802.D
 Acq On : 27 Dec 2021 14:39
 Operator : CG/JU
 Sample : M5201-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P036-TW001-01

Quant Time: Dec 27 15:28:52 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 23 13:37:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.272	152	33179	20.000	ng/u1	-0.02
20) Naphthalene-d8	11.109	136	138765	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.904	164	94311	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.653	188	210899	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.971	240	201521	20.000	ng/u1	#-0.01
88) Perylene-d12	25.472	264	188658	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.602	96	4498	5.630	ng/uL	0.00
4) Pyridine-d5	4.031	84	27779	11.508	ng/u1	-0.01
7) Phenol-d5	7.408	99	23399	7.899	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.573	67	67024	38.058	ng/u1	-0.02
11) 2-Chlorophenol-d4	7.796	132	58264	28.279	ng/u1	-0.01
15) 4-Methylphenol-d8	8.965	113	41399	18.079	ng/u1	-0.01
21) Nitrobenzene-d5	9.441	128	38478	37.821	ng/u1	-0.01
24) 2-Nitrophenol-d4	10.169	143	40786	36.673	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.716	165	73251	30.372	ng/u1	-0.01
31) 4-Chloroaniline-d4	11.233	131	96798	30.484	ng/u1	0.00
46) Dimethylphthalate-d6	14.293	166	271873	36.016	ng/u1	-0.02
49) Acenaphthylene-d8	14.605	160	340720	36.343	ng/u1	0.00
54) 4-Nitrophenol-d4	15.074	143	6431	5.239	ng/u1	0.00
60) Fluorene-d10	15.897	176	246068	36.384	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.997	200	31735	28.881	ng/u1	-0.01
73) Anthracene-d10	17.753	188	437868	43.523	ng/u1	0.00
81) Pyrene-d10	20.032	212	500421	41.260	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.231	264	451935	45.528	ng/u1	-0.02
Target Compounds						
78) Di-n-butylphthalate	18.593	149	13416	1.136	ng/u1	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
Data File : BG051802.D
Acq On : 27 Dec 2021 14:39
Operator : CG/JU
Sample : M5201-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P036-TW001-01

Quant Time: Dec 27 15:28:52 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 23 13:37:07 2021
Response via : Initial Calibration

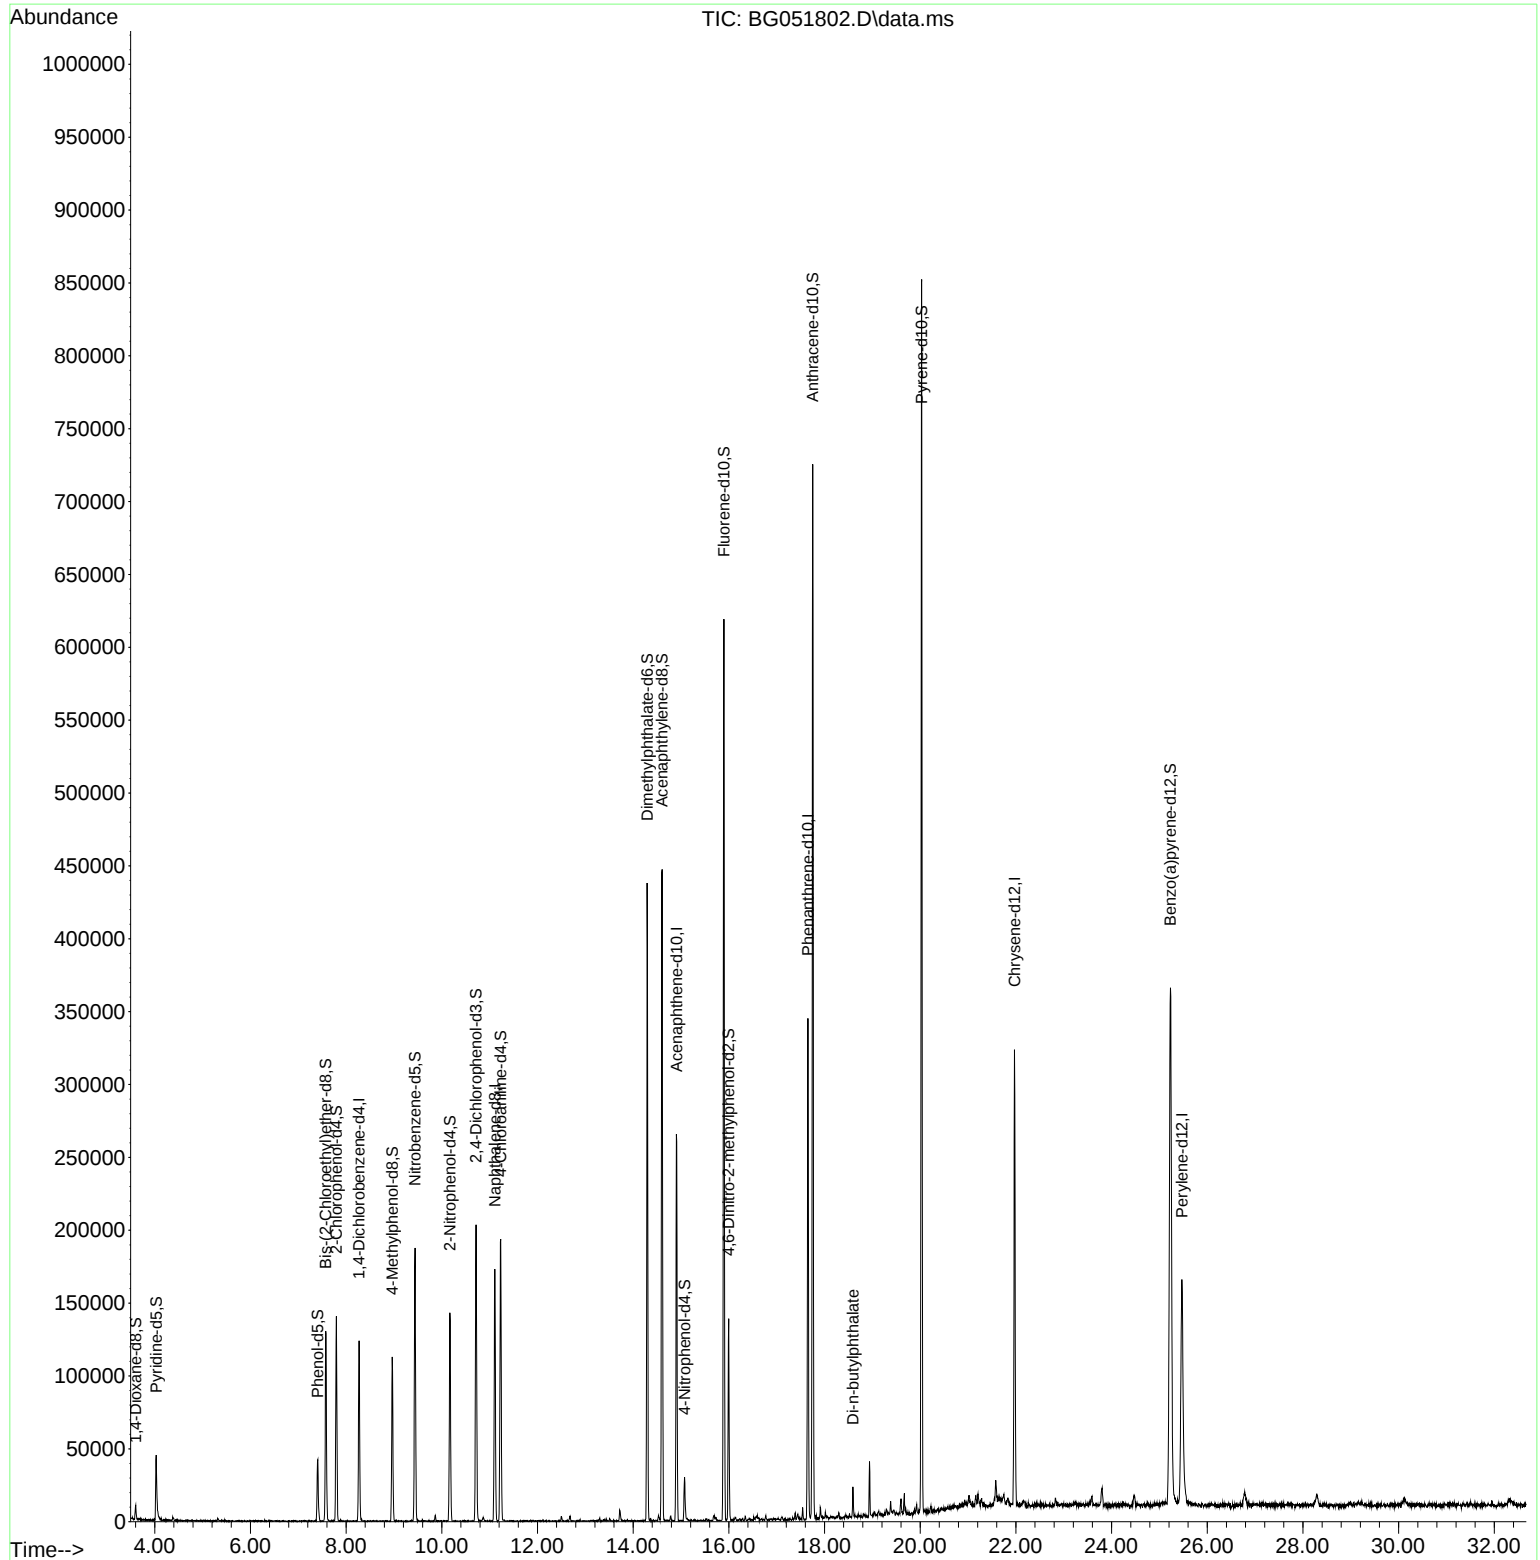

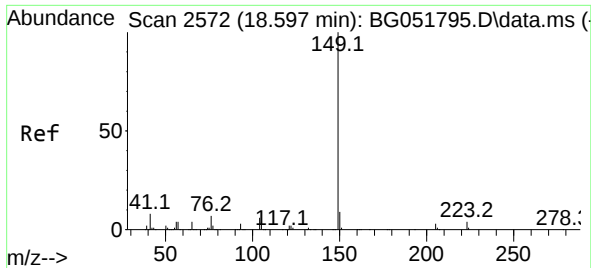

#78
 Di-n-butylphthalate
 Concen: 1.136 ng/ul
 RT: 18.593 min Scan# 21
 Delta R.T. -0.021 min
 Lab File: BG051802.D
 Acq: 27 Dec 2021 14:39

Instrument :
 BNA_G
 ClientSampleId :
 P036-TW001-01

Tgt Ion:149 Resp: 13416
 Ion Ratio Lower Upper
 149 100
 150 9.0 7.5 11.3
 104 6.1 5.0 7.6

