

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
 Data File : BG051801.D
 Acq On : 27 Dec 2021 13:58
 Operator : CG/JU
 Sample : M5201-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P035-TW001-C-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051801.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.600	13	19	24	rVV2	9623	15086	1.20%	0.134%
2	4.029	88	92	105	rBV	34121	62654	4.98%	0.556%
3	4.387	149	153	156	rBV	2882	3213	0.26%	0.029%
4	7.406	660	667	673	rBV	53300	94794	7.53%	0.841%
5	7.577	689	696	704	rVB	144663	239808	19.05%	2.128%
6	7.794	727	733	742	rVB	150059	262909	20.89%	2.333%
7	8.270	807	814	824	rVB	119070	210095	16.69%	1.864%
8	8.969	925	933	941	rBV	134868	240799	19.13%	2.136%
9	9.439	1005	1013	1022	rVB	194775	348947	27.72%	3.096%
10	9.856	1081	1084	1090	rVB3	1589	2628	0.21%	0.023%
11	10.173	1127	1138	1146	rBV	154287	276378	21.96%	2.452%
12	10.714	1223	1230	1244	rVB	219281	401510	31.90%	3.562%
13	11.107	1291	1297	1306	rVB	166274	302906	24.06%	2.688%
14	11.231	1309	1318	1330	rBV	204930	387334	30.77%	3.437%
15	12.682	1558	1565	1570	rVB	4628	6585	0.52%	0.058%
16	14.291	1833	1839	1846	rBV	430167	639489	50.81%	5.674%
17	14.602	1885	1892	1900	rBV	497646	781976	62.13%	6.938%
18	14.902	1937	1943	1953	rVB	267176	426565	33.89%	3.785%
19	15.072	1965	1972	1987	rBV2	36973	65479	5.20%	0.581%
20	15.895	2105	2112	2119	rBV	650738	975743	77.52%	8.657%
21	15.995	2123	2129	2138	rBV	130202	195460	15.53%	1.734%
22	16.130	2150	2152	2157	rVB2	2593	3061	0.24%	0.027%
23	17.446	2371	2376	2379	rBV3	1264	2084	0.17%	0.018%
24	17.651	2403	2411	2421	rBV	355115	521339	41.42%	4.626%
25	17.751	2421	2428	2438	rVV	739967	1101276	87.49%	9.771%
26	19.590	2735	2741	2747	rBV3	8642	13988	1.11%	0.124%
27	19.666	2747	2754	2758	rVV2	9358	15357	1.22%	0.136%
28	19.931	2795	2799	2803	rBV4	2864	4595	0.37%	0.041%
29	20.030	2807	2816	2822	rBV	871101	1258707	100.00%	11.168%
30	20.465	2889	2890	2894	rVB4	2138	2459	0.20%	0.022%
31	20.494	2894	2895	2898	rBV3	2129	2506	0.20%	0.022%
32	20.712	2929	2932	2934	rBV3	2611	3292	0.26%	0.029%
33	20.765	2938	2941	2942	rBV3	1948	1998	0.16%	0.018%
34	20.917	2963	2967	2974	rVB3	16510	21314	1.69%	0.189%
35	21.311	3033	3034	3037	rBV3	2847	2487	0.20%	0.022%
36	21.387	3046	3047	3051	rBV4	2750	2885	0.23%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
 Data File : BG051801.D
 Acq On : 27 Dec 2021 13:58
 Operator : CG/JU
 Sample : M5201-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P035-TW001-C-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	21.434	3053	3055	3058	rBV4	2379	2995	0.24%	0.027%
38	21.552	3072	3075	3076	rBV3	2296	2457	0.20%	0.022%
39	21.570	3076	3078	3081	rVV4	3079	3184	0.25%	0.028%
40	21.640	3088	3090	3091	rVV2	3244	2423	0.19%	0.021%
41	21.663	3092	3094	3098	rVB5	3696	3563	0.28%	0.032%
42	21.975	3139	3147	3156	rBV	301714	533201	42.36%	4.731%
43	22.163	3177	3179	3185	rVB6	3808	4126	0.33%	0.037%
44	22.821	3286	3291	3295	rBV7	4496	8091	0.64%	0.072%
45	22.915	3305	3307	3309	rBV3	2486	2338	0.19%	0.021%
46	23.097	3337	3338	3342	rVB4	2991	2918	0.23%	0.026%
47	23.232	3359	3361	3363	rVB3	2292	1946	0.15%	0.017%
48	23.555	3413	3416	3417	rBV3	5840	5621	0.45%	0.050%
49	23.631	3428	3429	3431	rBV2	2640	2185	0.17%	0.019%
50	23.737	3445	3447	3452	rVB6	2480	3352	0.27%	0.030%
51	23.778	3452	3454	3457	rBV4	3237	3418	0.27%	0.030%
52	24.148	3515	3517	3518	rVB2	3388	1996	0.16%	0.018%
53	24.471	3567	3572	3580	rVB9	12068	28296	2.25%	0.251%
54	25.082	3672	3676	3677	rVB3	2803	2906	0.23%	0.026%
55	25.229	3689	3701	3716	rVV2	341762	1096817	87.14%	9.731%
56	25.394	3728	3729	3730	rBV	4036	1914	0.15%	0.017%
57	25.470	3732	3742	3762	rVB2	152945	532679	42.32%	4.726%
58	25.599	3762	3764	3766	rBV3	2246	1917	0.15%	0.017%
59	25.787	3795	3796	3798	rBV2	3823	2401	0.19%	0.021%
60	25.958	3823	3825	3828	rBV4	1969	2626	0.21%	0.023%
61	26.128	3850	3854	3856	rBV3	3515	4736	0.38%	0.042%
62	26.269	3877	3878	3880	rBV2	3328	2014	0.16%	0.018%
63	26.287	3880	3881	3884	rVV2	3051	2375	0.19%	0.021%
64	26.334	3887	3889	3892	rBV4	2312	2507	0.20%	0.022%
65	26.486	3912	3915	3918	rBV3	2955	4695	0.37%	0.042%
66	26.745	3957	3959	3960	rBV2	3092	3051	0.24%	0.027%
67	26.762	3960	3962	3963	rBV2	6015	4783	0.38%	0.042%
68	26.986	3998	4000	4003	rVB4	2897	2094	0.17%	0.019%
69	27.056	4010	4012	4017	rVB6	2717	3808	0.30%	0.034%
70	27.097	4017	4019	4021	rBV3	2830	2221	0.18%	0.020%
71	27.185	4033	4034	4039	rBV5	2752	3928	0.31%	0.035%
72	27.426	4074	4075	4077	rBV2	2275	1975	0.16%	0.018%
73	27.626	4107	4109	4112	rBV4	1983	2297	0.18%	0.020%
74	27.773	4133	4134	4136	rBV2	2403	2105	0.17%	0.019%
75	27.914	4156	4158	4164	rVB7	2569	3319	0.26%	0.029%
76	28.196	4202	4206	4209	rVB6	2534	3335	0.26%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
 Data File : BG051801.D
 Acq On : 27 Dec 2021 13:58
 Operator : CG/JU
 Sample : M5201-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P035-TW001-C-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	28.219	4209	4210	4213	rBV3	2213	2441	0.19%	0.022%
78	28.255	4215	4216	4217	rBV	4488	2885	0.23%	0.026%
79	28.272	4217	4219	4220	rBV2	3775	2432	0.19%	0.022%
80	28.660	4281	4285	4286	rBV4	3413	4175	0.33%	0.037%
81	28.995	4341	4342	4344	rBV2	3647	2574	0.20%	0.023%
82	29.212	4378	4379	4382	rVB3	4765	3756	0.30%	0.033%
83	29.412	4412	4413	4415	rBV2	4168	3040	0.24%	0.027%
84	29.753	4469	4471	4474	rVB4	3127	2221	0.18%	0.020%
85	29.835	4483	4485	4488	rBV4	2305	2524	0.20%	0.022%
86	30.011	4514	4515	4519	rBV4	2209	3129	0.25%	0.028%
87	30.082	4524	4527	4528	rBV3	2628	2791	0.22%	0.025%
88	30.311	4564	4566	4567	rBV2	2358	1986	0.16%	0.018%
89	30.446	4587	4589	4592	rBV4	2194	2290	0.18%	0.020%
90	30.857	4656	4659	4662	rBV4	1897	3361	0.27%	0.030%
91	31.051	4689	4692	4693	rBV2	2304	2322	0.18%	0.021%
92	31.227	4721	4722	4725	rVB3	2769	1942	0.15%	0.017%
93	31.368	4744	4746	4749	rVB4	2464	2169	0.17%	0.019%
94	31.438	4756	4758	4762	rVB4	2736	2857	0.23%	0.025%
95	31.838	4824	4826	4827	rBV2	2606	2153	0.17%	0.019%
96	31.903	4835	4837	4838	rBV2	2500	1910	0.15%	0.017%
97	31.920	4838	4840	4842	rVV3	3012	2768	0.22%	0.025%
98	32.302	4901	4905	4908	rBV6	3694	7317	0.58%	0.065%
99	32.343	4910	4912	4915	rVV3	5031	5502	0.44%	0.049%
100	32.561	4947	4949	4951	rVB3	2472	1972	0.16%	0.017%




Sum of corrected areas: 11270836

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
Data File : BG051801.D
Acq On : 27 Dec 2021 13:58
Operator : CG/JU
Sample : M5201-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P035-TW001-C-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

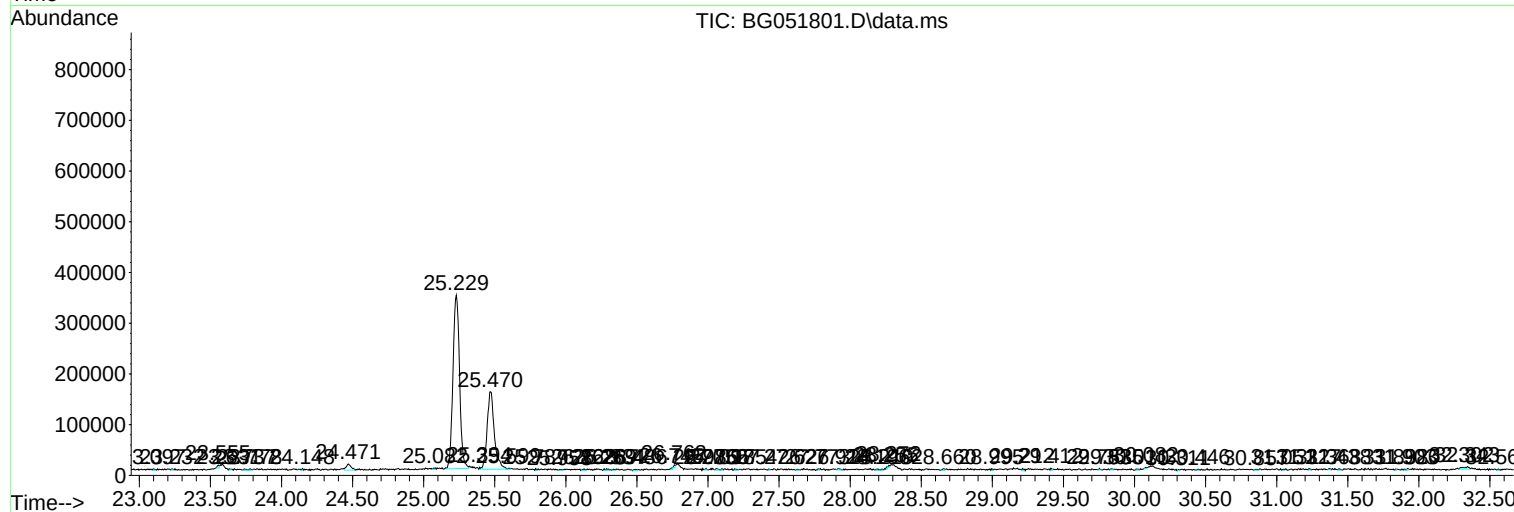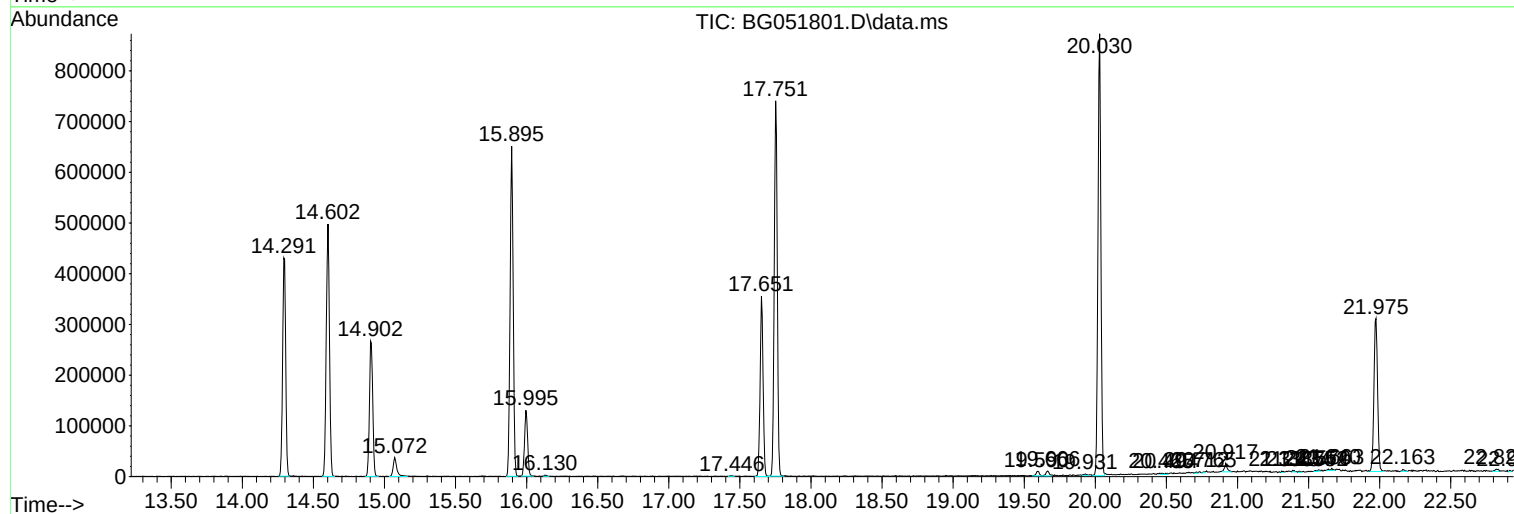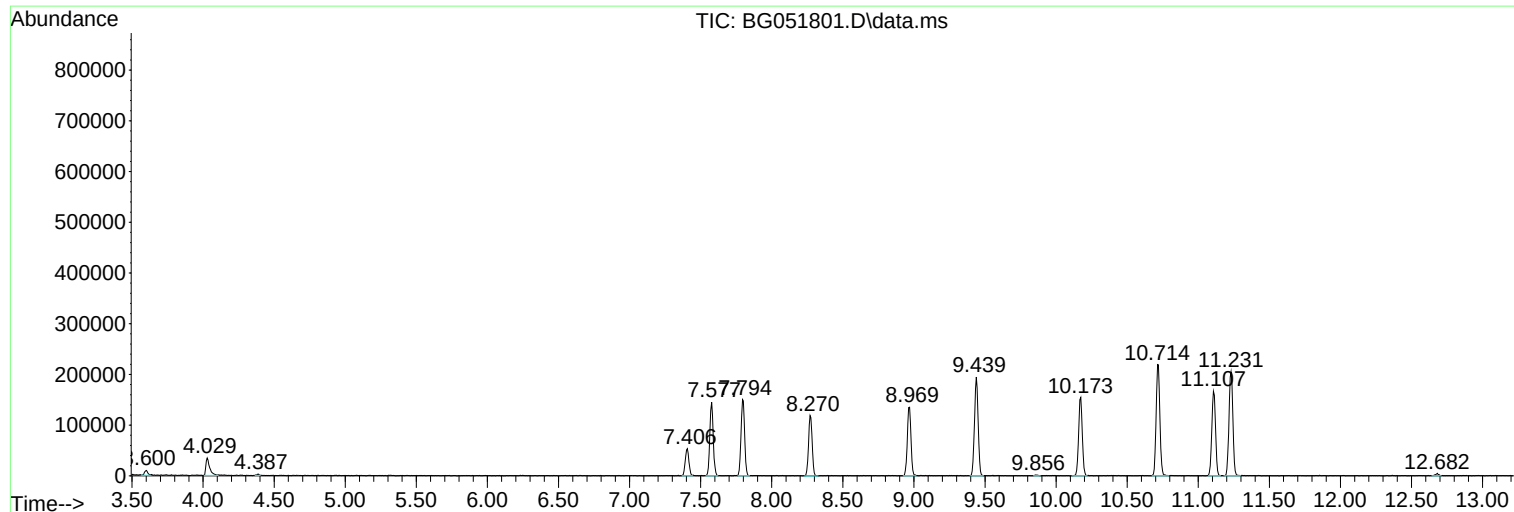

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
Data File : BG051801.D
Acq On : 27 Dec 2021 13:58
Operator : CG/JU
Sample : M5201-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P035-TW001-C-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
Data File : BG051801.D
Acq On : 27 Dec 2021 13:58
Operator : CG/JU
Sample : M5201-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P035-TW001-C-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc