

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
 Data File : BG051814.D
 Acq On : 27 Dec 2021 23:26
 Operator : CG/JU
 Sample : M5193-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0J00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051814.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.579	9	15	17	rBV5	13270	23502	2.01%	0.219%
2	3.837	57	59	62	rBV2	1756	1991	0.17%	0.019%
3	3.878	62	66	68	rBV	4785	5683	0.49%	0.053%
4	4.031	88	92	105	rBV	37674	73425	6.28%	0.684%
5	4.383	149	152	155	rVB3	2328	2152	0.18%	0.020%
6	4.712	205	208	214	rVB2	1145	1856	0.16%	0.017%
7	4.795	218	222	224	rBV3	1416	1697	0.15%	0.016%
8	7.250	637	640	642	rBV3	1558	1546	0.13%	0.014%
9	7.409	659	667	673	rBV3	34169	66618	5.70%	0.621%
10	7.573	688	695	703	rBV	126554	219543	18.78%	2.045%
11	7.796	726	733	742	rBV	127029	221132	18.92%	2.060%
12	8.272	807	814	820	rBV	138807	228848	19.58%	2.132%
13	8.325	820	823	827	rVB	2156	2319	0.20%	0.022%
14	8.742	891	894	897	rBV	1171	1619	0.14%	0.015%
15	8.883	912	918	923	rBV3	2129	4404	0.38%	0.041%
16	8.965	925	932	940	rVB2	98819	178845	15.30%	1.666%
17	9.441	1006	1013	1024	rBV	182821	323313	27.66%	3.012%
18	9.870	1081	1086	1089	rVB2	5379	8005	0.68%	0.075%
19	10.170	1129	1137	1146	rVB	137086	249372	21.34%	2.323%
20	10.716	1223	1230	1244	rVB	192754	354002	30.29%	3.298%
21	11.110	1290	1297	1306	rVB	175217	334423	28.61%	3.115%
22	11.233	1309	1318	1326	rBV	158104	296645	25.38%	2.763%
23	12.361	1505	1510	1514	rVB3	6317	9823	0.84%	0.092%
24	12.672	1559	1563	1570	rVB3	2971	4702	0.40%	0.044%
25	12.972	1611	1614	1621	rVB	911	1778	0.15%	0.017%
26	13.506	1700	1705	1708	rBV2	1429	1681	0.14%	0.016%
27	13.724	1736	1742	1745	rBV2	4066	6777	0.58%	0.063%
28	14.293	1833	1839	1848	rVB	401586	606963	51.93%	5.654%
29	14.534	1877	1880	1885	rBV3	3250	5410	0.46%	0.050%
30	14.605	1885	1892	1902	rVB	450049	724908	62.02%	6.753%
31	14.787	1919	1923	1927	rVB4	2723	3548	0.30%	0.033%
32	14.904	1935	1943	1950	rBV	296035	473650	40.53%	4.412%
33	15.075	1966	1972	1979	rBV2	23753	44068	3.77%	0.411%
34	15.527	2043	2049	2055	rBV3	2226	3797	0.32%	0.035%
35	15.686	2072	2076	2081	rBV3	3884	6928	0.59%	0.065%
36	15.733	2082	2084	2089	rVB3	2179	2589	0.22%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
 Data File : BG051814.D
 Acq On : 27 Dec 2021 23:26
 Operator : CG/JU
 Sample : M5193-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0J00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	15.897	2103	2112	2120	rBV	600665	914950	78.29%	8.523%
38	15.997	2123	2129	2139	rVV	156158	240436	20.57%	2.240%
39	16.138	2151	2153	2158	rVB3	3586	3830	0.33%	0.036%
40	16.285	2174	2178	2182	rVV4	1796	3134	0.27%	0.029%
41	16.344	2186	2188	2191	rVB3	2197	2035	0.17%	0.019%
42	16.532	2216	2220	2223	rVB4	2593	3168	0.27%	0.030%
43	16.567	2223	2226	2227	rBV2	2741	2826	0.24%	0.026%
44	16.579	2227	2228	2233	rVB4	2150	3041	0.26%	0.028%
45	16.678	2243	2245	2248	rVB2	2342	1806	0.15%	0.017%
46	16.767	2258	2260	2264	rVB3	2090	1651	0.14%	0.015%
47	16.960	2289	2293	2297	rBV3	4142	4512	0.39%	0.042%
48	17.025	2302	2304	2311	rVB3	1564	2962	0.25%	0.028%
49	17.107	2314	2318	2319	rBV3	2557	2739	0.23%	0.026%
50	17.172	2326	2329	2331	rVB2	2652	1688	0.14%	0.016%
51	17.289	2347	2349	2352	rVB2	1715	1569	0.13%	0.015%
52	17.319	2352	2354	2357	rBV3	1561	2060	0.18%	0.019%
53	17.389	2362	2366	2370	rVB2	4243	6443	0.55%	0.060%
54	17.442	2370	2375	2379	rBV5	3274	5816	0.50%	0.054%
55	17.542	2388	2392	2397	rBV4	5474	6584	0.56%	0.061%
56	17.654	2405	2411	2418	rBV	377109	558922	47.82%	5.207%
57	17.754	2420	2428	2437	rVB2	641205	1021321	87.39%	9.514%
58	17.918	2452	2456	2459	rBV3	4373	6190	0.53%	0.058%
59	18.000	2469	2470	2473	rBV3	2696	1569	0.13%	0.015%
60	18.030	2473	2475	2478	rBV3	2176	2961	0.25%	0.028%
61	18.129	2490	2492	2494	rBV2	2254	2653	0.23%	0.025%
62	18.306	2518	2522	2526	rVB5	3641	5178	0.44%	0.048%
63	18.388	2532	2536	2538	rBV3	1971	2798	0.24%	0.026%
64	18.441	2543	2545	2549	rVB5	2847	3780	0.32%	0.035%
65	18.476	2549	2551	2553	rBV2	2122	1991	0.17%	0.019%
66	18.523	2554	2559	2566	rVV2	24624	38533	3.30%	0.359%
67	18.594	2567	2571	2575	rVB	10560	14653	1.25%	0.137%
68	18.705	2588	2590	2595	rVB3	2649	2806	0.24%	0.026%
69	18.746	2595	2597	2600	rVB4	2049	2221	0.19%	0.021%
70	18.811	2605	2608	2611	rBV4	2495	3511	0.30%	0.033%
71	18.934	2627	2629	2636	rVB7	5024	7255	0.62%	0.068%
72	19.040	2645	2647	2652	rVB5	2612	3492	0.30%	0.033%
73	19.134	2660	2663	2668	rBV5	4170	6288	0.54%	0.059%
74	19.281	2683	2688	2689	rBV4	2636	3507	0.30%	0.033%
75	19.381	2702	2705	2710	rVB6	5723	6200	0.53%	0.058%
76	19.598	2738	2742	2745	rBV4	7915	11293	0.97%	0.105%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
 Data File : BG051814.D
 Acq On : 27 Dec 2021 23:26
 Operator : CG/JU
 Sample : M5193-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0J00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	19.669	2749	2754	2756	rBV2	10540	14518	1.24%	0.135%
78	19.698	2757	2759	2762	rVB4	5836	6300	0.54%	0.059%
79	19.780	2770	2773	2778	rBV6	9030	13885	1.19%	0.129%
80	20.033	2809	2816	2822	rBV	791087	1168741	100.00%	10.887%
81	21.584	3077	3080	3083	rBV5	8982	11658	1.00%	0.109%
82	21.971	3140	3146	3153	rVB2	326063	569764	48.75%	5.308%
83	23.575	3417	3419	3425	rVB6	8746	15376	1.32%	0.143%
84	25.226	3690	3700	3716	rBV2	300889	978280	83.70%	9.113%
85	25.467	3733	3741	3759	rVB2	153260	537809	46.02%	5.010%
86	28.128	4193	4194	4196	rBV2	4124	2510	0.21%	0.023%




Sum of corrected areas: 10734775

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
Data File : BG051814.D
Acq On : 27 Dec 2021 23:26
Operator : CG/JU
Sample : M5193-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0J00

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

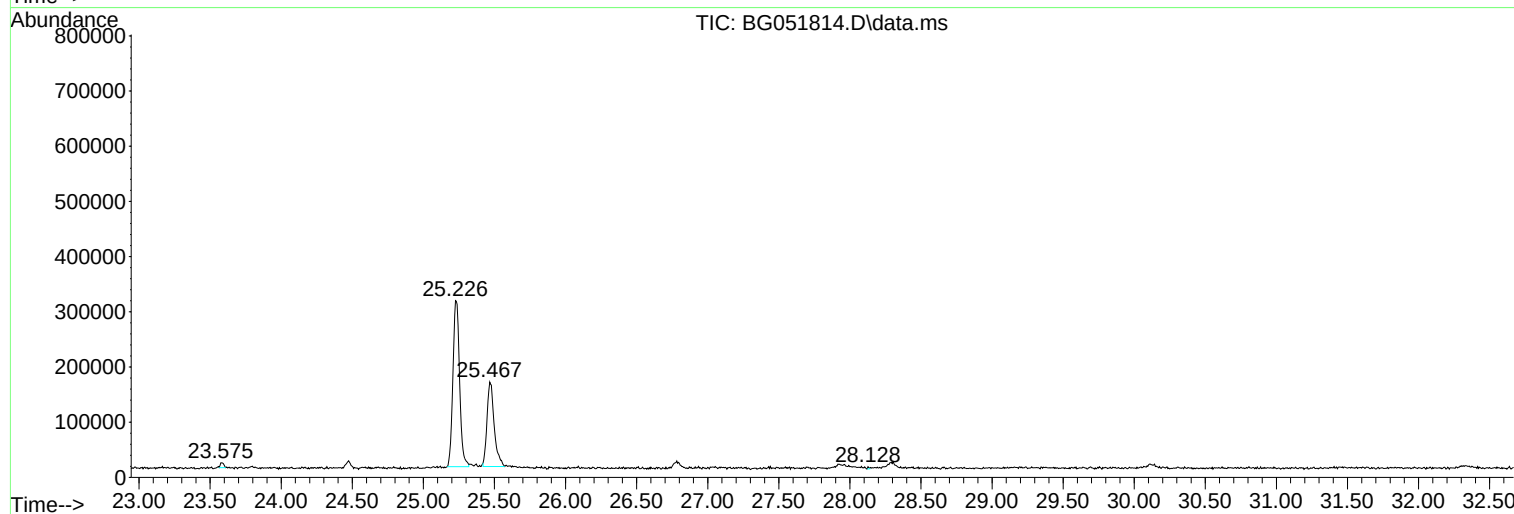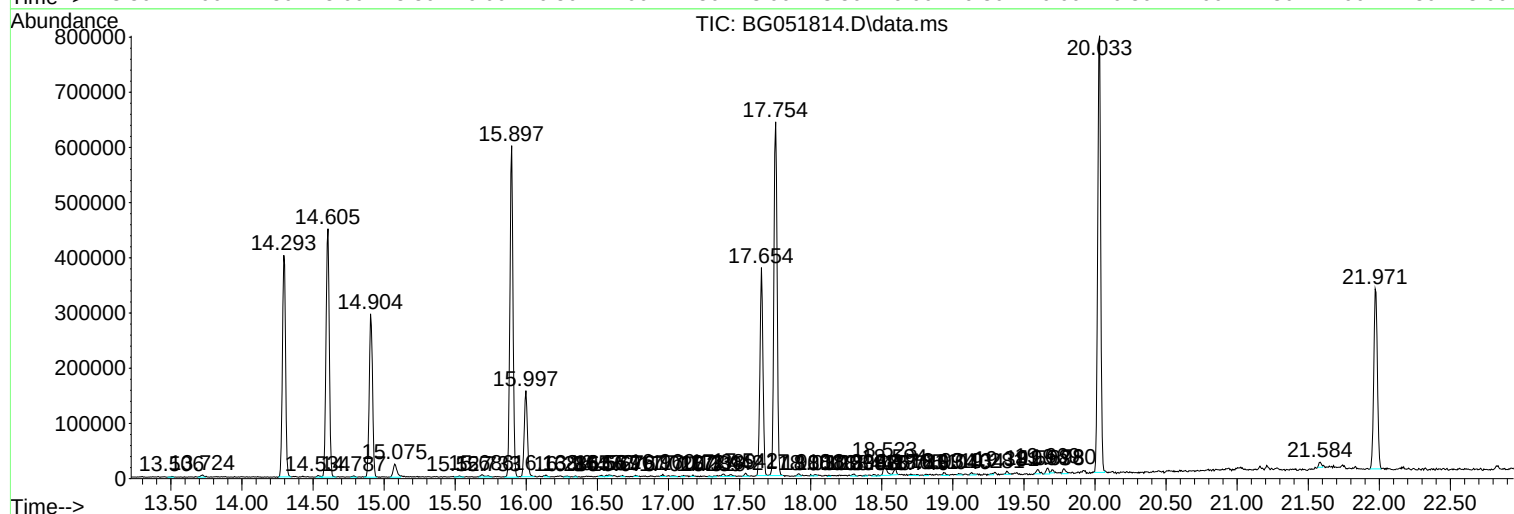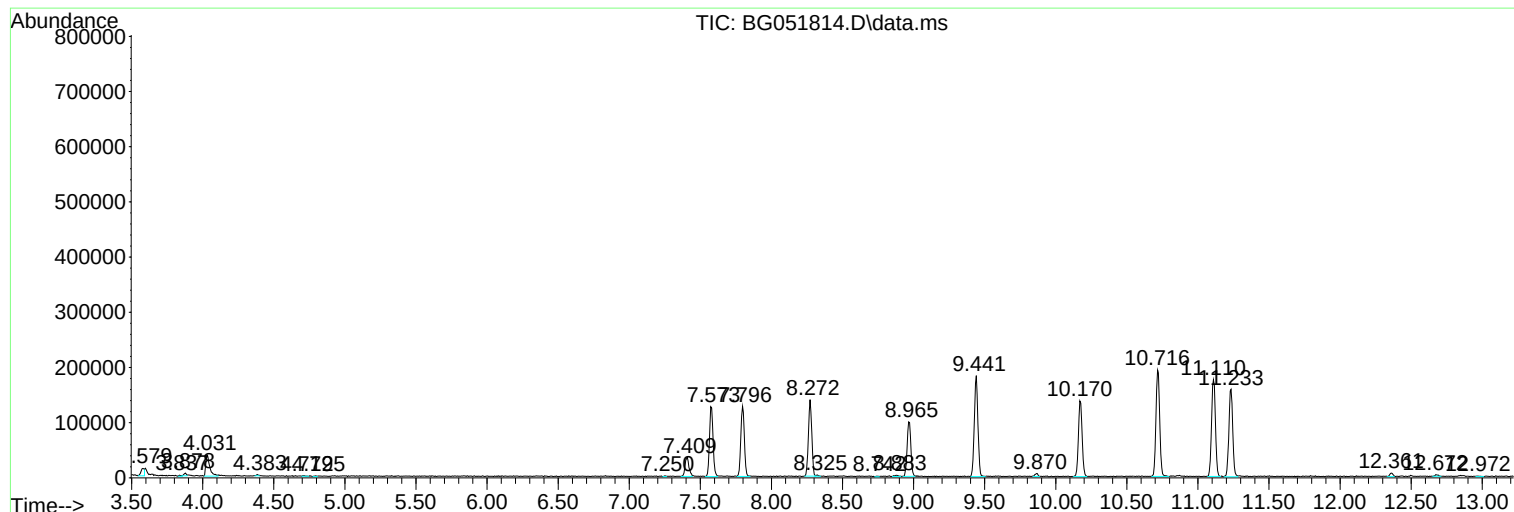

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
Data File : BG051814.D
Acq On : 27 Dec 2021 23:26
Operator : CG/JU
Sample : M5193-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0J00

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
Data File : BG051814.D
Acq On : 27 Dec 2021 23:26
Operator : CG/JU
Sample : M5193-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0J00

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc