

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
 Data File : BG051822.D
 Acq On : 28 Dec 2021 4:48
 Operator : CG/JU
 Sample : M5193-13
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0J32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051822.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.558	9	12	14	rVB3	1273	1371	0.10%	0.012%
2	3.599	14	19	23	rBV2	8373	11592	0.88%	0.102%
3	3.740	41	43	48	rVB2	1087	1453	0.11%	0.013%
4	4.034	89	93	104	rBV	32265	58847	4.48%	0.520%
5	4.381	148	152	157	rVB4	2853	4683	0.36%	0.041%
6	4.610	188	191	194	rBV2	808	1407	0.11%	0.012%
7	5.315	308	311	314	rBV2	951	1388	0.11%	0.012%
8	7.165	623	626	631	rVB2	1101	1521	0.12%	0.013%
9	7.406	661	667	673	rVB	37038	63796	4.85%	0.563%
10	7.576	688	696	705	rVB	144258	240046	18.26%	2.119%
11	7.800	727	734	743	rVV	140681	252253	19.19%	2.227%
12	8.270	807	814	823	rBV	134542	224620	17.09%	1.983%
13	8.510	850	855	856	rBV2	1988	1903	0.14%	0.017%
14	8.969	927	933	942	rVB2	112019	191970	14.60%	1.695%
15	9.362	999	1000	1006	rVB2	1225	1523	0.12%	0.013%
16	9.439	1006	1013	1022	rBV	196338	354763	26.98%	3.132%
17	9.591	1035	1039	1042	rBV3	1749	2284	0.17%	0.020%
18	9.862	1082	1085	1088	rBV2	1608	1681	0.13%	0.015%
19	10.173	1131	1138	1147	rVV2	158257	283613	21.57%	2.504%
20	10.719	1222	1231	1240	rBV	219268	393510	29.93%	3.474%
21	11.107	1290	1297	1309	rVB	181532	331618	25.22%	2.928%
22	11.230	1311	1318	1328	rVV2	204535	365995	27.84%	3.231%
23	11.712	1394	1400	1403	rBV2	721	1471	0.11%	0.013%
24	12.129	1467	1471	1474	rVB	1066	1664	0.13%	0.015%
25	12.229	1487	1488	1493	rBV2	1209	1690	0.13%	0.015%
26	12.681	1560	1565	1570	rVB3	3818	6227	0.47%	0.055%
27	14.297	1833	1840	1847	rBV	461872	671802	51.10%	5.931%
28	14.602	1885	1892	1904	rVB	493632	771186	58.66%	6.808%
29	14.908	1935	1944	1951	rBV	299503	473765	36.04%	4.182%
30	15.078	1968	1973	1982	rBV3	22681	44978	3.42%	0.397%
31	15.689	2075	2077	2082	rVV3	1439	2912	0.22%	0.026%
32	15.736	2082	2085	2087	rVB	1470	1653	0.13%	0.015%
33	15.895	2105	2112	2120	rVV	654137	1006002	76.52%	8.881%
34	16.000	2123	2130	2135	rBV	69956	111189	8.46%	0.982%
35	16.135	2149	2153	2156	rVB3	1818	2908	0.22%	0.026%
36	16.470	2205	2210	2213	rBV2	1360	2097	0.16%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
 Data File : BG051822.D
 Acq On : 28 Dec 2021 4:48
 Operator : CG/JU
 Sample : M5193-13
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0J32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	17.263	2344	2345	2350	rVB4	1650	2069	0.16%	0.018%
38	17.557	2393	2395	2398	rBV3	1778	1931	0.15%	0.017%
39	17.657	2405	2412	2421	rVB	374867	568260	43.22%	5.017%
40	17.757	2421	2429	2437	rBV2	742587	1160971	88.31%	10.249%
41	17.827	2437	2441	2444	rVV4	4411	5903	0.45%	0.052%
42	17.863	2446	2447	2452	rVB3	1402	1541	0.12%	0.014%
43	17.992	2466	2469	2471	rBV2	2045	1896	0.14%	0.017%
44	18.015	2471	2473	2477	rVB3	1556	1641	0.12%	0.014%
45	18.051	2477	2479	2481	rBV2	1834	1390	0.11%	0.012%
46	18.133	2490	2493	2494	rBV2	2170	2129	0.16%	0.019%
47	18.186	2500	2502	2506	rVB2	1217	1452	0.11%	0.013%
48	18.285	2515	2519	2520	rBV3	1467	1318	0.10%	0.012%
49	18.303	2520	2522	2529	rVB5	8182	10708	0.81%	0.095%
50	18.415	2539	2541	2547	rVB4	1588	1948	0.15%	0.017%
51	18.473	2547	2551	2554	rVB3	1933	2856	0.22%	0.025%
52	18.515	2554	2558	2561	rBV2	1526	2849	0.22%	0.025%
53	18.556	2564	2565	2567	rBV2	2137	1703	0.13%	0.015%
54	18.609	2572	2574	2575	rVV	1934	1378	0.10%	0.012%
55	18.638	2578	2579	2582	rVV2	1774	1461	0.11%	0.013%
56	18.708	2586	2591	2593	rVB5	1068	1764	0.13%	0.016%
57	18.820	2605	2610	2613	rVB6	2693	4358	0.33%	0.038%
58	18.891	2620	2622	2625	rBV4	2051	1940	0.15%	0.017%
59	19.020	2643	2644	2649	rBV4	2024	3427	0.26%	0.030%
60	19.084	2653	2655	2656	rBV2	2307	1741	0.13%	0.015%
61	19.331	2696	2697	2700	rVB3	2841	1392	0.11%	0.012%
62	19.378	2703	2705	2709	rBV5	1779	1965	0.15%	0.017%
63	19.437	2713	2715	2718	rVB4	5026	3842	0.29%	0.034%
64	19.466	2718	2720	2721	rBV2	4040	2590	0.20%	0.023%
65	19.554	2733	2735	2738	rBV3	2743	2889	0.22%	0.026%
66	19.595	2738	2742	2747	rVV5	12523	18945	1.44%	0.167%
67	19.666	2749	2754	2760	rVB2	11752	19520	1.48%	0.172%
68	19.719	2760	2763	2764	rBV3	2115	2374	0.18%	0.021%
69	19.866	2786	2788	2791	rBV4	1877	2112	0.16%	0.019%
70	20.030	2808	2816	2823	rBV	884588	1314683	100.00%	11.606%
71	20.095	2826	2827	2830	rBV3	3296	2939	0.22%	0.026%
72	20.130	2832	2833	2835	rBV2	3134	1987	0.15%	0.018%
73	20.242	2850	2852	2856	rVB5	3767	2804	0.21%	0.025%
74	20.336	2867	2868	2870	rBV2	2943	2163	0.16%	0.019%
75	20.465	2888	2890	2891	rBV2	2970	1742	0.13%	0.015%
76	20.529	2899	2901	2902	rBV2	2618	1792	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
 Data File : BG051822.D
 Acq On : 28 Dec 2021 4:48
 Operator : CG/JU
 Sample : M5193-13
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0J32

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	20.600	2912	2913	2914	rBV	3742	2565	0.20%	0.023%
78	21.305	3031	3033	3034	rBV2	3648	2689	0.20%	0.024%
79	21.975	3140	3147	3156	rBV	325724	571644	43.48%	5.047%
80	22.133	3173	3174	3175	rBV	5624	2375	0.18%	0.021%
81	22.204	3184	3186	3188	rBV3	4078	3307	0.25%	0.029%
82	22.380	3214	3216	3218	rVB3	5135	3696	0.28%	0.033%
83	22.826	3290	3292	3296	rVB5	7540	8071	0.61%	0.071%
84	23.473	3400	3402	3403	rVB2	4978	2780	0.21%	0.025%
85	24.424	3562	3564	3566	rBV3	4742	4401	0.33%	0.039%
86	24.471	3568	3572	3577	rVB8	10297	21329	1.62%	0.188%
87	25.059	3670	3672	3673	rBV2	4419	2384	0.18%	0.021%
88	25.235	3691	3702	3717	rVB2	362431	1077491	81.96%	9.512%
89	25.470	3733	3742	3759	rVB3	155037	538381	40.95%	4.753%
90	27.696	4120	4121	4122	rBV	5034	1966	0.15%	0.017%
91	28.583	4270	4272	4273	rBV2	6965	5264	0.40%	0.046%
92	29.147	4367	4368	4370	rBV2	5665	3269	0.25%	0.029%
93	30.111	4528	4532	4534	rBV4	5865	9369	0.71%	0.083%
94	31.538	4774	4775	4777	rBV2	5520	4719	0.36%	0.042%




Sum of corrected areas: 11327454

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
Data File : BG051822.D
Acq On : 28 Dec 2021 4:48
Operator : CG/JU
Sample : M5193-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0J32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

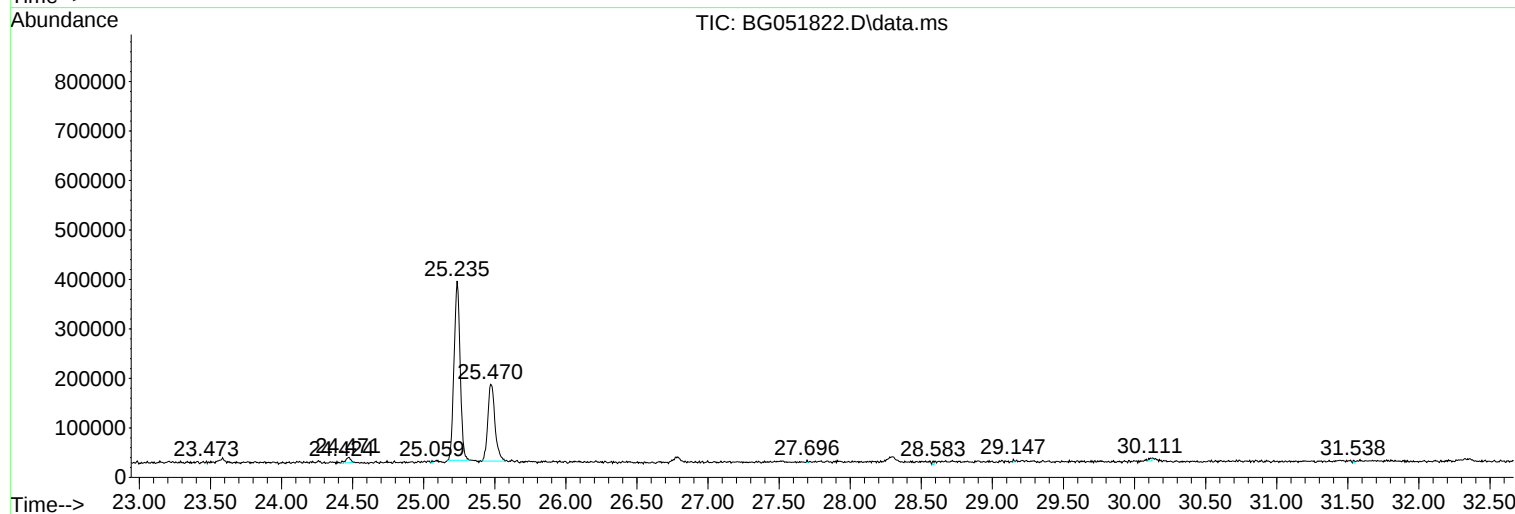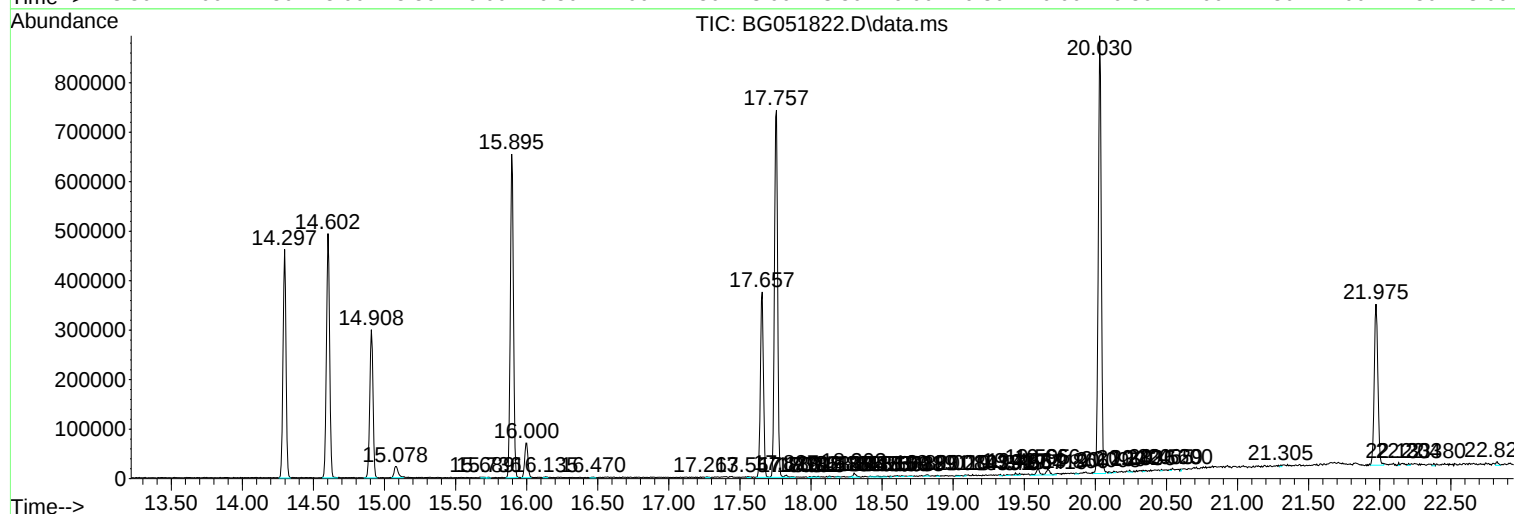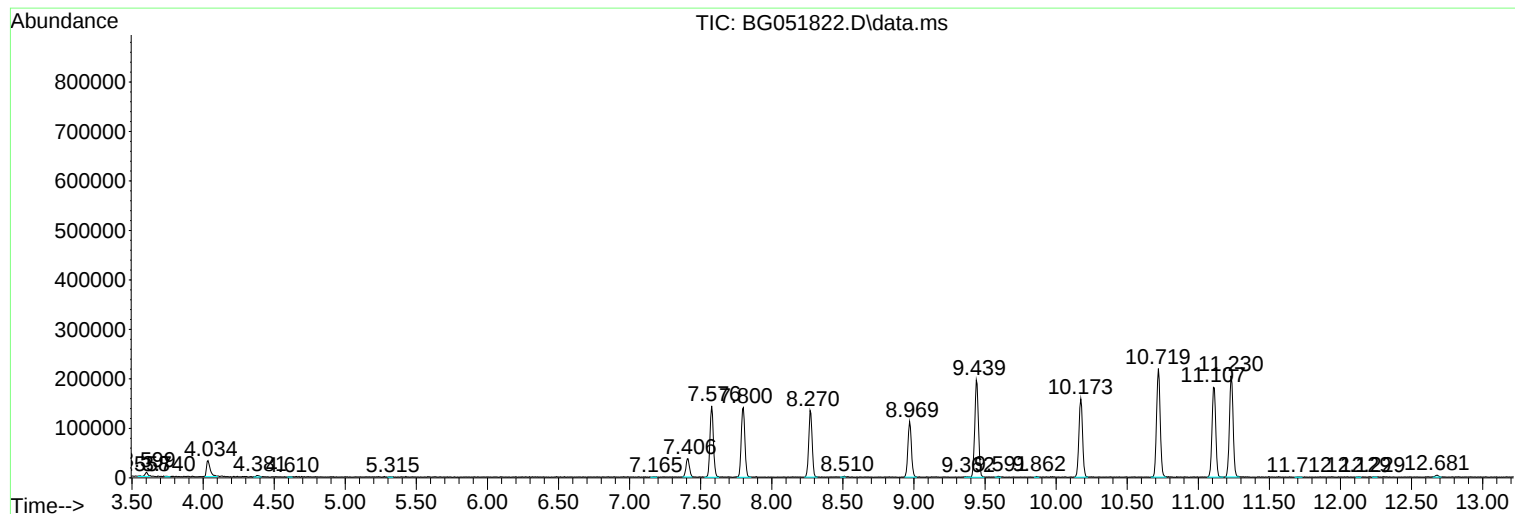

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
Data File : BG051822.D
Acq On : 28 Dec 2021 4:48
Operator : CG/JU
Sample : M5193-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0J32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
Data File : BG051822.D
Acq On : 28 Dec 2021 4:48
Operator : CG/JU
Sample : M5193-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0J32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc