

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
 Data File : BG051827.D
 Acq On : 28 Dec 2021 9:41
 Operator : CG/JU
 Sample : PB141643BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK643

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051827.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.517	4	5	7	rVB2	1844	1189	0.11%	0.011%
2	3.558	10	12	14	rVV2	1384	1203	0.11%	0.011%
3	3.605	14	20	28	rVB3	12162	21182	1.99%	0.191%
4	3.822	54	57	61	rVB4	1215	1951	0.18%	0.018%
5	3.869	63	65	68	rVB3	1066	1129	0.11%	0.010%
6	3.904	68	71	76	rBV5	1244	2295	0.22%	0.021%
7	4.034	88	93	109	rBV	144578	263522	24.74%	2.374%
8	4.139	109	111	115	rVV2	2053	2554	0.24%	0.023%
9	4.386	149	153	158	rVB4	3584	4965	0.47%	0.045%
10	4.545	179	180	184	rVB2	1144	1216	0.11%	0.011%
11	4.603	187	190	192	rVV3	856	1123	0.11%	0.010%
12	4.639	195	196	199	rBV3	1347	1600	0.15%	0.014%
13	5.015	259	260	263	rBV3	1301	1505	0.14%	0.014%
14	7.417	662	669	676	rBV	205357	352719	33.11%	3.178%
15	7.588	691	698	706	rBV	132470	224921	21.11%	2.026%
16	7.805	725	735	743	rBV	183934	317820	29.84%	2.863%
17	8.281	810	816	824	rBV	133445	220325	20.68%	1.985%
18	8.980	928	935	946	rBV	225427	396938	37.26%	3.576%
19	9.091	951	954	956	rBV	1112	1440	0.14%	0.013%
20	9.162	963	966	971	rVB2	1071	1170	0.11%	0.011%
21	9.450	1007	1015	1023	rBV	186633	335190	31.47%	3.020%
22	9.773	1065	1070	1072	rVB	983	1690	0.16%	0.015%
23	9.796	1072	1074	1077	rBV	1298	1631	0.15%	0.015%
24	10.184	1133	1140	1150	rVB	159284	284087	26.67%	2.559%
25	10.730	1226	1233	1241	rBV	228053	410935	38.58%	3.702%
26	10.783	1241	1242	1249	rVB3	1125	1232	0.12%	0.011%
27	11.118	1290	1299	1307	rBV	187671	330809	31.05%	2.980%
28	11.242	1311	1320	1336	rBV	204903	386663	36.30%	3.483%
29	11.935	1433	1438	1439	rBV2	737	1225	0.11%	0.011%
30	12.687	1562	1566	1571	rBV3	3928	5842	0.55%	0.053%
31	14.302	1835	1841	1849	rVV	395014	591508	55.53%	5.329%
32	14.613	1887	1894	1901	rVB	438266	715837	67.20%	6.449%
33	14.913	1938	1945	1957	rVB	286058	459502	43.14%	4.140%
34	15.083	1968	1974	1990	rBV	123836	242298	22.75%	2.183%
35	15.659	2070	2072	2075	rVB2	1138	1138	0.11%	0.010%
36	15.694	2075	2078	2080	rBV2	820	1133	0.11%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
 Data File : BG051827.D
 Acq On : 28 Dec 2021 9:41
 Operator : CG/JU
 Sample : PB141643BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK643

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	15.900	2107	2113	2122	rVB	562941	854654	80.23%	7.699%
38	16.006	2124	2131	2139	rBV	122881	193488	18.16%	1.743%
39	16.094	2145	2146	2149	rBV2	1274	1337	0.13%	0.012%
40	16.147	2151	2155	2159	rVV2	2963	3576	0.34%	0.032%
41	17.010	2300	2302	2305	rVB2	1506	1380	0.13%	0.012%
42	17.175	2329	2330	2335	rVB2	1024	1436	0.13%	0.013%
43	17.304	2349	2352	2355	rBV3	877	1228	0.12%	0.011%
44	17.451	2373	2377	2384	rVB3	2228	4781	0.45%	0.043%
45	17.521	2388	2389	2394	rVB3	862	1147	0.11%	0.010%
46	17.568	2394	2397	2400	rBV	882	1193	0.11%	0.011%
47	17.656	2406	2412	2421	rBV	356462	555256	52.12%	5.002%
48	17.756	2423	2429	2436	rVV2	585445	920068	86.37%	8.289%
49	18.073	2482	2483	2488	rVB2	1628	1953	0.18%	0.018%
50	18.138	2490	2494	2495	rBV2	1554	1412	0.13%	0.013%
51	18.226	2505	2509	2513	rBV4	1130	2020	0.19%	0.018%
52	18.273	2515	2517	2519	rVV3	1911	1204	0.11%	0.011%
53	18.338	2525	2528	2529	rVB3	1187	1175	0.11%	0.011%
54	18.432	2541	2544	2547	rVB2	1428	2064	0.19%	0.019%
55	18.567	2566	2567	2569	rBV	1394	1150	0.11%	0.010%
56	18.814	2607	2609	2612	rBV2	1223	1181	0.11%	0.011%
57	18.843	2612	2614	2620	rBV4	1359	2302	0.22%	0.021%
58	18.884	2620	2621	2624	rBV2	1442	1505	0.14%	0.014%
59	18.996	2637	2640	2643	rBV3	1604	2742	0.26%	0.025%
60	19.054	2648	2650	2653	rVB3	1384	1531	0.14%	0.014%
61	19.096	2653	2657	2659	rBV3	1795	2167	0.20%	0.020%
62	19.137	2662	2664	2668	rBV5	1083	1817	0.17%	0.016%
63	19.278	2687	2688	2690	rBV2	1893	1152	0.11%	0.010%
64	19.301	2690	2692	2695	rVV3	1463	1130	0.11%	0.010%
65	19.425	2712	2713	2714	rBV2	1712	1135	0.11%	0.010%
66	19.442	2714	2716	2719	rVB2	2444	1688	0.16%	0.015%
67	19.489	2723	2724	2728	rBV4	1900	2474	0.23%	0.022%
68	19.554	2732	2735	2736	rBV2	1560	1531	0.14%	0.014%
69	19.571	2736	2738	2739	rBV2	1364	1159	0.11%	0.010%
70	19.601	2739	2743	2748	rVB4	9730	13923	1.31%	0.125%
71	19.665	2751	2754	2759	rVV3	7645	10346	0.97%	0.093%
72	19.994	2807	2810	2811	rBV3	2503	1915	0.18%	0.017%
73	20.035	2811	2817	2825	rVV	728184	1065258	100.00%	9.597%
74	20.118	2830	2831	2833	rBV	2834	2124	0.20%	0.019%
75	20.335	2866	2868	2869	rBV2	2113	1636	0.15%	0.015%
76	20.388	2874	2877	2878	rBV3	3161	2901	0.27%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
 Data File : BG051827.D
 Acq On : 28 Dec 2021 9:41
 Operator : CG/JU
 Sample : PB141643BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK643

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	20.482	2891	2893	2894	rBV2	2296	1325	0.12%	0.012%
78	20.500	2894	2896	2897	rBV2	1919	1274	0.12%	0.011%
79	20.682	2922	2927	2928	rBV5	4965	7563	0.71%	0.068%
80	21.381	3045	3046	3047	rBV	4120	1539	0.14%	0.014%
81	21.980	3141	3148	3160	rBV	308992	542970	50.97%	4.892%
82	22.162	3176	3179	3180	rBV3	6004	5300	0.50%	0.048%
83	22.262	3195	3196	3197	rBV	3351	1353	0.13%	0.012%
84	23.595	3418	3423	3427	rVB7	10620	19711	1.85%	0.178%
85	24.183	3521	3523	3524	rBV2	4646	2880	0.27%	0.026%
86	24.471	3570	3572	3583	rVB9	15185	30500	2.86%	0.275%
87	24.717	3612	3614	3615	rBV2	4259	3391	0.32%	0.031%
88	25.240	3693	3703	3717	rBV2	227785	703103	66.00%	6.334%
89	25.481	3734	3744	3760	rBV2	120206	435756	40.91%	3.926%
90	26.797	3960	3968	3974	rBV9	12234	36892	3.46%	0.332%
91	27.373	4064	4066	4067	rVB2	5835	3781	0.35%	0.034%
92	27.402	4067	4071	4075	rBV7	6036	13897	1.30%	0.125%
93	27.602	4103	4105	4106	rBV2	3987	3608	0.34%	0.033%
94	28.254	4215	4216	4217	rBV	4429	1905	0.18%	0.017%
95	28.283	4219	4221	4222	rBV2	6315	4480	0.42%	0.040%
96	28.806	4308	4310	4311	rBV2	3596	1904	0.18%	0.017%
97	29.611	4445	4447	4450	rVB4	5982	3392	0.32%	0.031%
98	29.634	4450	4451	4454	rBV2	5693	4047	0.38%	0.036%
99	30.386	4577	4579	4581	rBV3	3935	2916	0.27%	0.026%
100	31.379	4746	4748	4751	rBV4	3826	3085	0.29%	0.028%




Sum of corrected areas: 11100198

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
Data File : BG051827.D
Acq On : 28 Dec 2021 9:41
Operator : CG/JU
Sample : PB141643BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK643

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

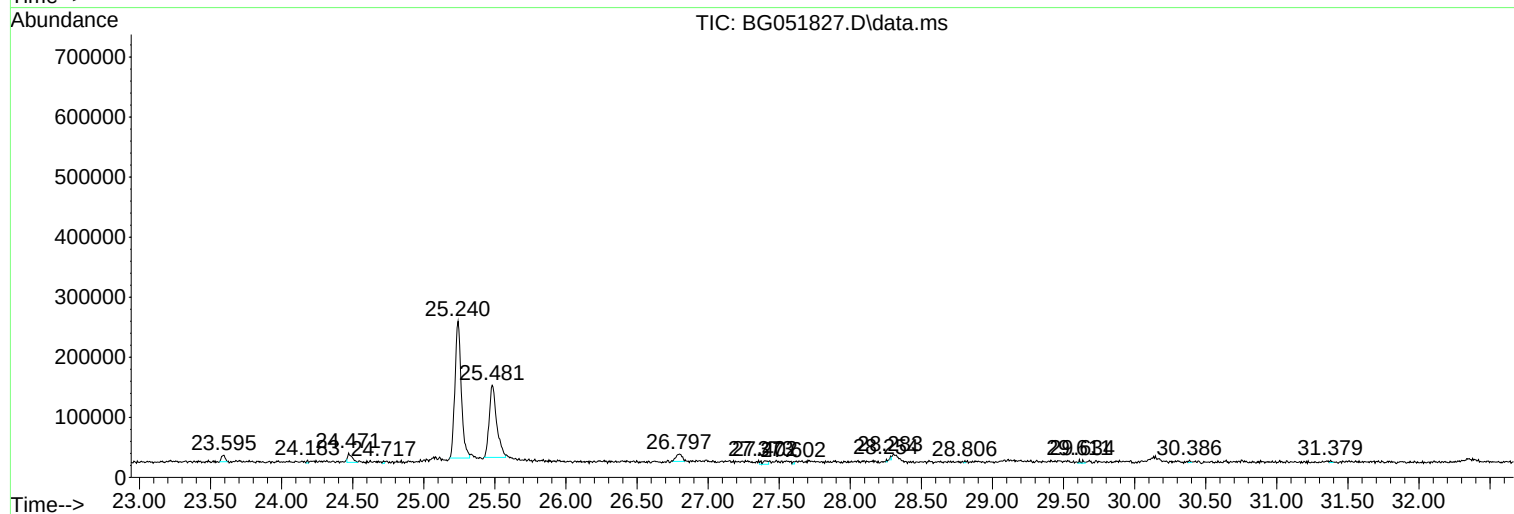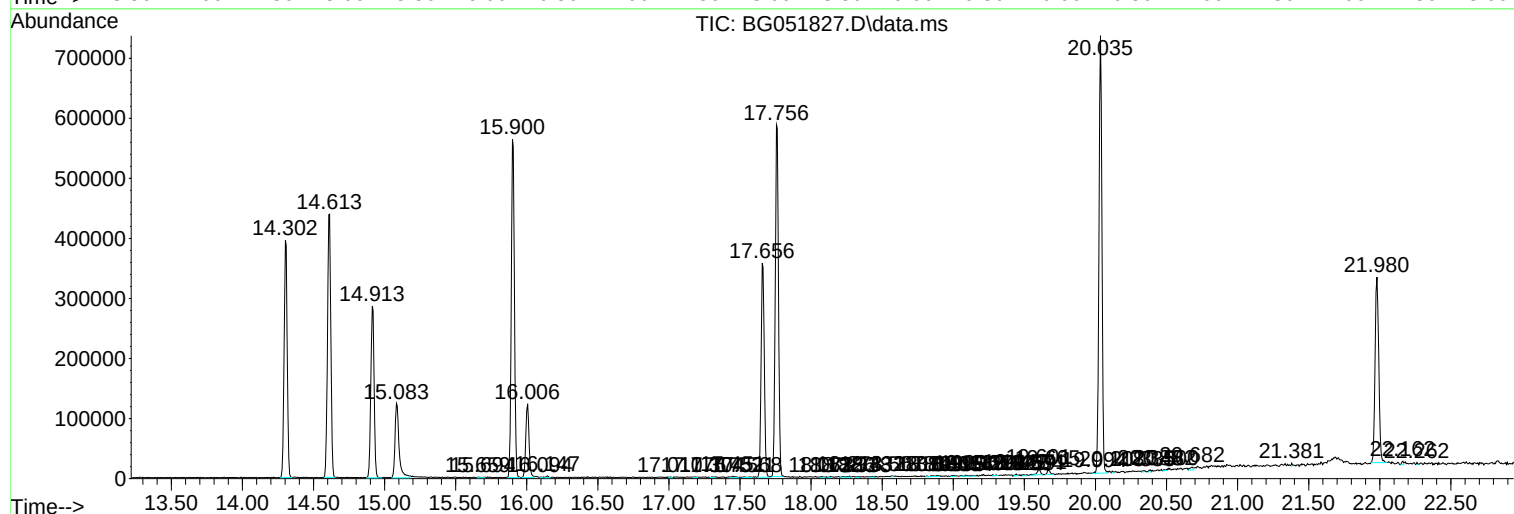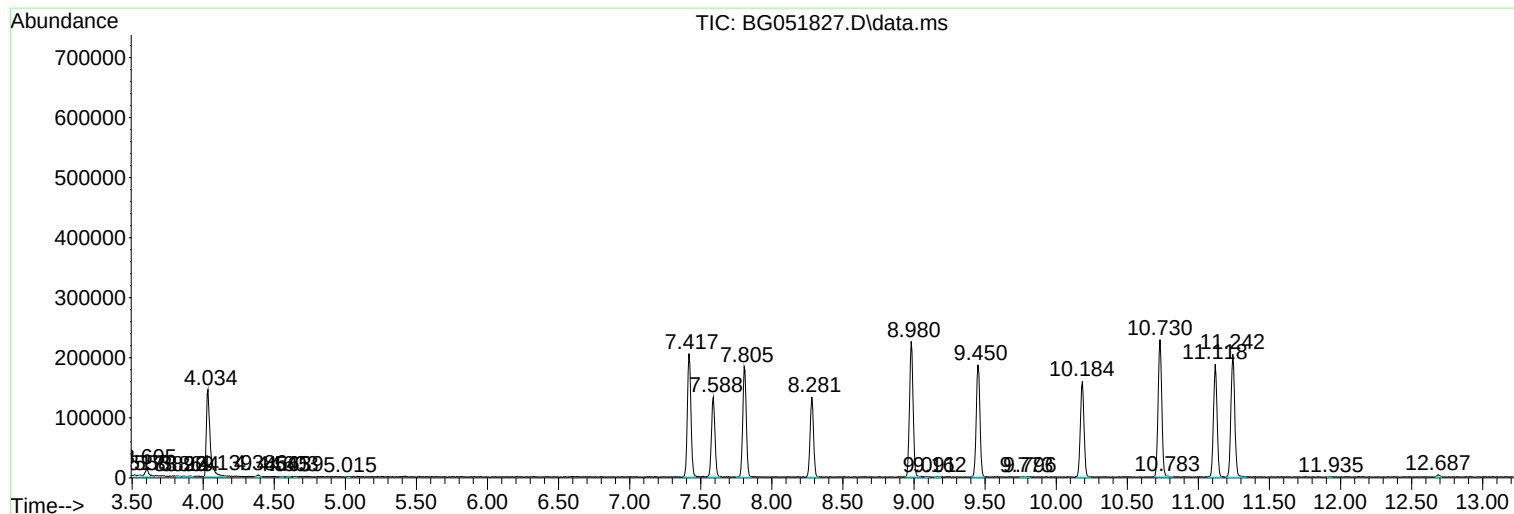

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
Data File : BG051827.D
Acq On : 28 Dec 2021 9:41
Operator : CG/JU
Sample : PB141643BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK643

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
Data File : BG051827.D
Acq On : 28 Dec 2021 9:41
Operator : CG/JU
Sample : PB141643BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK643

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc