

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
 Data File : BG051835.D
 Acq On : 28 Dec 2021 18:49
 Operator : CG/JU
 Sample : PB141700BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK700

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051835.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.602	14	19	26	rVB2	9243	15447	1.53%	0.151%
2	3.726	39	40	43	rVB3	1587	1244	0.12%	0.012%
3	3.879	63	66	69	rVB2	998	1479	0.15%	0.014%
4	4.031	87	92	107	rBV	127939	237883	23.60%	2.326%
5	4.290	133	136	143	rVB4	962	2036	0.20%	0.020%
6	4.384	149	152	155	rVB3	1734	2489	0.25%	0.024%
7	4.666	198	200	204	rBV3	924	1243	0.12%	0.012%
8	4.707	204	207	210	rVB3	974	1313	0.13%	0.013%
9	5.118	275	277	280	rBV2	1312	1236	0.12%	0.012%
10	5.142	280	281	284	rVB	1422	1186	0.12%	0.012%
11	5.183	284	288	289	rBV3	835	1209	0.12%	0.012%
12	5.629	361	364	366	rBV	1868	1931	0.19%	0.019%
13	5.964	419	421	425	rBV	1067	1326	0.13%	0.013%
14	6.076	437	440	444	rBV2	931	1407	0.14%	0.014%
15	6.481	506	509	514	rVB2	867	1270	0.13%	0.012%
16	6.516	514	515	520	rBV2	696	1166	0.12%	0.011%
17	6.798	561	563	566	rBV	1321	1174	0.12%	0.011%
18	7.109	611	616	619	rBV2	746	1689	0.17%	0.017%
19	7.409	657	667	677	rBV	185013	331971	32.93%	3.245%
20	7.579	688	696	704	rBV	120860	206543	20.49%	2.019%
21	7.797	726	733	743	rBV	168100	294685	29.23%	2.881%
22	8.273	807	814	822	rVB2	123485	200183	19.86%	1.957%
23	8.484	847	850	855	rBV2	785	1177	0.12%	0.012%
24	8.972	925	933	945	rVV	215764	386481	38.34%	3.778%
25	9.442	1005	1013	1023	rVB	175245	315722	31.32%	3.087%
26	10.176	1130	1138	1148	rVB	145864	270302	26.81%	2.643%
27	10.464	1186	1187	1191	rBV	947	1167	0.12%	0.011%
28	10.722	1223	1231	1243	rBV	211302	396101	39.29%	3.872%
29	11.110	1289	1297	1305	rBV	163381	303071	30.06%	2.963%
30	11.233	1310	1318	1329	rBV	196677	371651	36.87%	3.633%
31	12.678	1560	1564	1570	rBV3	3143	5341	0.53%	0.052%
32	13.330	1672	1675	1679	rBV	1146	1333	0.13%	0.013%
33	13.424	1689	1691	1694	rBV2	1271	1165	0.12%	0.011%
34	14.206	1821	1824	1827	rVB2	1072	1495	0.15%	0.015%
35	14.294	1833	1839	1848	rBV	379335	570438	56.59%	5.577%
36	14.505	1870	1875	1877	rBV2	1043	1670	0.17%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
 Data File : BG051835.D
 Acq On : 28 Dec 2021 18:49
 Operator : CG/JU
 Sample : PB141700BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK700

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	14.605	1885	1892	1901	rVB	425822	688188	68.27%	6.728%
38	14.817	1923	1928	1930	rBV2	938	1292	0.13%	0.013%
39	14.905	1936	1943	1950	rBV	276293	433304	42.98%	4.236%
40	15.081	1967	1973	1990	rBV2	104702	215170	21.34%	2.104%
41	15.216	1995	1996	1999	rVV3	1848	1698	0.17%	0.017%
42	15.410	2027	2029	2033	rBV2	917	1206	0.12%	0.012%
43	15.710	2079	2080	2083	rBV	1300	1233	0.12%	0.012%
44	15.798	2092	2095	2098	rBV2	992	1404	0.14%	0.014%
45	15.898	2103	2112	2120	rBV	532263	833973	82.73%	8.153%
46	15.997	2123	2129	2137	rBV2	111067	170684	16.93%	1.669%
47	16.133	2148	2152	2158	rVB6	2132	3708	0.37%	0.036%
48	16.274	2173	2176	2179	rVB2	1288	1460	0.14%	0.014%
49	16.467	2207	2209	2211	rBV2	1069	1174	0.12%	0.011%
50	16.497	2212	2214	2218	rVB	1129	1573	0.16%	0.015%
51	16.673	2240	2244	2245	rBV3	1334	1377	0.14%	0.013%
52	16.984	2293	2297	2298	rBV2	1077	1461	0.14%	0.014%
53	17.114	2318	2319	2323	rVB2	1423	1257	0.12%	0.012%
54	17.149	2323	2325	2328	rBV2	1502	1809	0.18%	0.018%
55	17.284	2346	2348	2351	rBV3	1363	1200	0.12%	0.012%
56	17.349	2357	2359	2363	rVB2	1028	1471	0.15%	0.014%
57	17.384	2363	2365	2368	rBV2	820	1199	0.12%	0.012%
58	17.437	2371	2374	2377	rBV2	2394	3157	0.31%	0.031%
59	17.554	2392	2394	2399	rBV	1260	1509	0.15%	0.015%
60	17.654	2404	2411	2419	rBV	349443	520654	51.65%	5.090%
61	17.754	2421	2428	2437	rBV	577175	892171	88.50%	8.722%
62	17.912	2451	2455	2456	rBV2	1658	1531	0.15%	0.015%
63	17.930	2456	2458	2461	rVB4	2252	1832	0.18%	0.018%
64	17.977	2464	2466	2471	rBV3	861	1259	0.12%	0.012%
65	18.018	2471	2473	2479	rVB4	1746	2800	0.28%	0.027%
66	18.071	2479	2482	2484	rBV	1501	1318	0.13%	0.013%
67	18.153	2495	2496	2500	rVB3	1426	1566	0.16%	0.015%
68	18.194	2500	2503	2506	rBV4	1801	2011	0.20%	0.020%
69	18.241	2509	2511	2515	rVB3	1155	1391	0.14%	0.014%
70	18.306	2520	2522	2524	rBV2	1124	1284	0.13%	0.013%
71	18.400	2535	2538	2540	rBV4	1101	1319	0.13%	0.013%
72	18.582	2565	2569	2570	rBV2	1170	1518	0.15%	0.015%
73	18.647	2579	2580	2582	rBV	2220	2045	0.20%	0.020%
74	18.706	2588	2590	2592	rBV2	1738	1618	0.16%	0.016%
75	18.735	2594	2595	2597	rVV	1703	1354	0.13%	0.013%
76	18.776	2600	2602	2605	rVV3	1307	1350	0.13%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
 Data File : BG051835.D
 Acq On : 28 Dec 2021 18:49
 Operator : CG/JU
 Sample : PB141700BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK700

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	18.893	2619	2622	2624	rBV2	1366	1429	0.14%	0.014%
78	18.982	2636	2637	2641	rVB3	1695	1180	0.12%	0.012%
79	19.093	2655	2656	2659	rVB2	2021	1583	0.16%	0.015%
80	19.117	2659	2660	2663	rBV3	3351	2565	0.25%	0.025%
81	19.205	2672	2675	2676	rBV3	2703	2229	0.22%	0.022%
82	19.358	2699	2701	2703	rVB2	2098	1510	0.15%	0.015%
83	19.381	2703	2705	2706	rBV2	2945	1799	0.18%	0.018%
84	19.428	2711	2713	2715	rVV3	2354	2309	0.23%	0.023%
85	19.598	2737	2742	2746	rBV7	9753	14759	1.46%	0.144%
86	19.669	2749	2754	2760	rBV3	8243	13889	1.38%	0.136%
87	19.734	2763	2765	2766	rBV2	1839	1283	0.13%	0.013%
88	19.845	2781	2784	2785	rBV3	3561	2488	0.25%	0.024%
89	19.886	2789	2791	2793	rBV3	2760	2588	0.26%	0.025%
90	20.027	2808	2815	2826	rBV	707063	1008076	100.00%	9.855%
91	21.972	3139	3146	3156	rBV	263967	479708	47.59%	4.690%
92	23.323	3374	3376	3379	rBV4	6075	5004	0.50%	0.049%
93	25.226	3690	3700	3711	rBV2	168609	574201	56.96%	5.613%
94	25.467	3733	3741	3756	rBV2	90062	337327	33.46%	3.298%
95	26.859	3976	3978	3980	rBV3	6819	6679	0.66%	0.065%
96	27.593	4101	4103	4104	rBV2	6634	4190	0.42%	0.041%
97	27.864	4147	4149	4151	rBV2	7892	6774	0.67%	0.066%
98	29.655	4452	4454	4456	rBV3	5651	3861	0.38%	0.038%
99	31.065	4692	4694	4695	rBV2	6145	3597	0.36%	0.035%
100	32.281	4899	4901	4902	rBV2	6388	5230	0.52%	0.051%




Sum of corrected areas: 10229010

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
Data File : BG051835.D
Acq On : 28 Dec 2021 18:49
Operator : CG/JU
Sample : PB141700BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK700

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

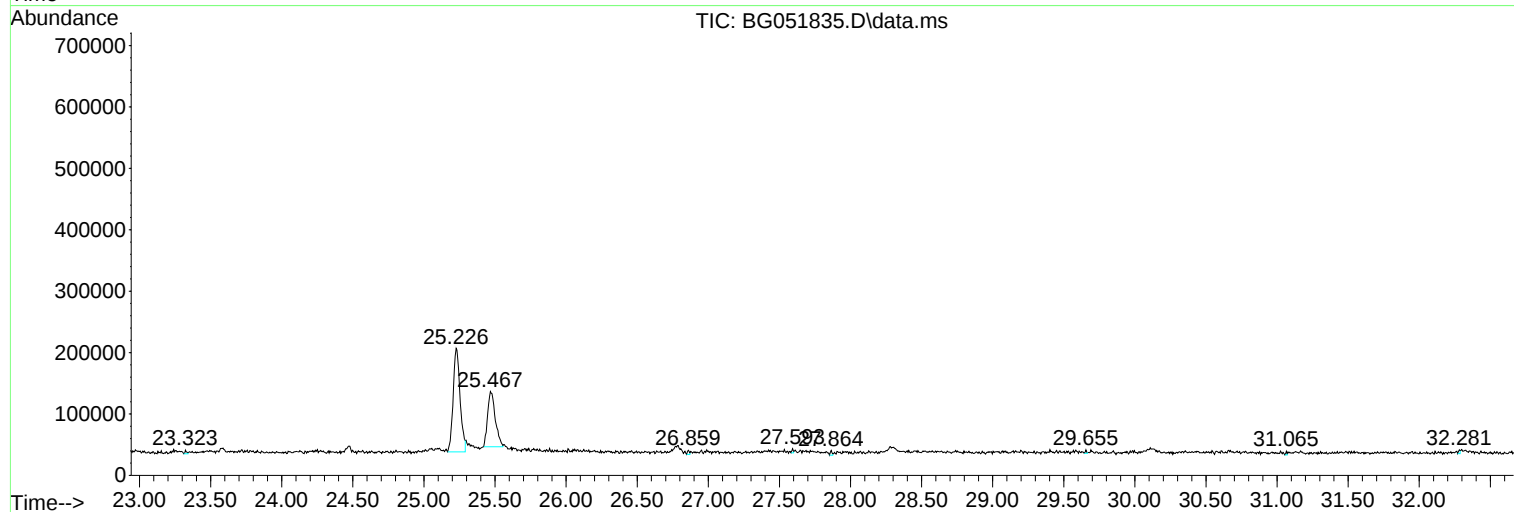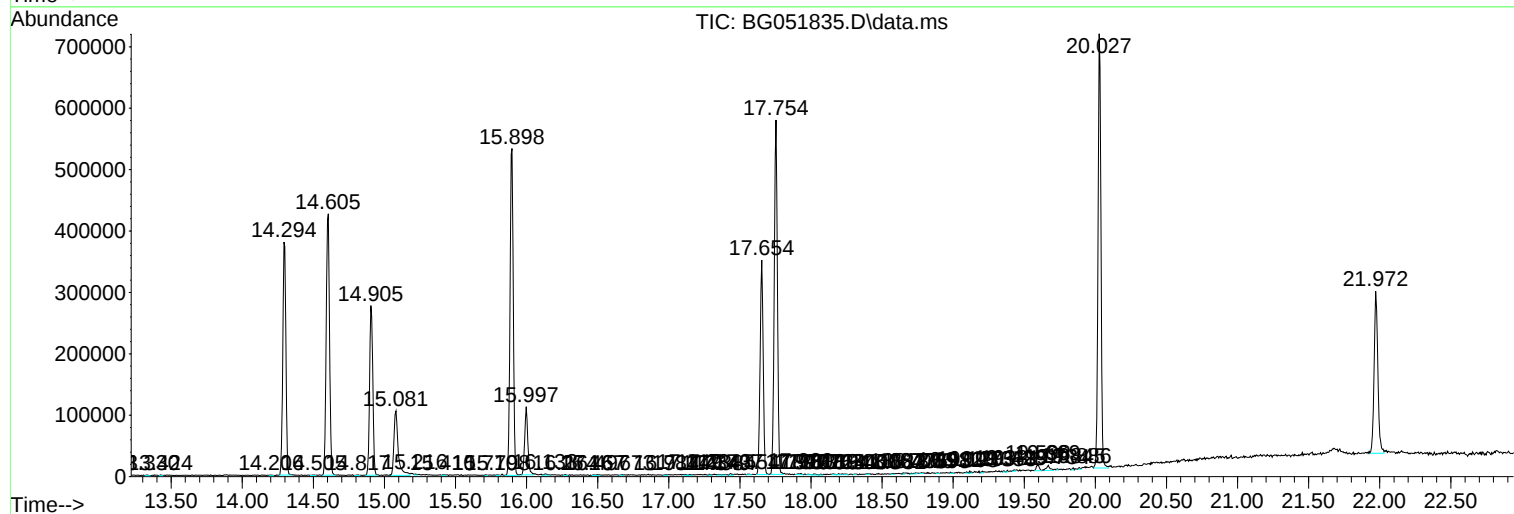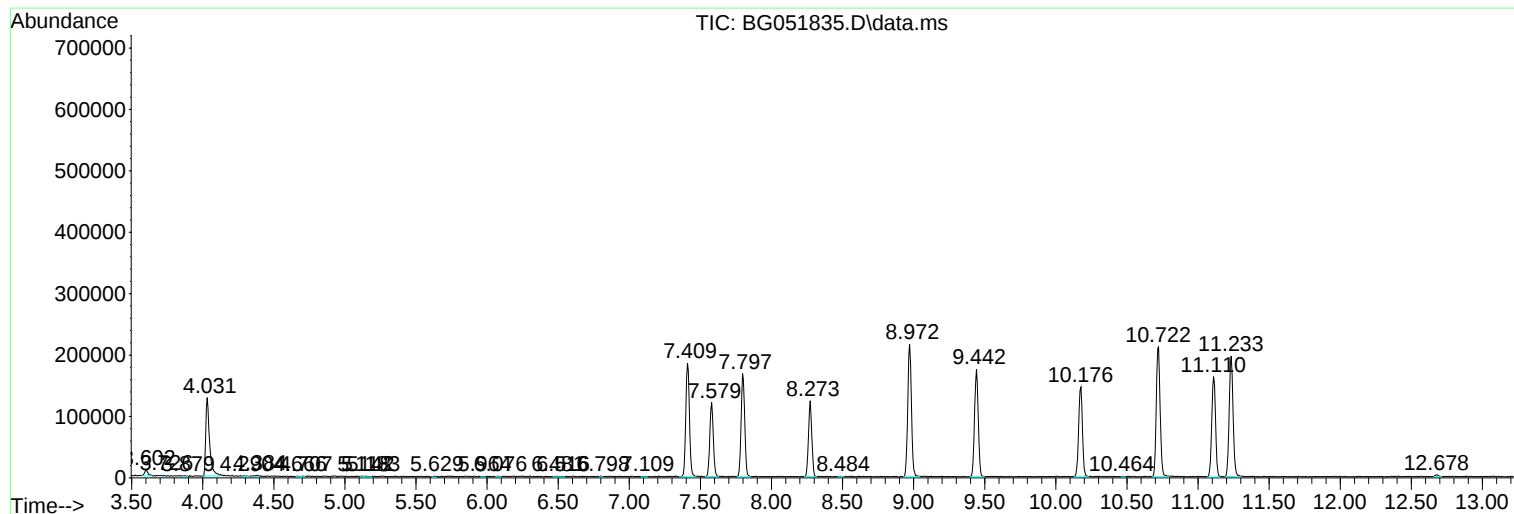

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
Data File : BG051835.D
Acq On : 28 Dec 2021 18:49
Operator : CG/JU
Sample : PB141700BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK700

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122721\
Data File : BG051835.D
Acq On : 28 Dec 2021 18:49
Operator : CG/JU
Sample : PB141700BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK700

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc