


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG122818\
 Data File : BG038875.D
 Acq On : 28 Dec 2018 15:41
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

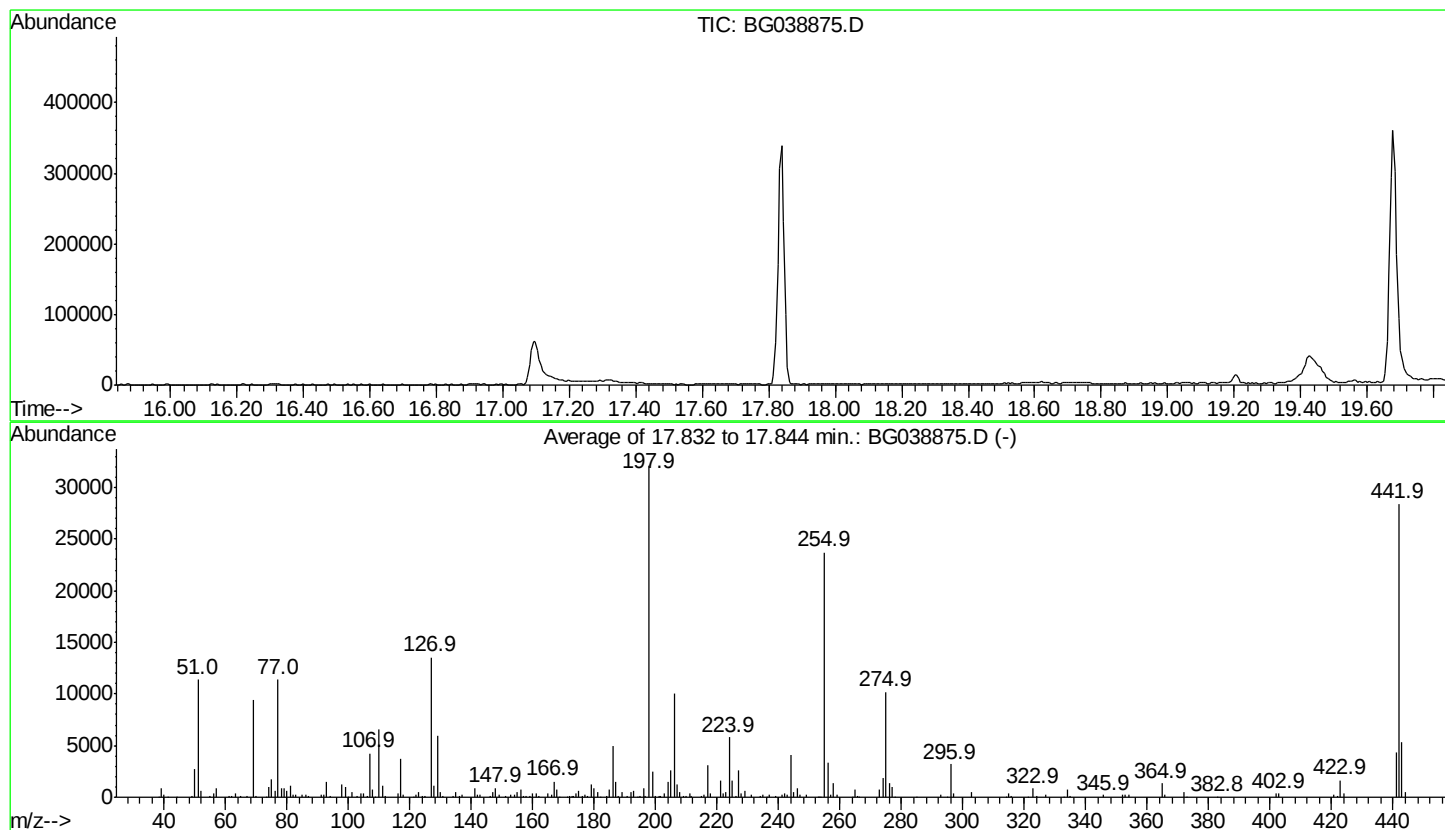

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	11394	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.5	9471	PASS
70	69	0.00	2	1.1	104	PASS
127	198	10	80	42.1	13529	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	32106	PASS
199	198	5	9	7.6	2433	PASS
275	198	10	60	31.8	10196	PASS
365	198	1	100	4.1	1325	PASS
441	198	0.01	100	13.6	4369	PASS
442	198	50	100	88.5	28405	PASS
443	442	15	24	18.8	5342	PASS