
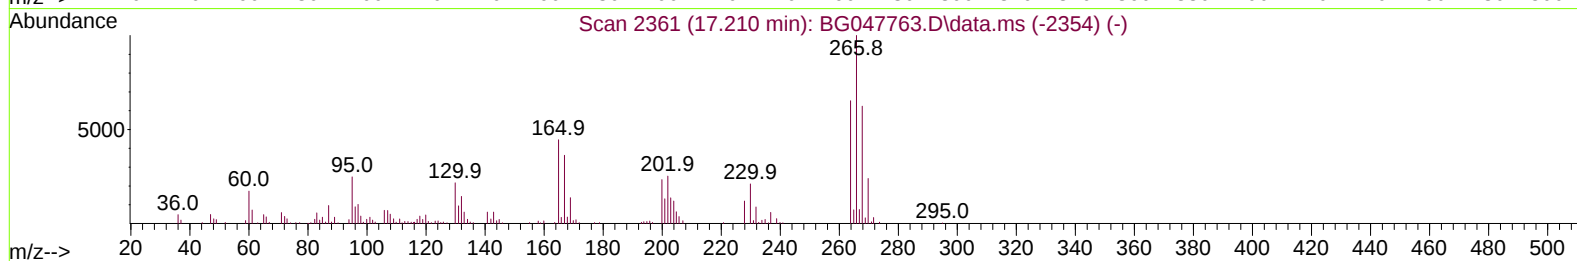
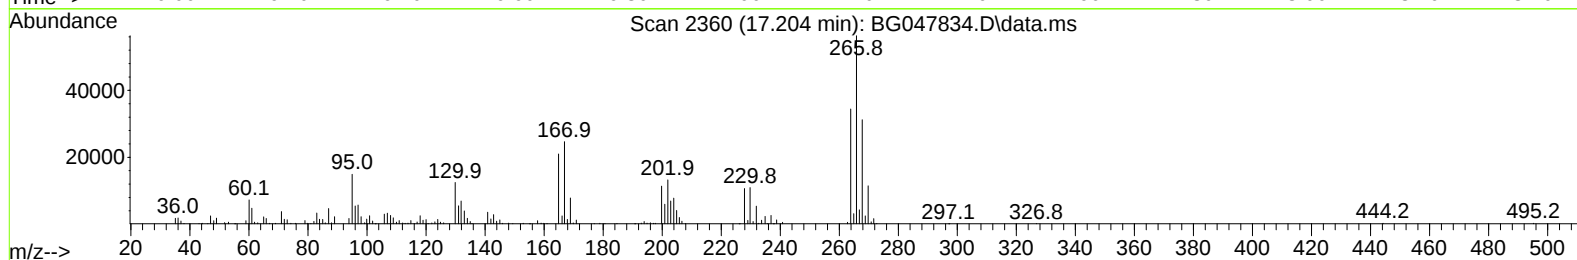


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122920\
Data File : BG047834.D
Acq On : 29 Dec 2020 13:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 01:05:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 17 15:55:16 2020
Response via : Initial Calibration

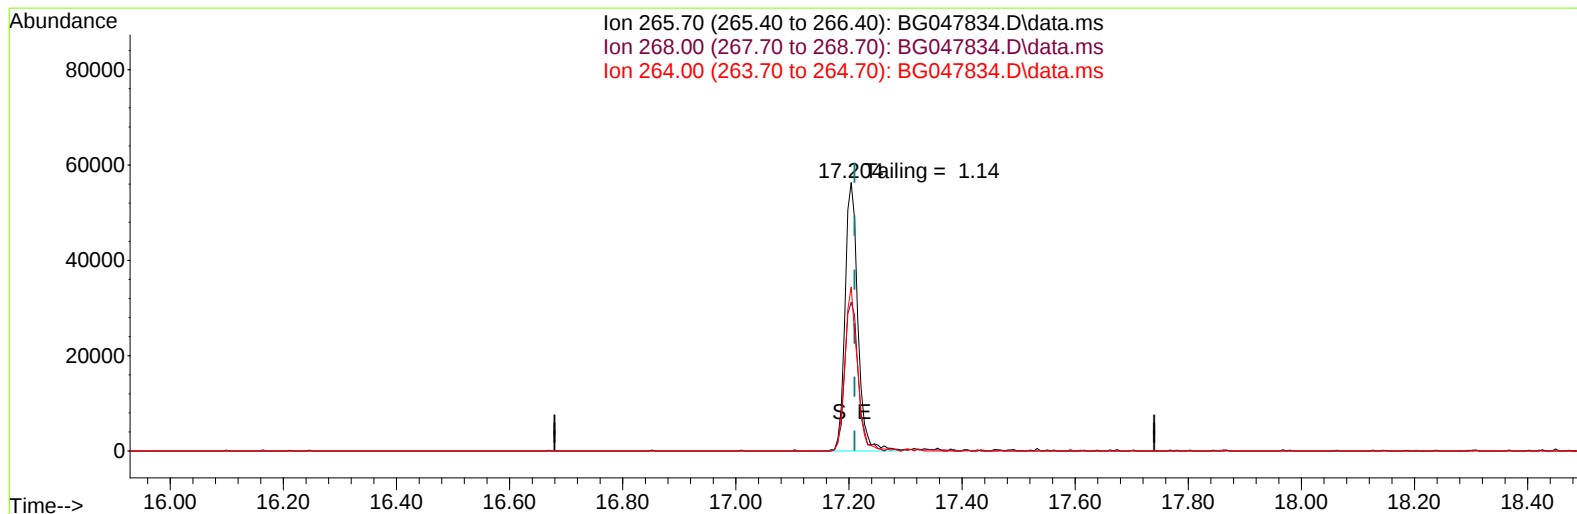

TIC: BG047834.D\data.ms

(70) Pentachlorophenol (C)




17.204min (-0.006) 3633.96 ng

response 88898

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	55.41
264.00	61.60	61.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122920\
Data File : BG047834.D
Acq On : 29 Dec 2020 13:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 01:05:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 17 15:55:16 2020
Response via : Initial Calibration

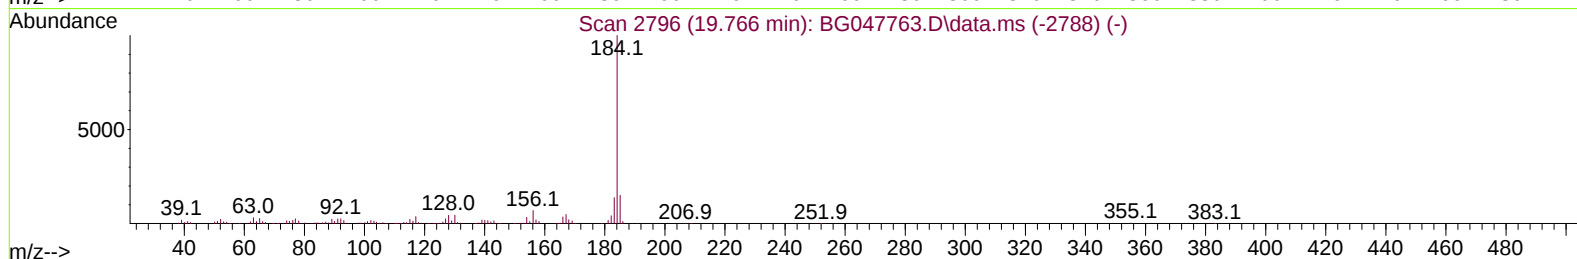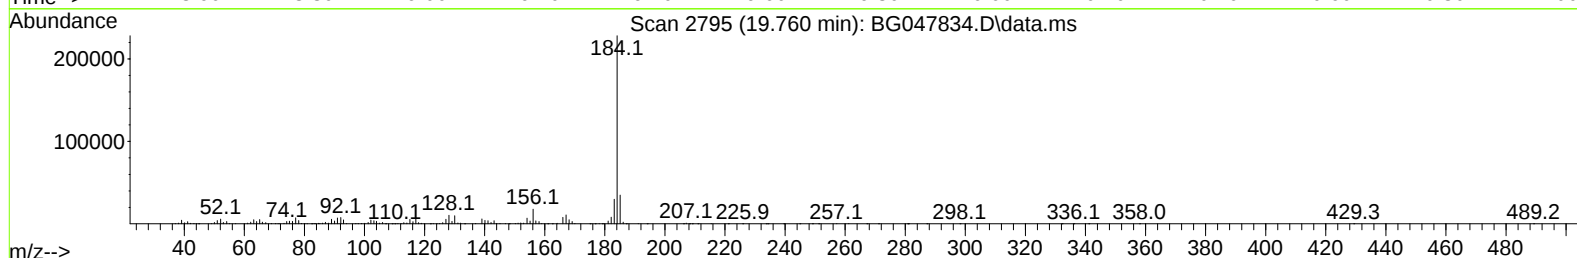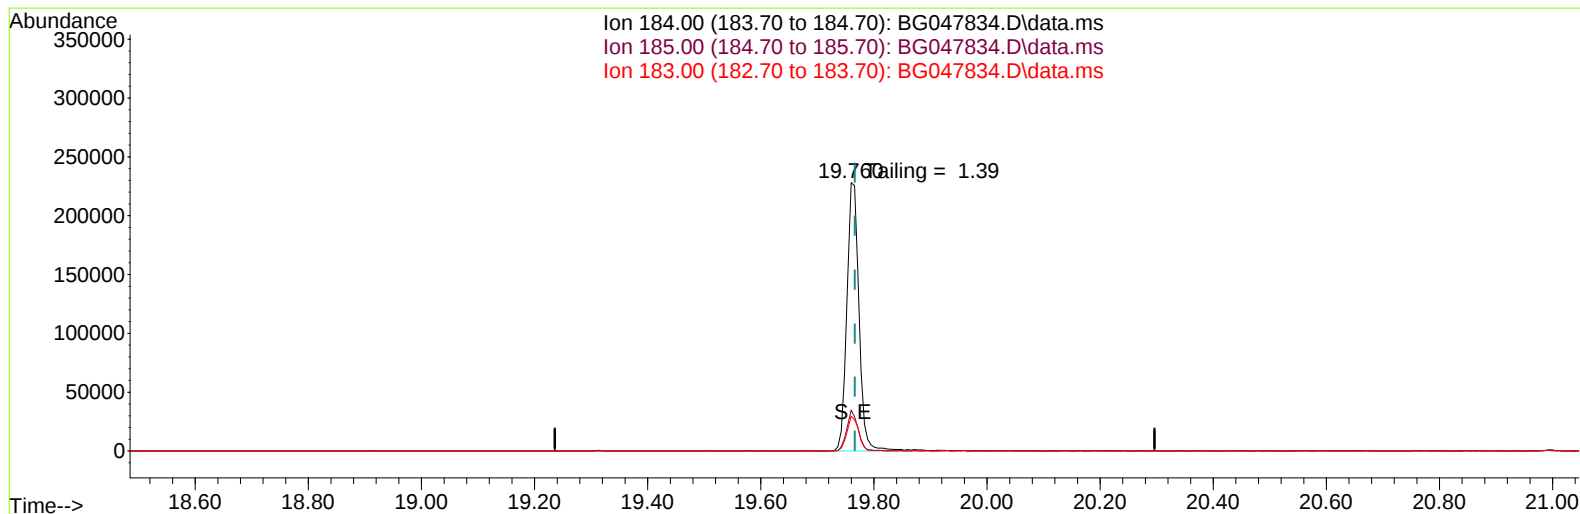

TIC: BG047834.D\data.ms

(77) Benzidine**19.760min (-0.006) 70188.49 ng****response 334086**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.26
183.00	13.20	13.04
0.00	0.00	0.00