
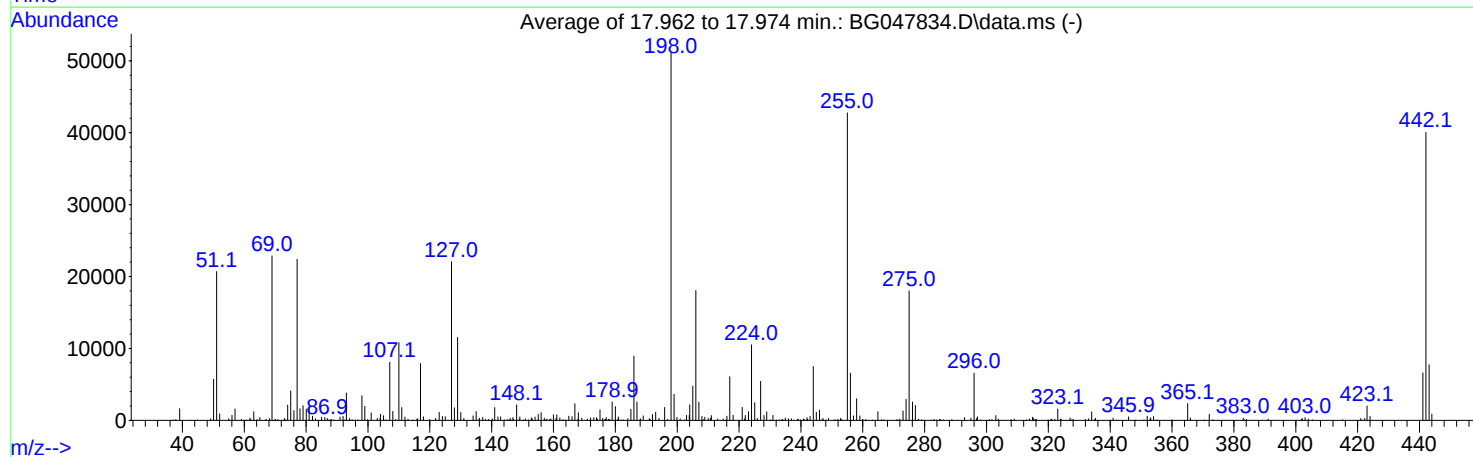


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122920\
 Data File : BG047834.D
 Acq On : 29 Dec 2020 13:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 17 15:55:16 2020

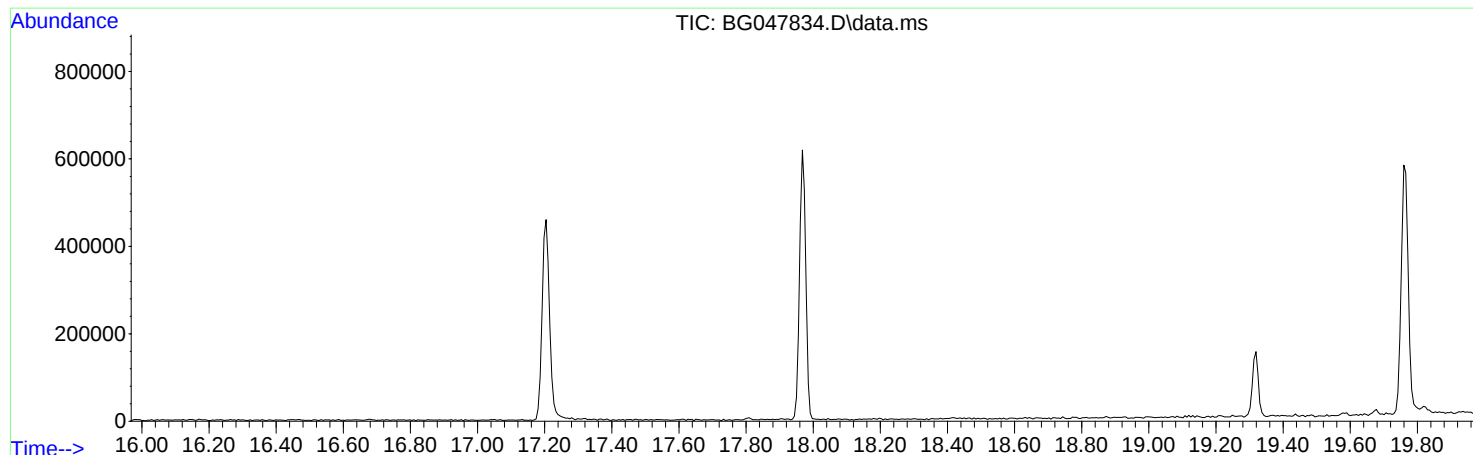

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	20696	PASS
68	69	0.00	2	1.1	251	PASS
69	198	0.00	100	44.7	22880	PASS
70	69	0.00	2	0.6	131	PASS
127	198	10	80	43.1	22040	PASS
197	198	0.00	2	0.3	132	PASS
198	198	100	100	100.0	51149	PASS
199	198	5	9	7.1	3632	PASS
275	198	10	60	35.2	17994	PASS
365	198	1	100	4.6	2329	PASS
441	198	0.01	100	12.9	6608	PASS
442	198	50	100	78.3	40072	PASS
443	442	15	24	19.3	7739	PASS