
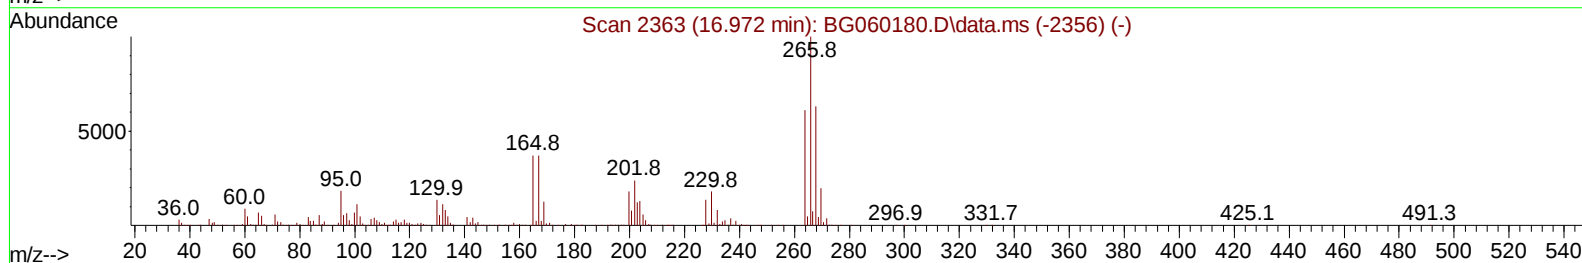
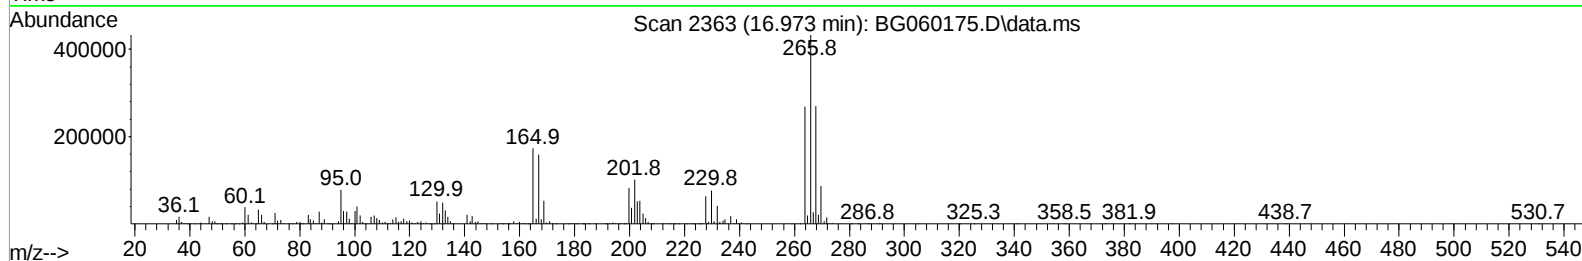


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122923\
Data File : BG060175.D
Acq On : 29 Dec 2023 11:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 11:59:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 29 11:57:19 2023
Response via : Initial Calibration

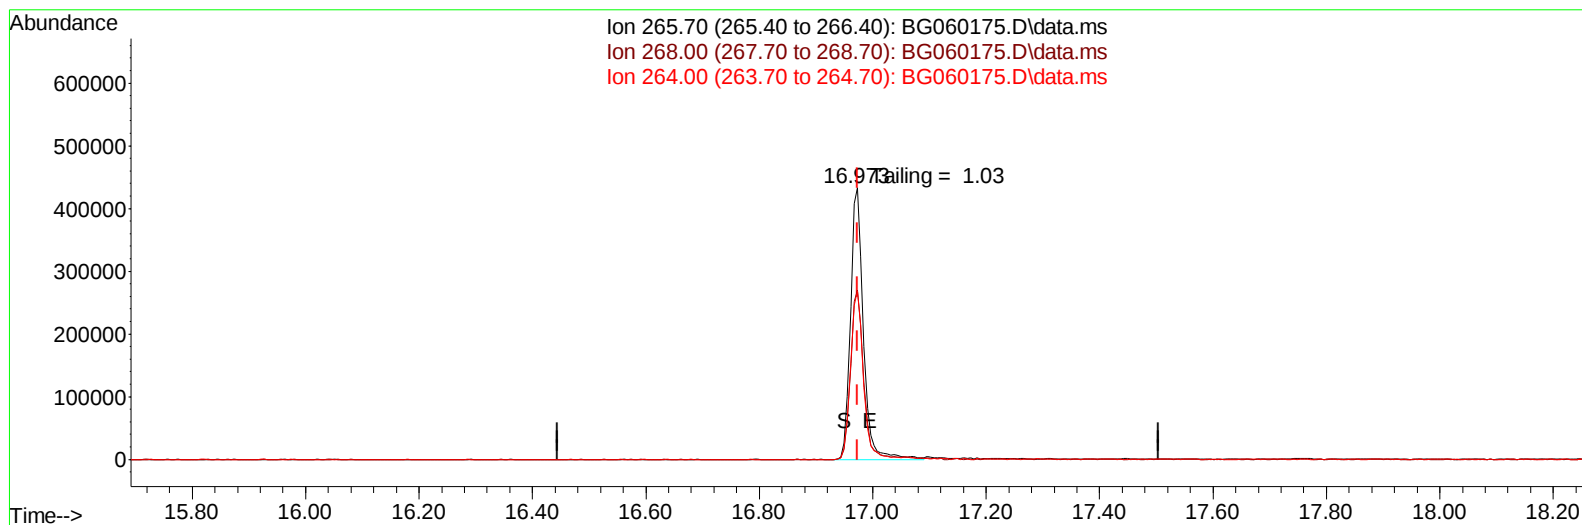

TIC: BG060175.D\data.ms

(70) Pentachlorophenol (C)




16.973min (-0.001) 493823.43 ng

response 680900

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.30	66.93
264.00	67.10	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122923\
Data File : BG060175.D
Acq On : 29 Dec 2023 11:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 11:59:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 29 11:57:19 2023
Response via : Initial Calibration

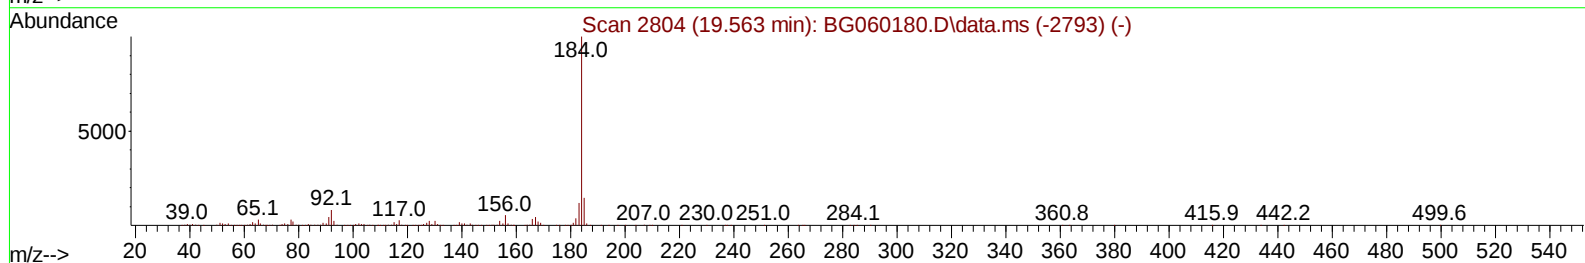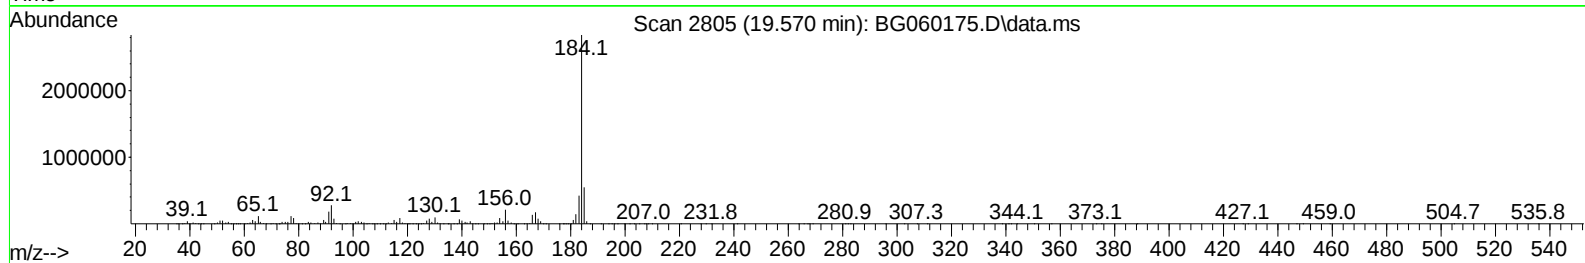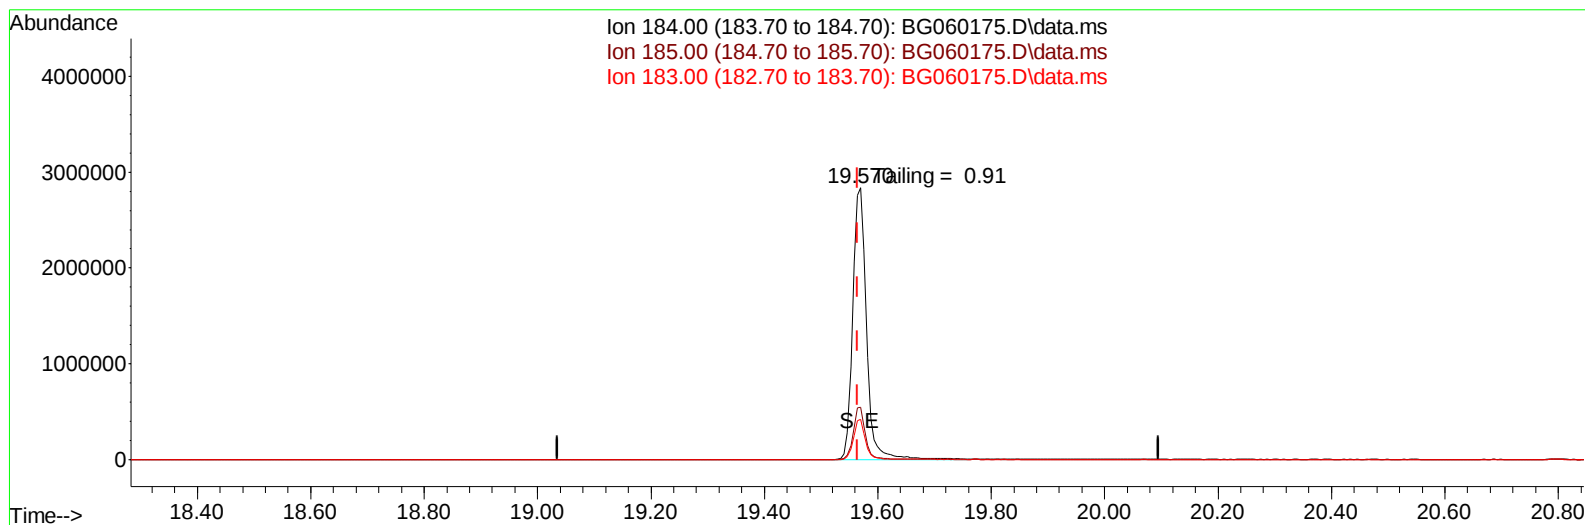

TIC: BG060175.D\data.ms

(77) Benzidine**19.570min (+ 0.005) 2310367.26 ng****response 4804552**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	19.33#
183.00	10.80	14.81#
0.00	0.00	0.00