

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122923\  
 Data File : BG060185.D  
 Acq On : 29 Dec 2023 18:00  
 Operator : MA/JU  
 Sample : PB158041BL  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB158041BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122923.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG060185.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.514       | 406           | 413         | 428          | rBV      | 5821652        | 9425468       | 40.09%          | 10.049%       |
| 2         | 7.107       | 675           | 684         | 699          | rBV      | 5137004        | 9158216       | 38.95%          | 9.764%        |
| 3         | 7.941       | 819           | 826         | 838          | rBV      | 704355         | 1261473       | 5.37%           | 1.345%        |
| 4         | 9.104       | 1016          | 1024        | 1038         | rBV      | 3023909        | 5476929       | 23.30%          | 5.839%        |
| 5         | 10.744      | 1294          | 1303        | 1315         | rBV      | 1038245        | 1912550       | 8.14%           | 2.039%        |
| 6         | 13.199      | 1712          | 1721        | 1736         | rBV      | 8954088        | 13997925      | 59.54%          | 14.923%       |
| 7         | 14.574      | 1948          | 1955        | 1968         | rBV      | 2054323        | 3158497       | 13.43%          | 3.367%        |
| 8         | 16.067      | 2201          | 2209        | 2227         | rBV      | 6972695        | 10876585      | 46.26%          | 11.596%       |
| 9         | 17.324      | 2414          | 2423        | 2436         | rBV      | 2983381        | 4505506       | 19.16%          | 4.803%        |
| 10        | 19.945      | 2862          | 2869        | 2885         | rBV      | 16498199       | 23509856      | 100.00%         | 25.064%       |
| 11        | 21.590      | 3141          | 3149        | 3162         | rBV      | 3108189        | 5125779       | 21.80%          | 5.465%        |
| 12        | 24.762      | 3679          | 3689        | 3708         | rBV2     | 1825396        | 5390686       | 22.93%          | 5.747%        |




Sum of corrected areas: 93799470

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122923\  
Data File : BG060185.D  
Acq On : 29 Dec 2023 18:00  
Operator : MA/JU  
Sample : PB158041BL  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB158041BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122923.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

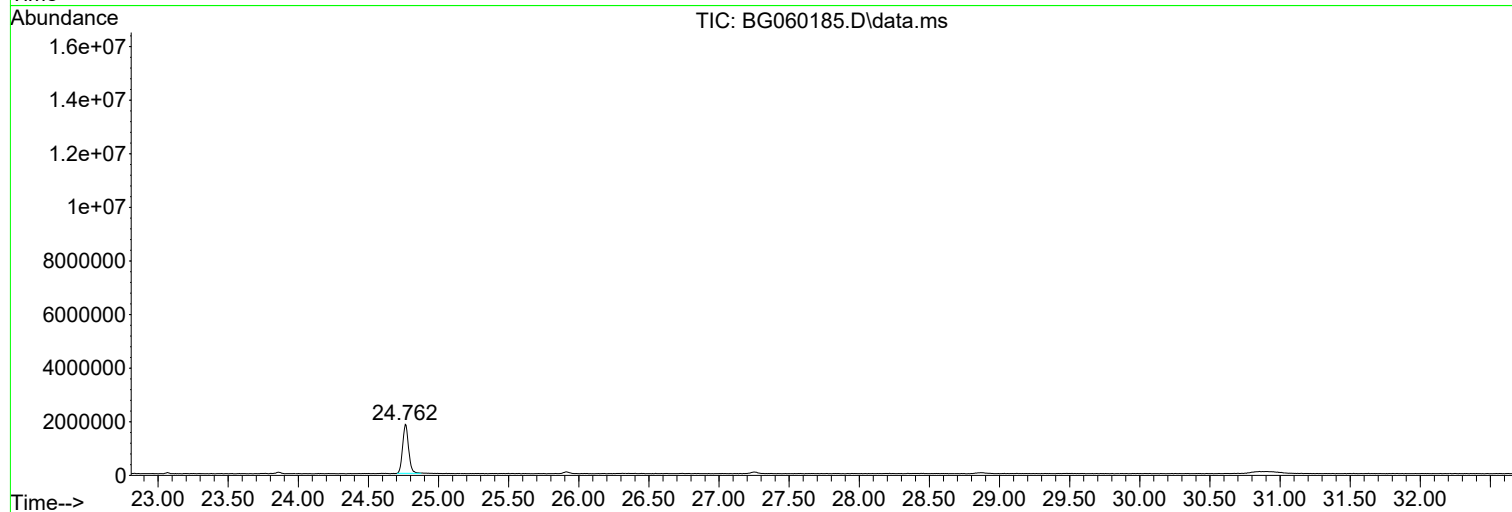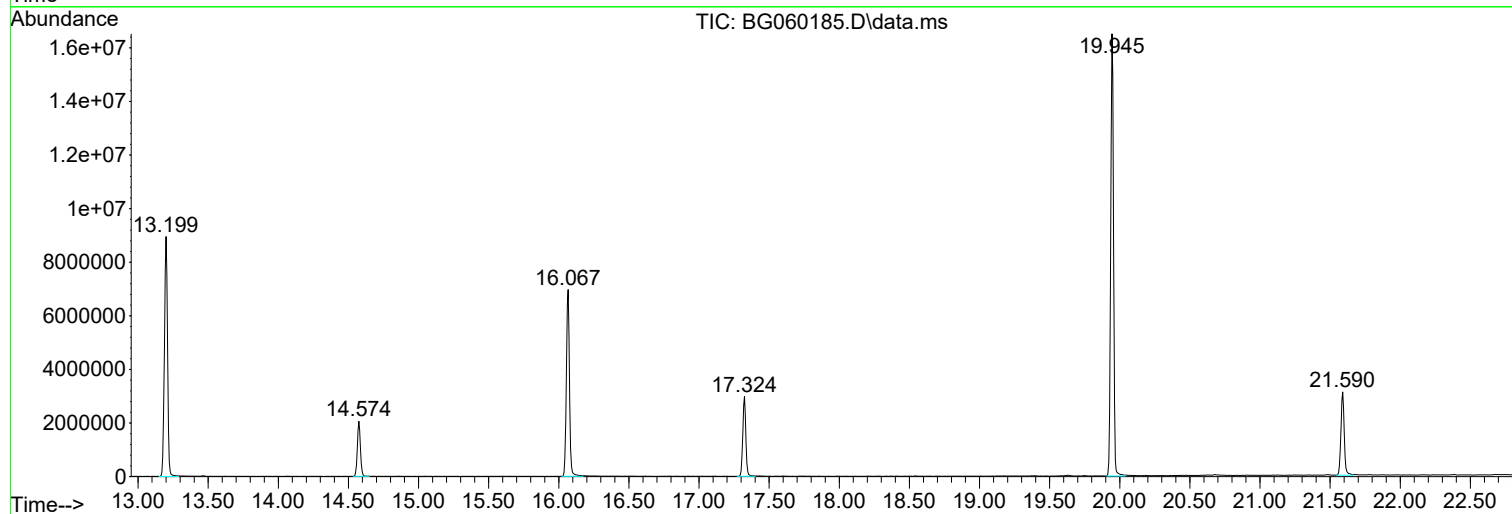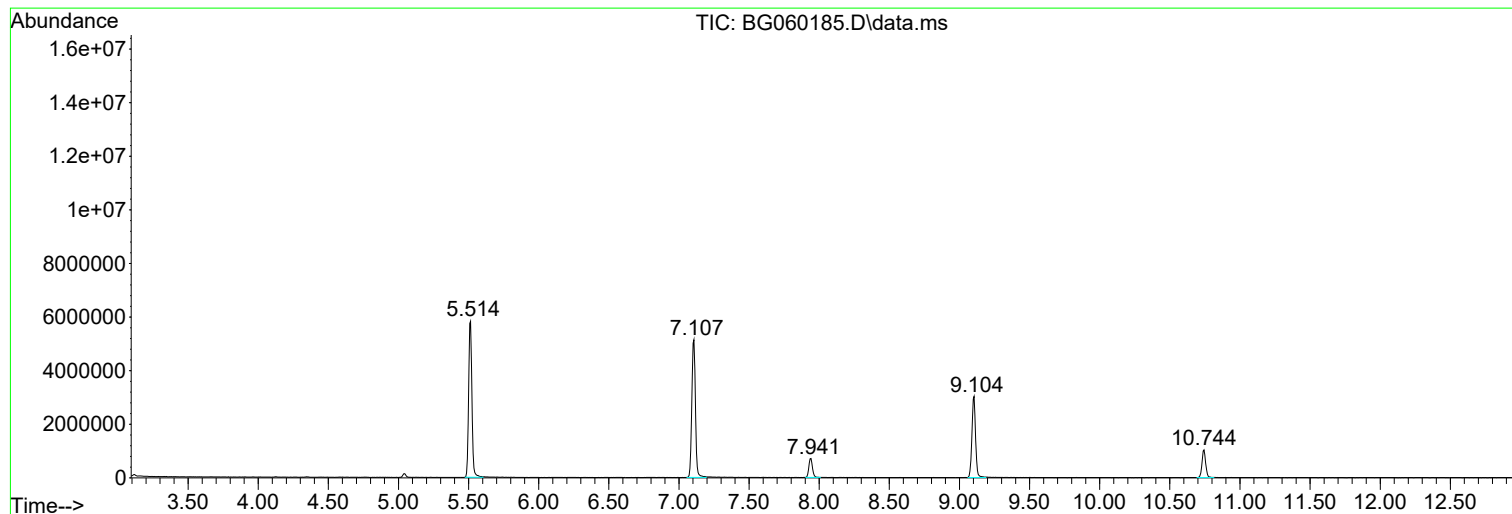

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122923\  
Data File : BG060185.D  
Acq On : 29 Dec 2023 18:00  
Operator : MA/JU  
Sample : PB158041BL  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB158041BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122923.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122923\  
Data File : BG060185.D  
Acq On : 29 Dec 2023 18:00  
Operator : MA/JU  
Sample : PB158041BL  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB158041BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122923.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|