


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122923\
Data File : BG060175.D
Acq On : 29 Dec 2023 11:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Dec 30 03:14:04 2023

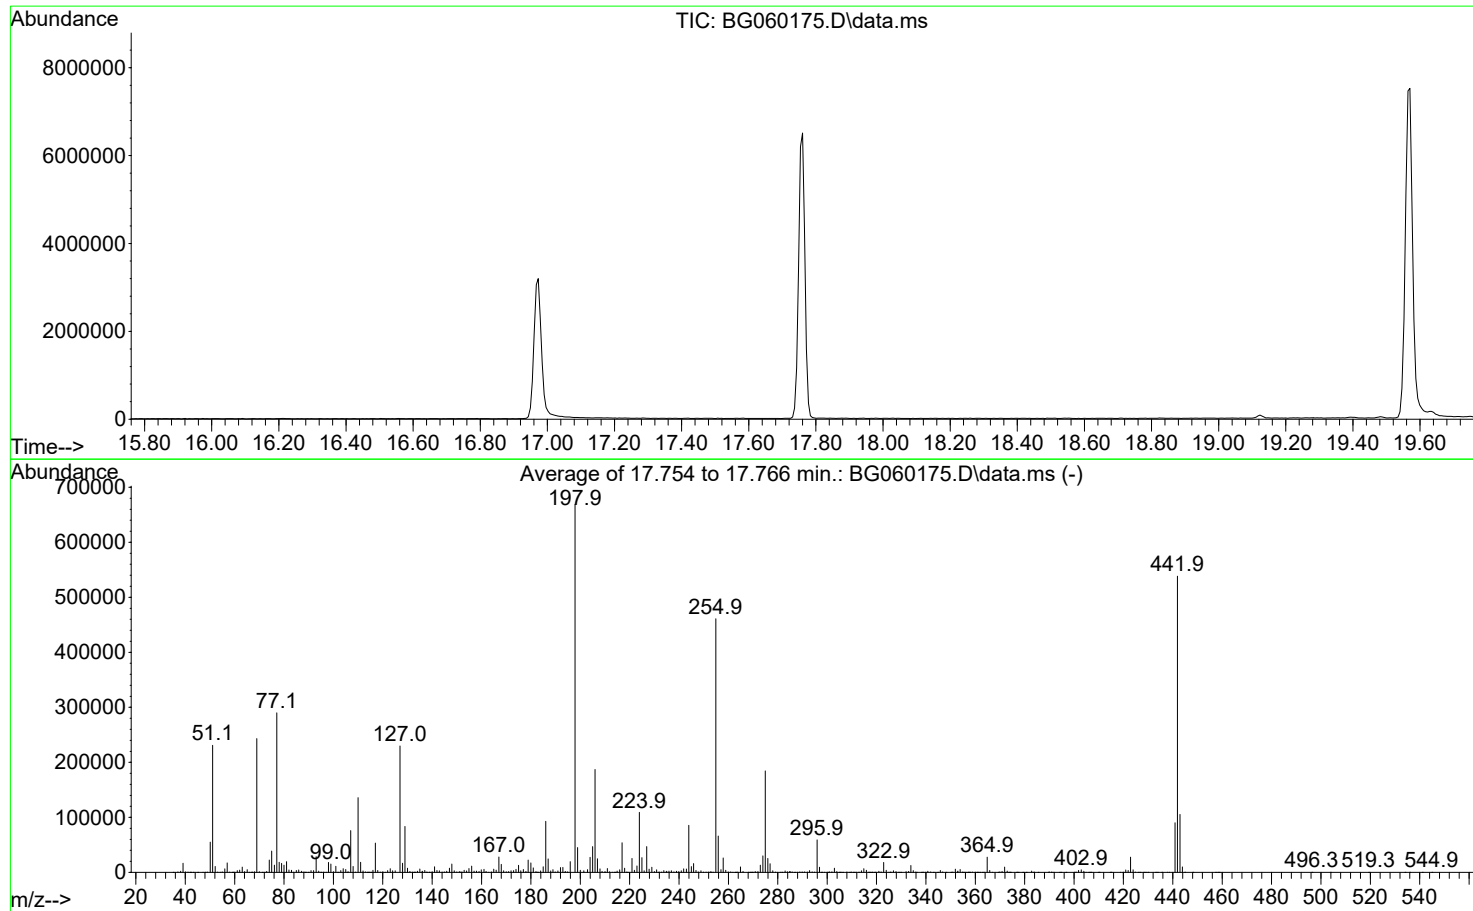

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	230976	PASS
68	69	0.00	2	0.5	1226	PASS
69	198	0.00	100	36.4	243141	PASS
70	69	0.00	2	0.5	1139	PASS
127	198	10	80	34.4	229824	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	668629	PASS
199	198	5	9	6.8	45203	PASS
275	198	10	60	27.6	184469	PASS
365	198	1	100	4.1	27611	PASS
441	198	0.01	100	13.5	90155	PASS
442	442	50	100	100.0	538240	PASS
443	442	15	24	19.6	105323	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/29/2023	BNA_G	BG060175.D
Compound Name	Response	Retention Time
DDT	2127150	20.798
DDD	25803	20.404
DDE	0	19.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25803	2152953	1.20

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122923\
Data File : BG060175.D
Acq On : 29 Dec 2023 11:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 29 11:59:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 29 11:57:19 2023
Response via : Initial Calibration

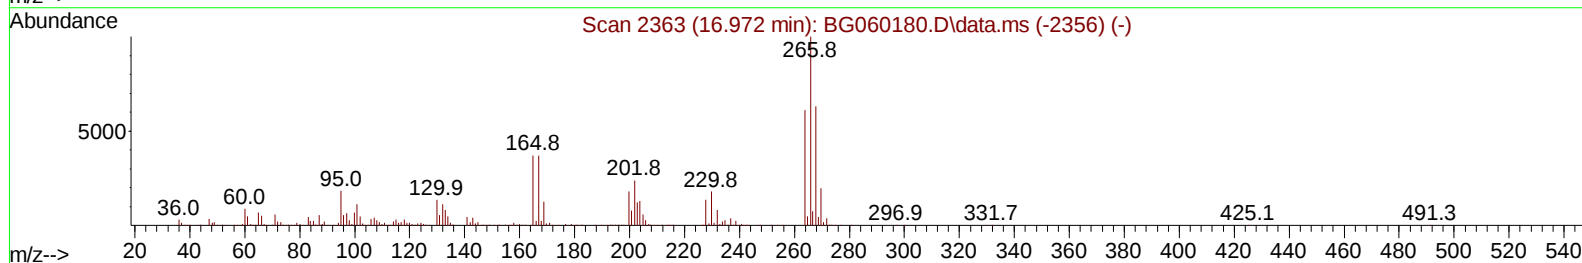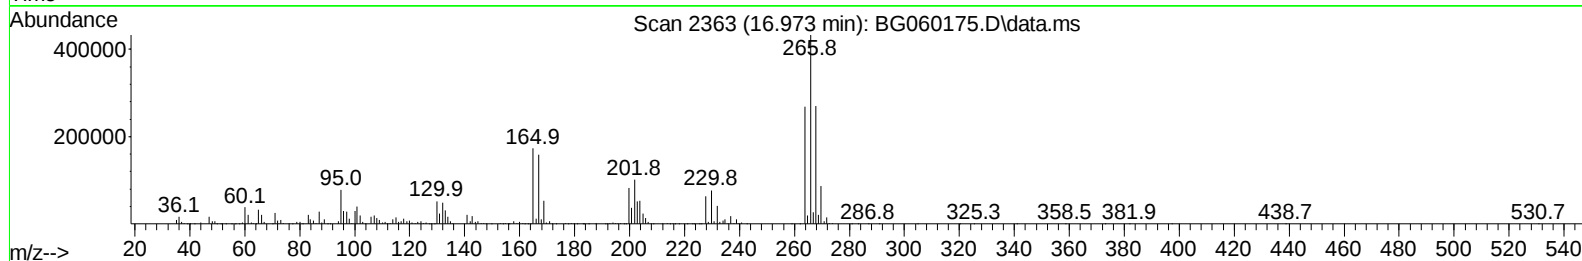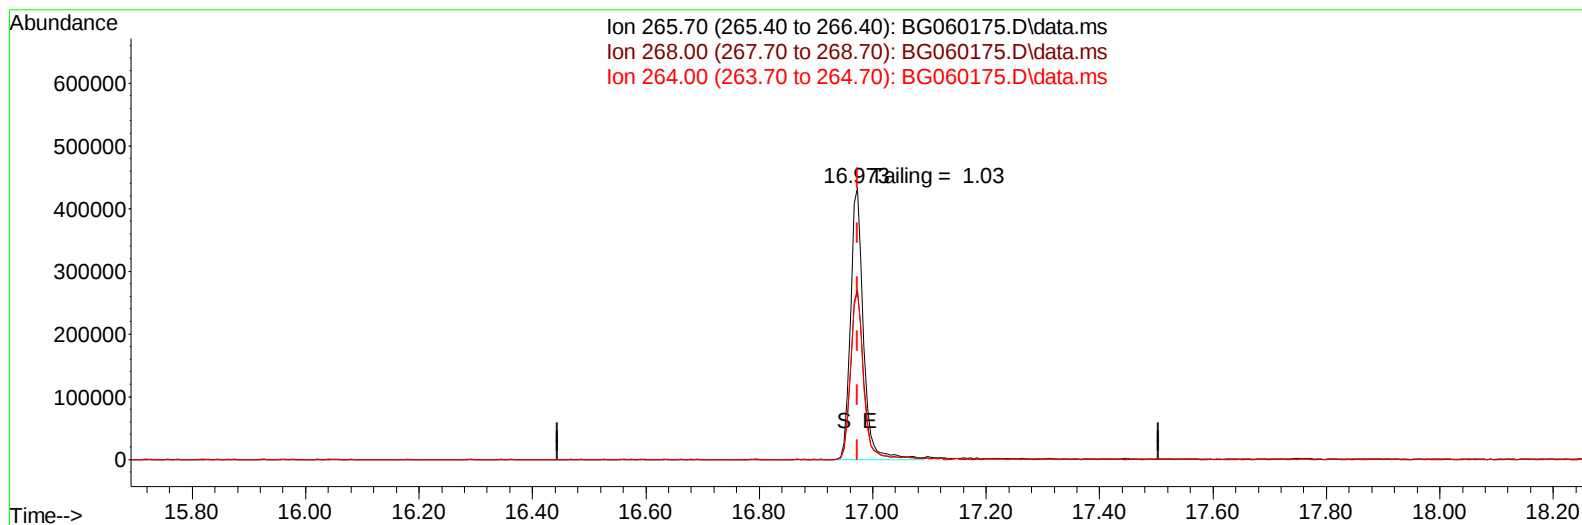

TIC: BG060175.D\data.ms

(70) Pentachlorophenol (C)

16.973min (-0.001) 493823.43 ng




response 680900

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.30	66.93
264.00	67.10	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122923\
Data File : BG060175.D
Acq On : 29 Dec 2023 11:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 29 11:59:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 29 11:57:19 2023
Response via : Initial Calibration

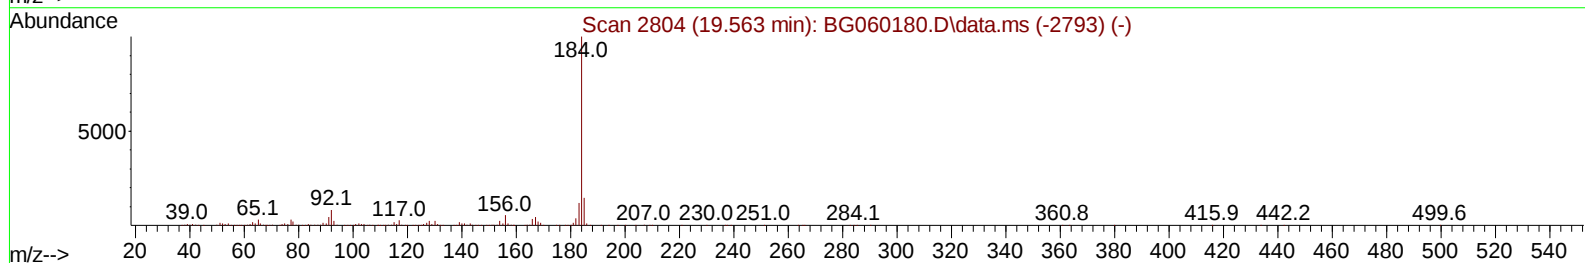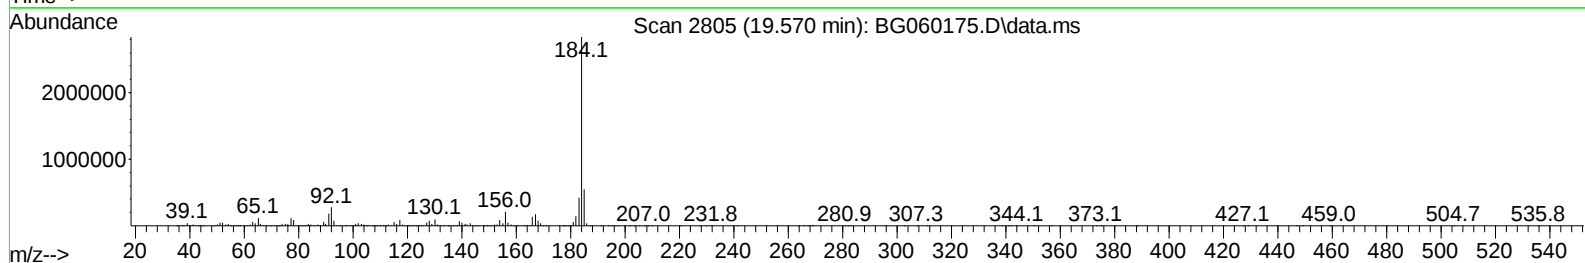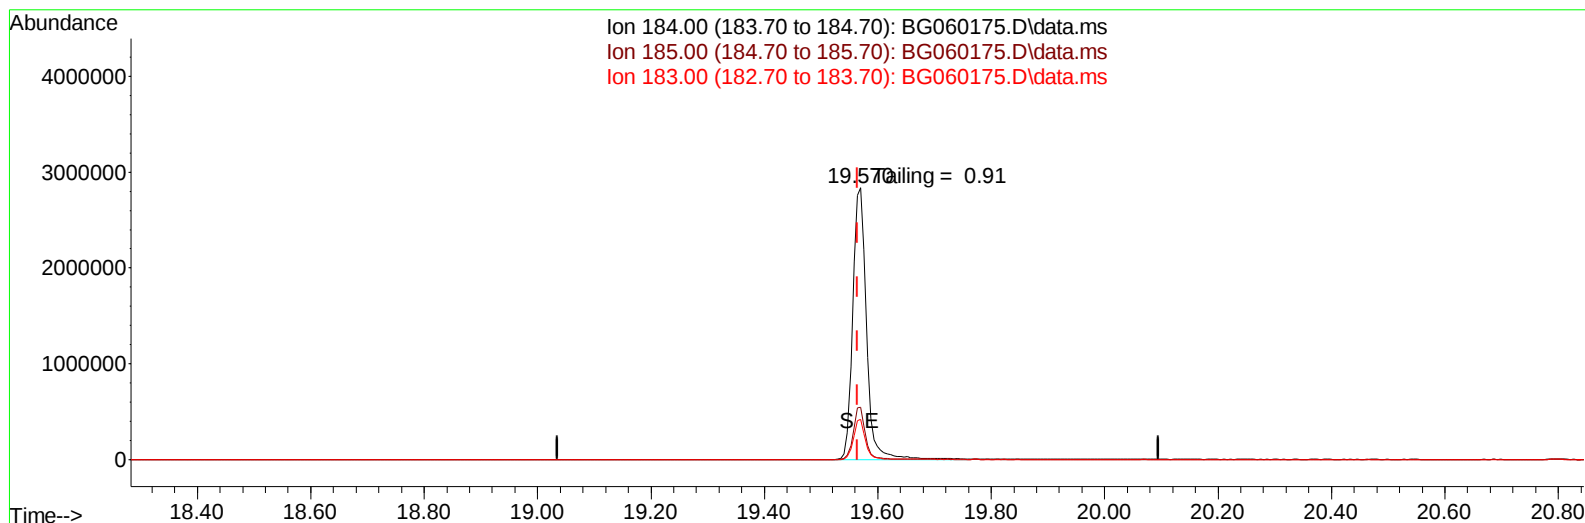

TIC: BG060175.D\data.ms

(77) Benzidine

19.570min (+ 0.005) 2310367.26 ng

response 4804552

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	19.33#
183.00	10.80	14.81#
0.00	0.00	0.00