



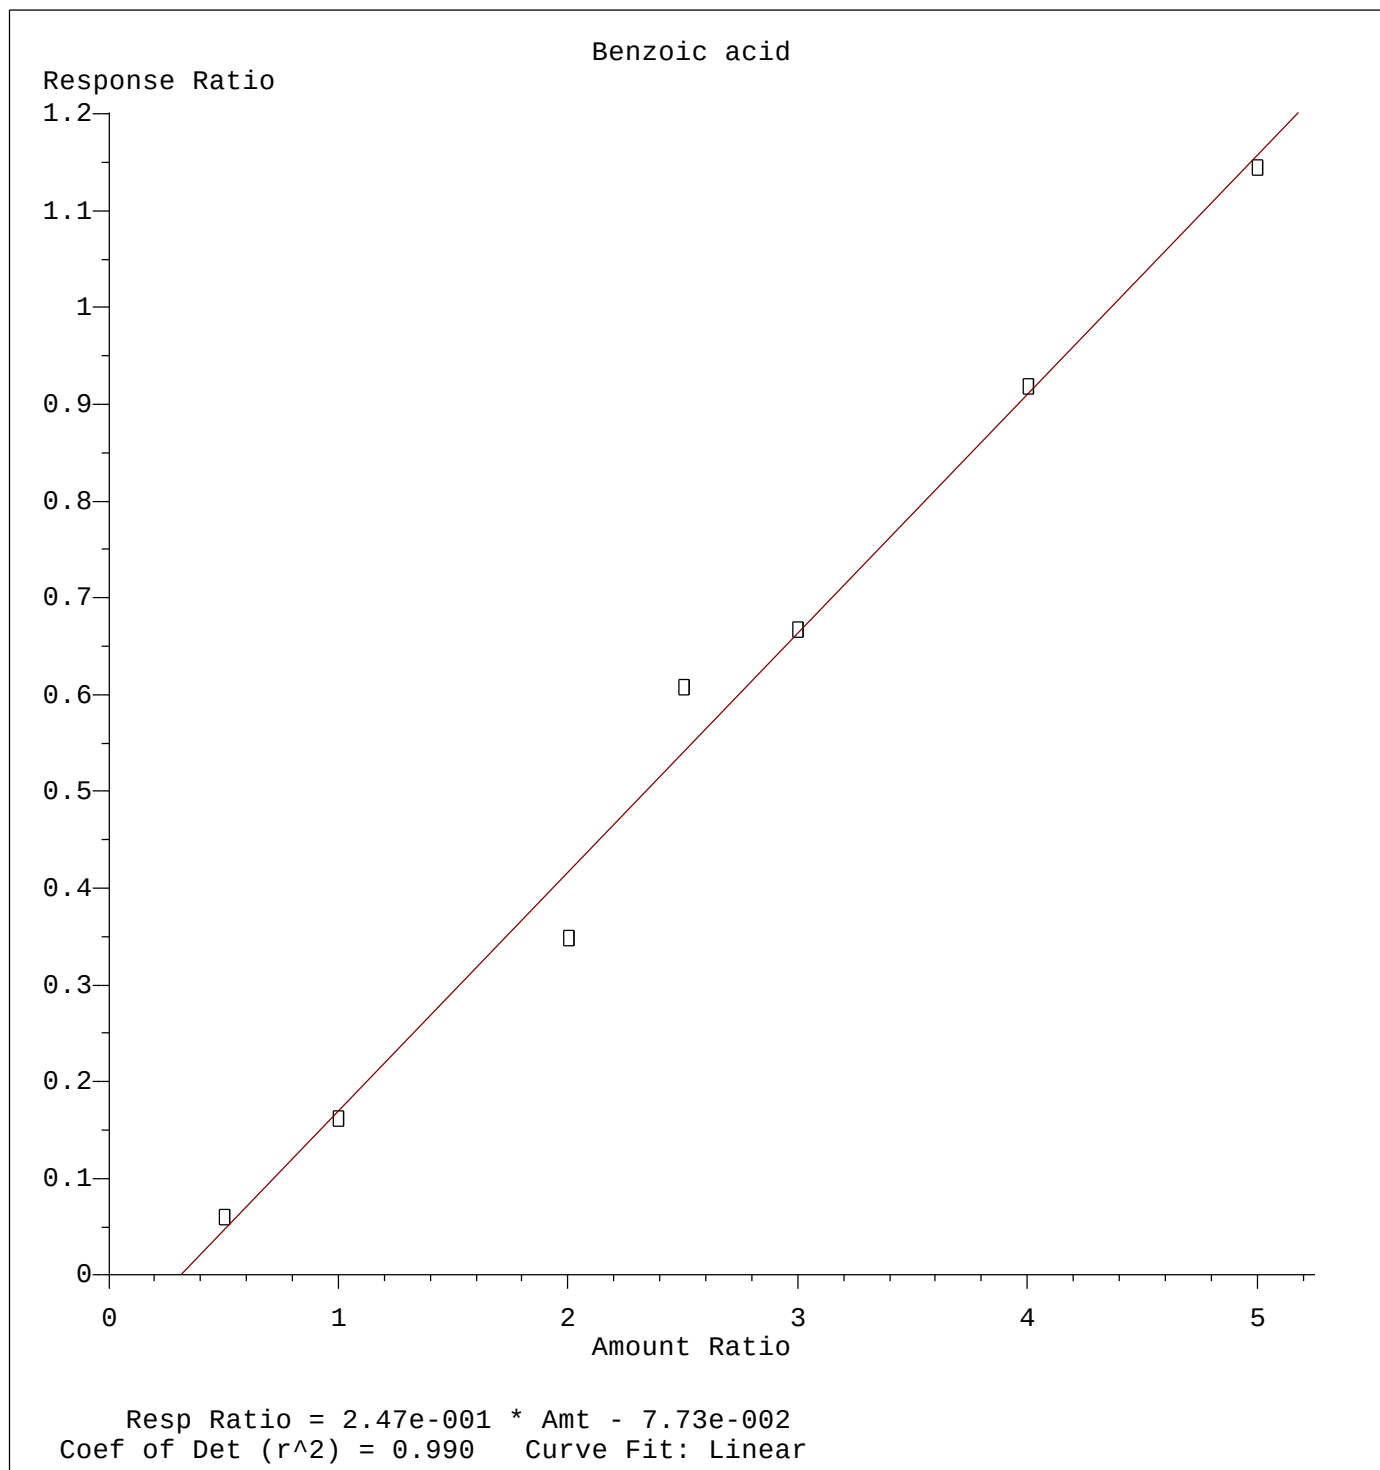

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Calibration Table Last Updated: Tue Dec 31 13:32:23 2019

2,4-Dinitrophenol


Response Ratio

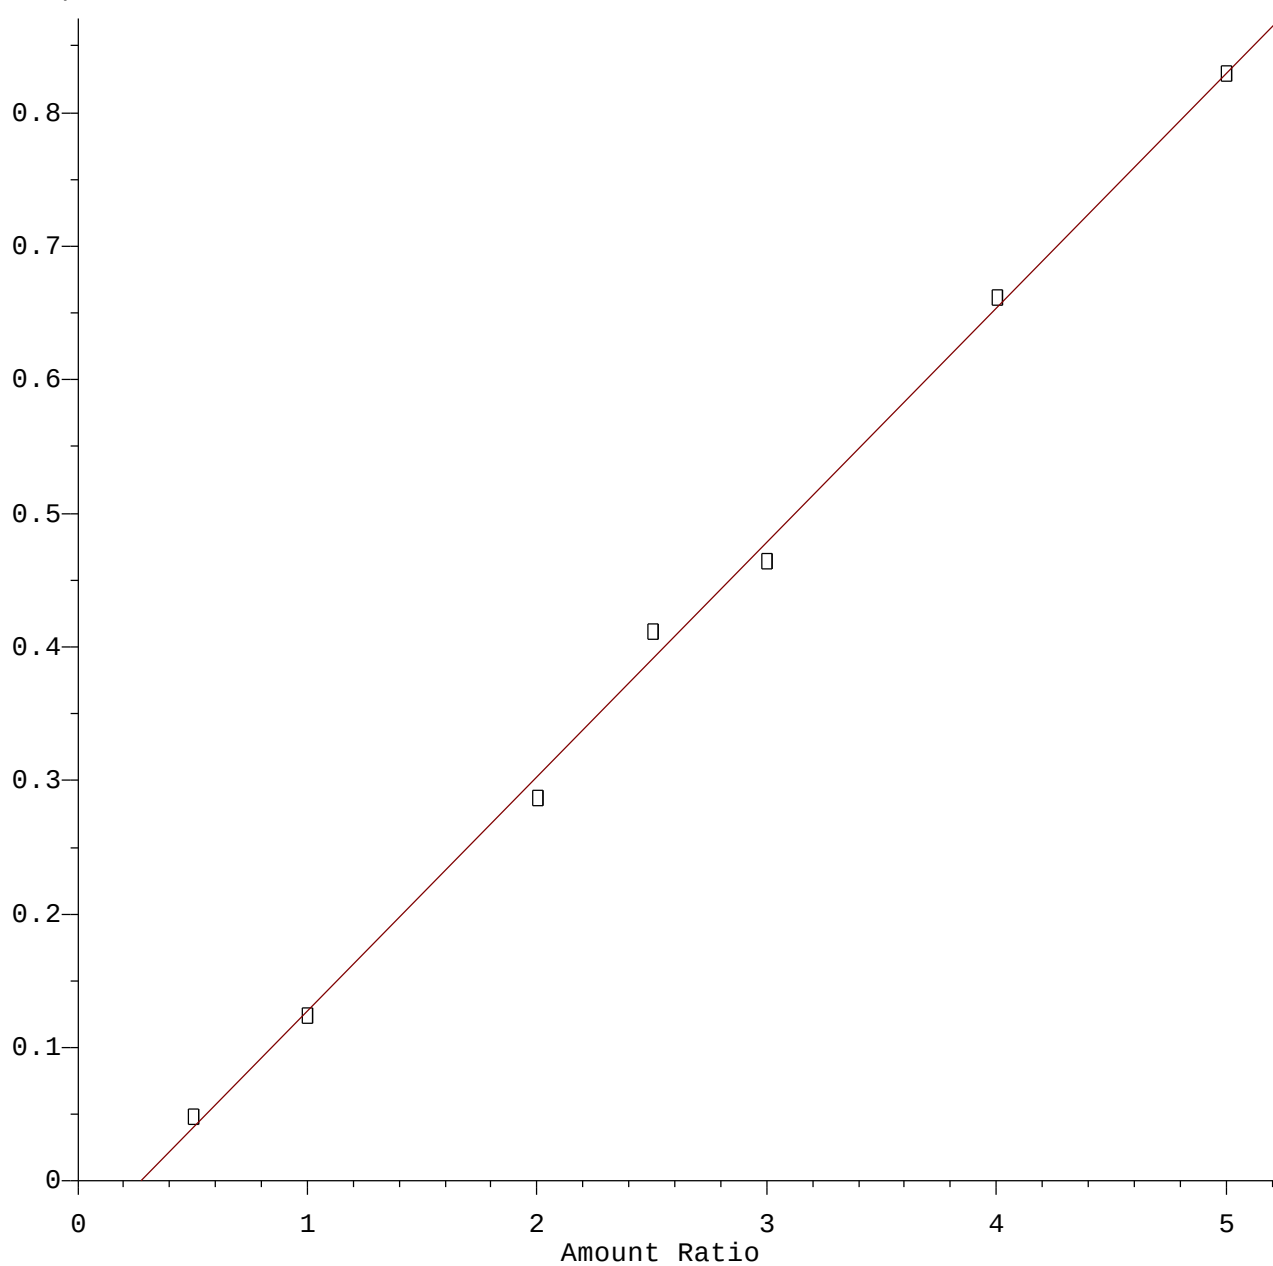

Resp Ratio = 1.76e-001 * Amt - 4.81e-002
Coef of Det (r²) = 0.998 Curve Fit: Linear


Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Calibration Table Last Updated: Tue Dec 31 13:32:23 2019

4,6-Dinitro-2-methylphenol

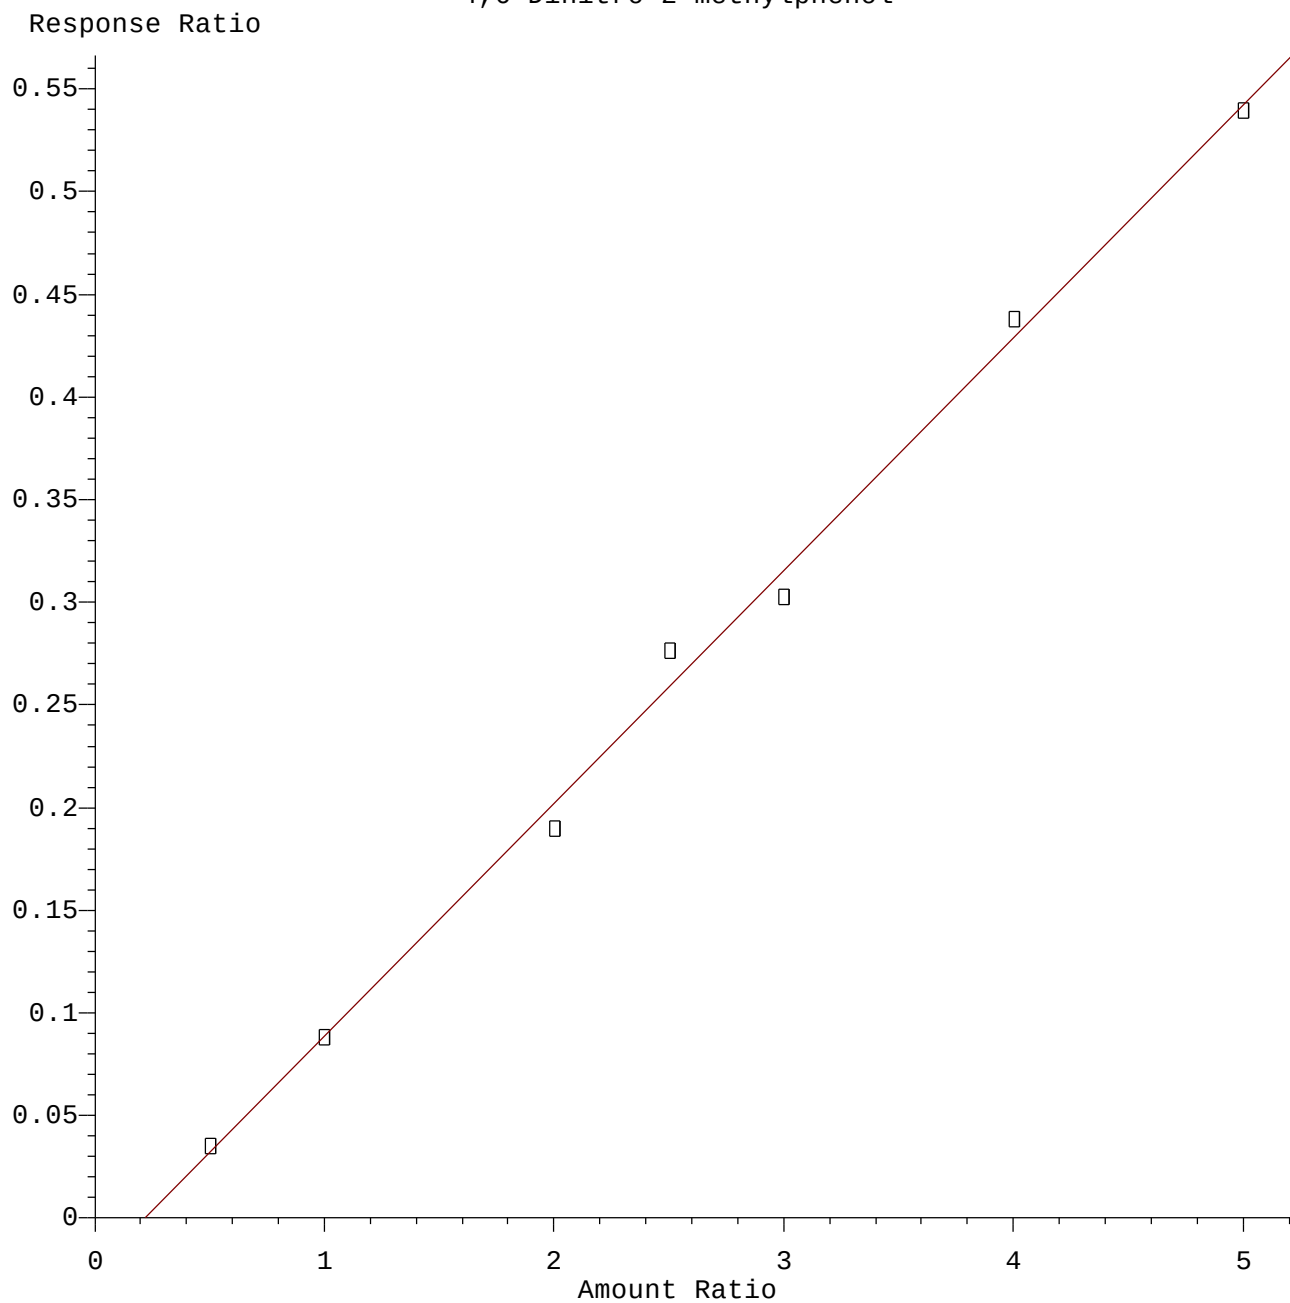

Resp Ratio = $1.13 \times 10^{-1} \times \text{Amt} - 2.49 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Calibration Table Last Updated: Tue Dec 31 13:32:23 2019

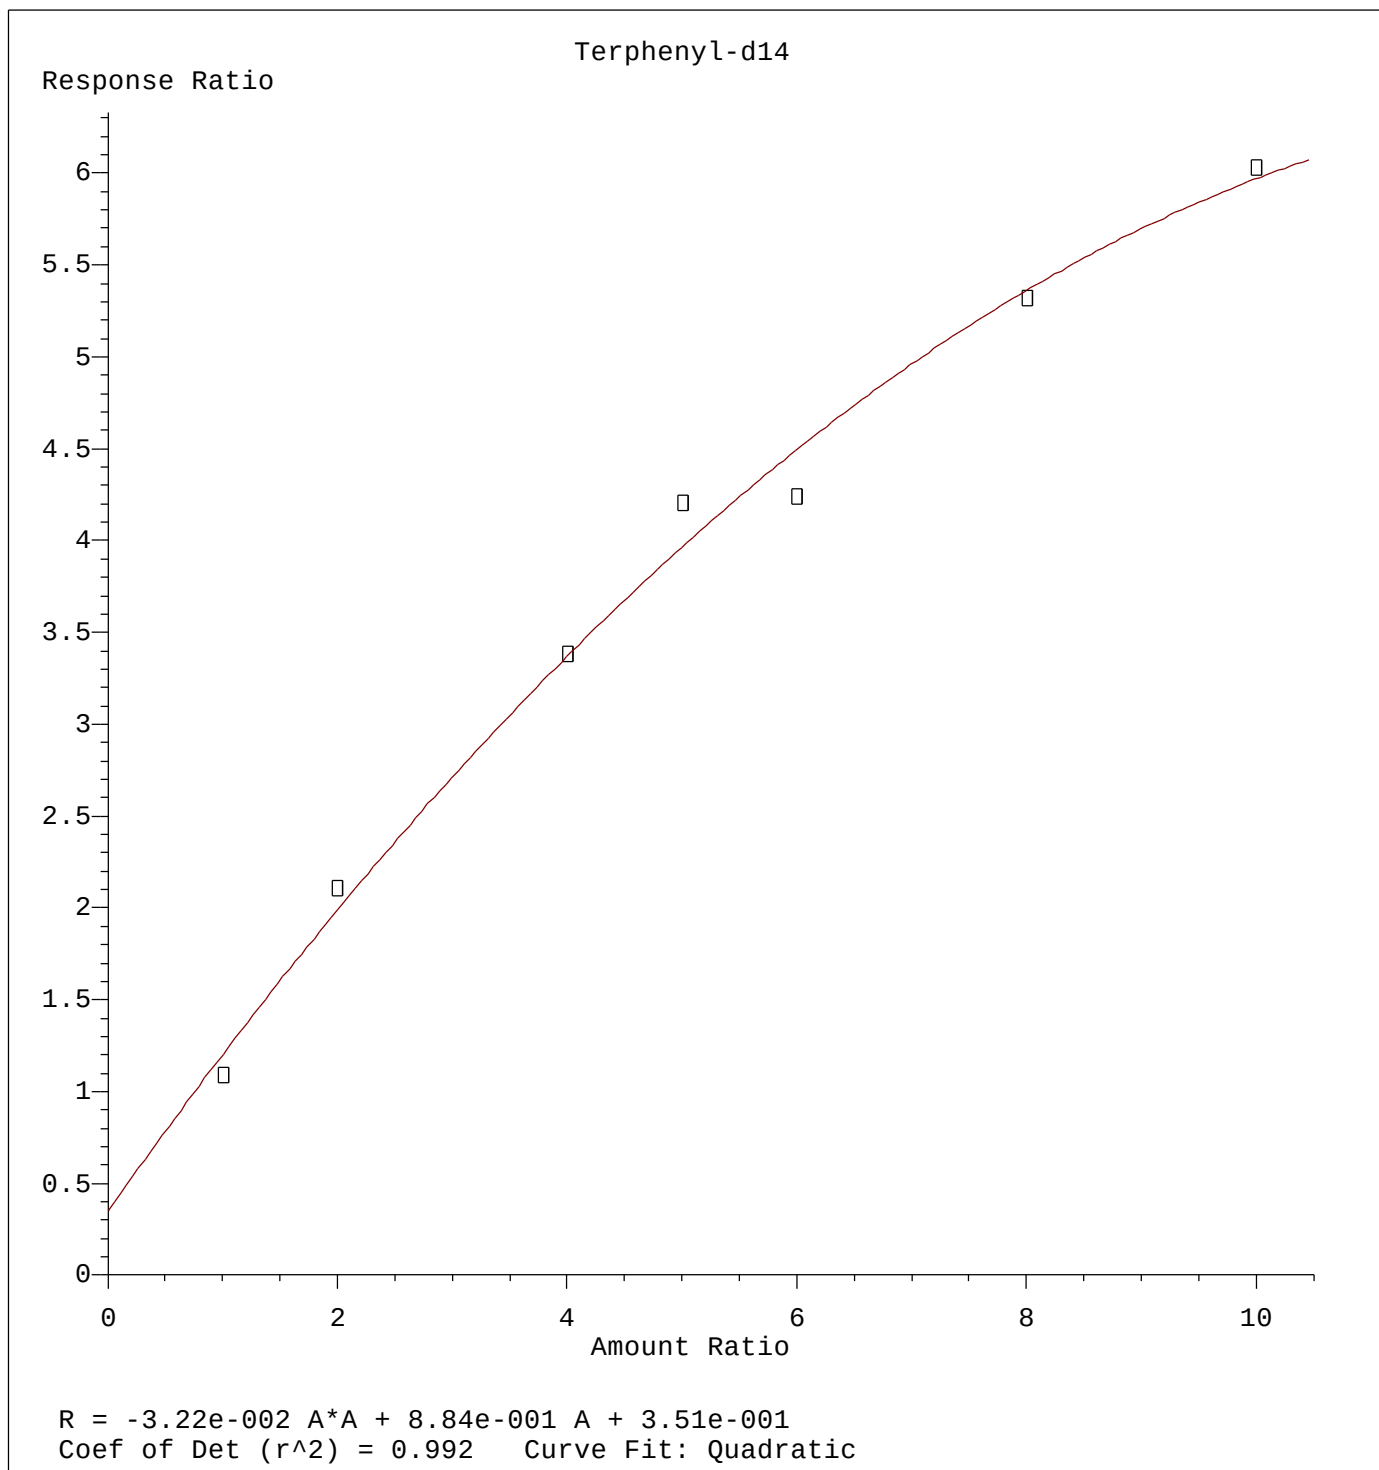

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Calibration Table Last Updated: Tue Dec 31 13:32:23 2019