
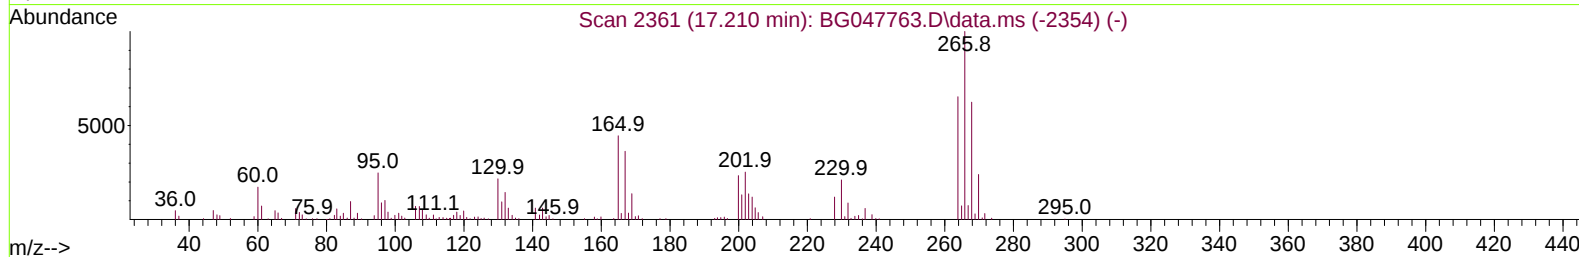
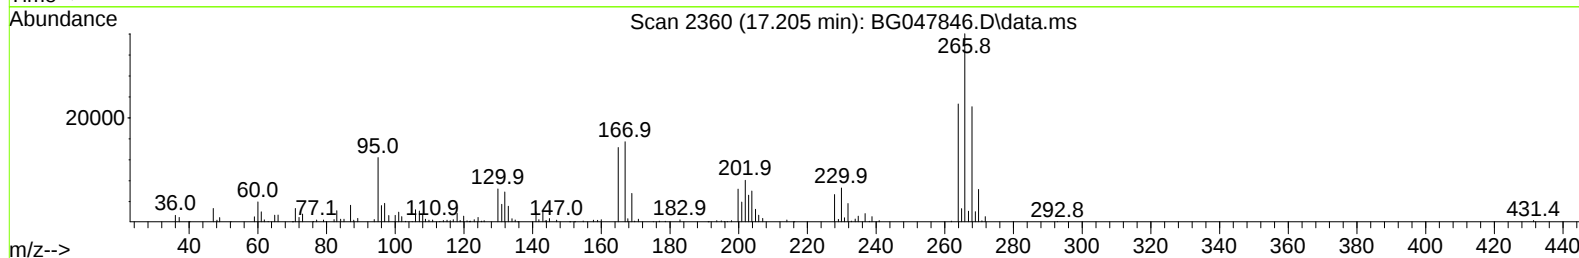


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG123120\
Data File : BG047846.D
Acq On : 31 Dec 2020 13:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 01 01:43:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 17 15:55:16 2020
Response via : Initial Calibration

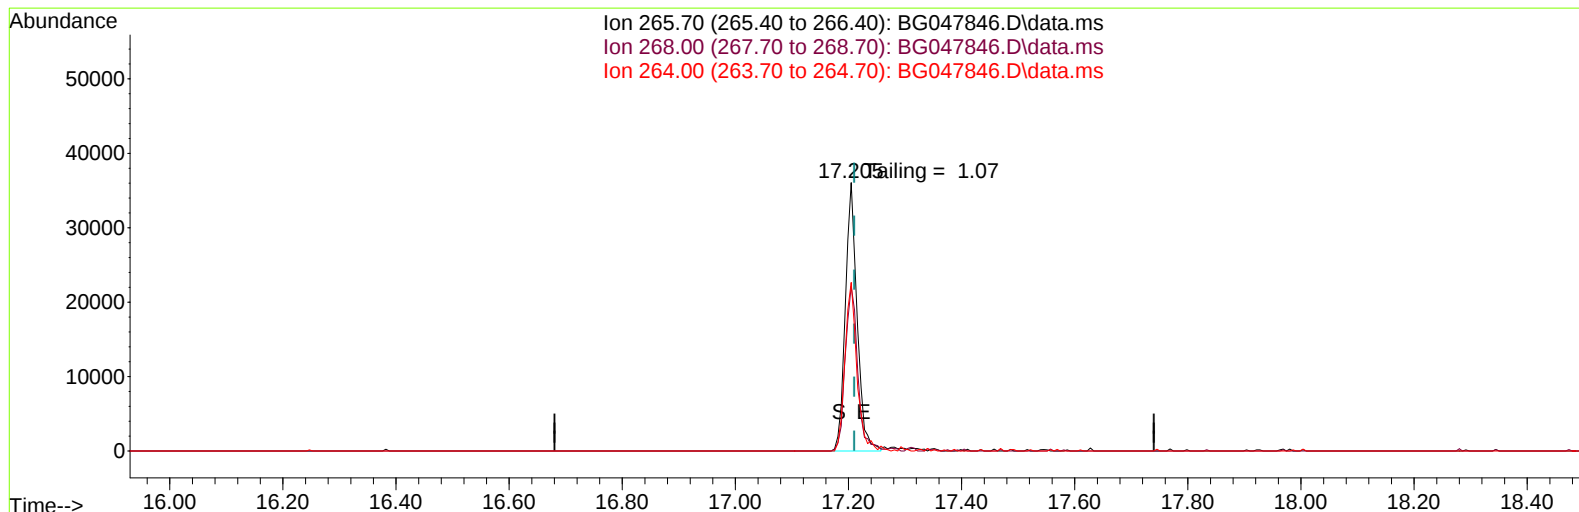

TIC: BG047846.D\data.ms

(70) Pentachlorophenol (C)




17.205min (-0.005) 2208.60 ng

response 46466

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.40
264.00	61.60	62.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG123120\
Data File : BG047846.D
Acq On : 31 Dec 2020 13:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 01 01:43:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 17 15:55:16 2020
Response via : Initial Calibration

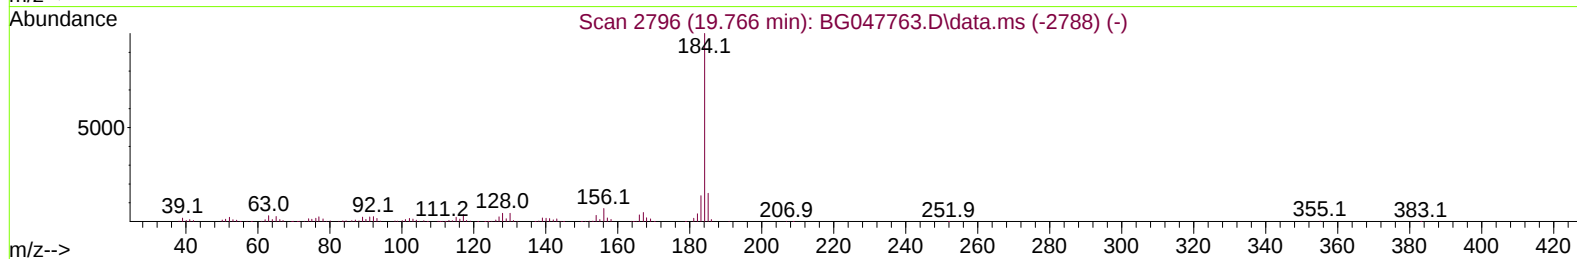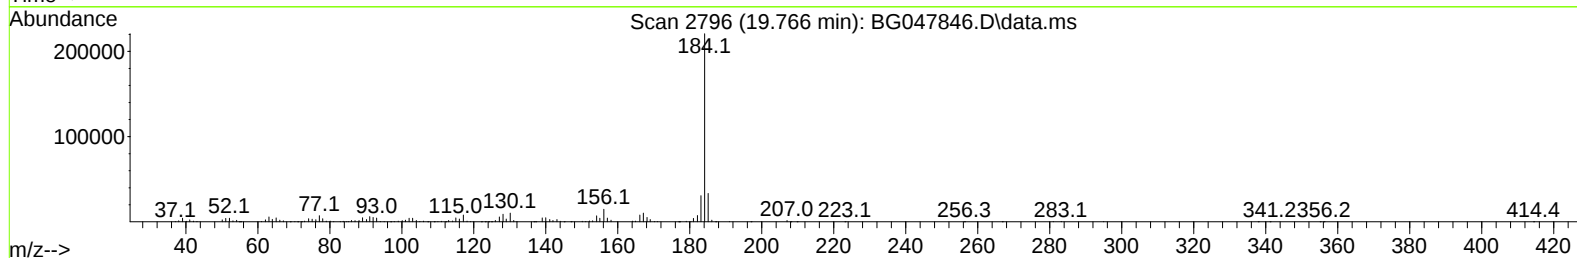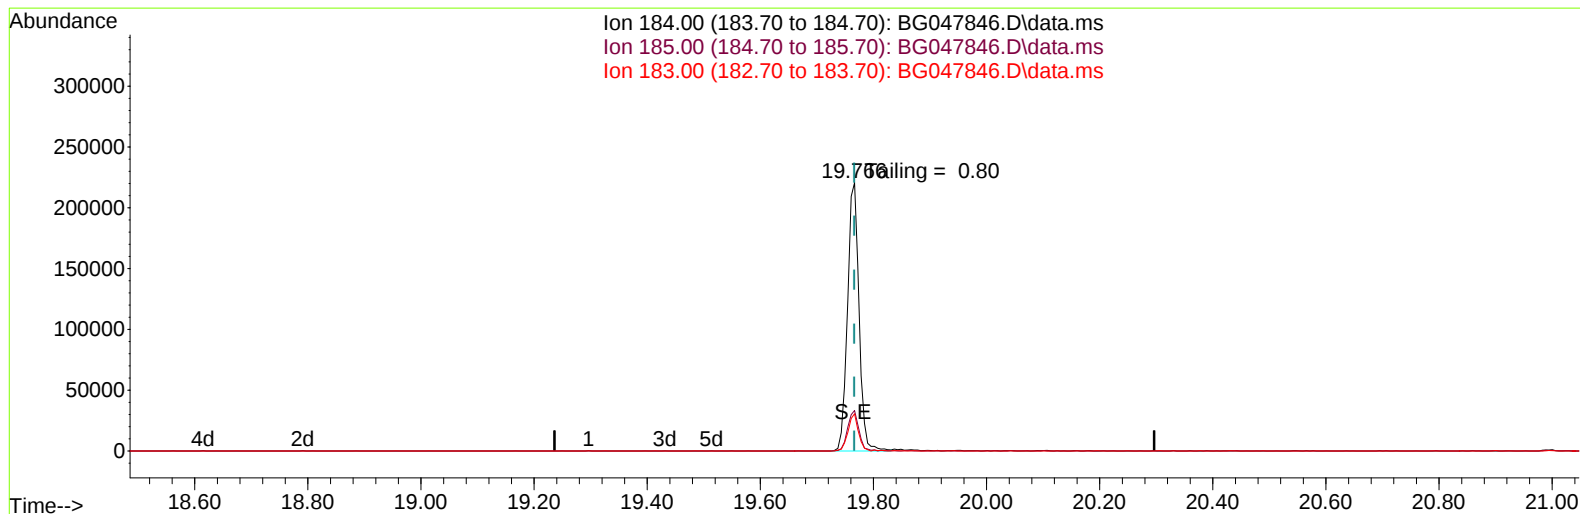

TIC: BG047846.D\data.ms

(77) Benzidine

19.766min (+ 0.000) 77252.08 ng m

response 313694

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.12
183.00	13.20	13.90
0.00	0.00	0.00