
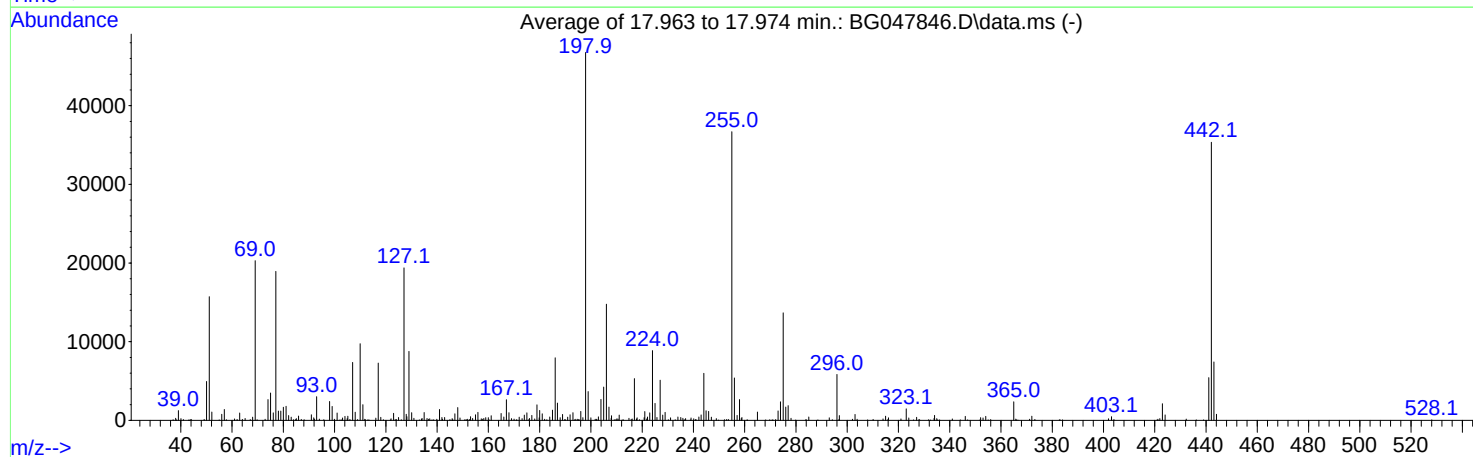


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG123120\
 Data File : BG047846.D
 Acq On : 31 Dec 2020 13:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 17 15:55:16 2020

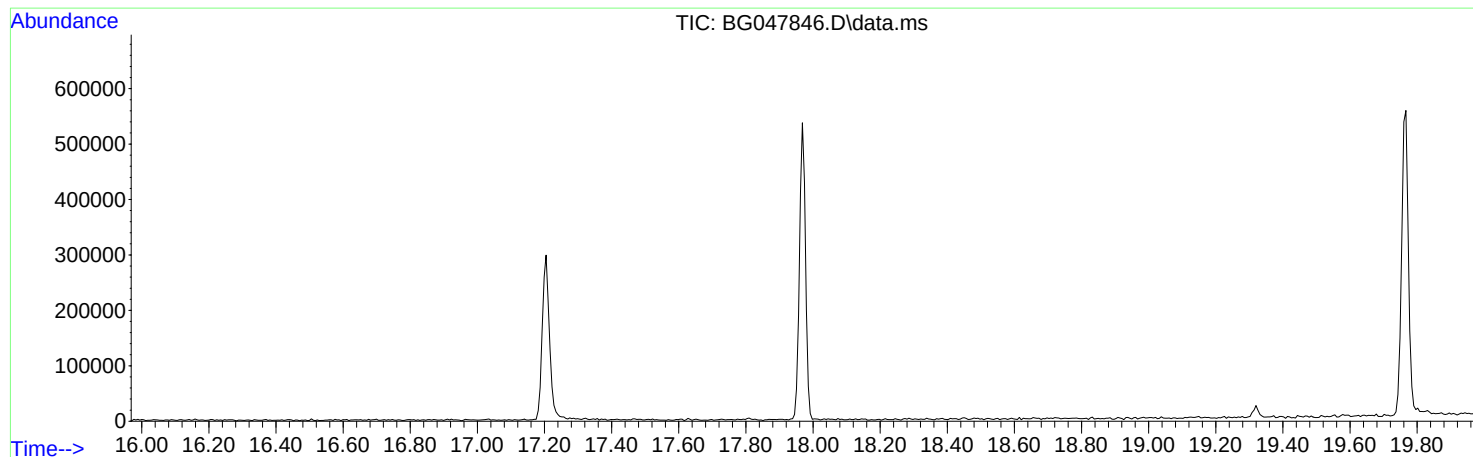

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	15725	PASS
68	69	0.00	2	2.0	405	PASS
69	198	0.00	100	43.4	20293	PASS
70	69	0.00	2	0.5	92	PASS
127	198	10	80	41.5	19392	PASS
197	198	0.00	2	0.7	343	PASS
198	198	100	100	100.0	46757	PASS
199	198	5	9	7.8	3658	PASS
275	198	10	60	29.2	13661	PASS
365	198	1	100	5.1	2365	PASS
441	198	0.01	100	11.6	5423	PASS
442	198	50	100	75.6	35339	PASS
443	442	15	24	21.0	7420	PASS