
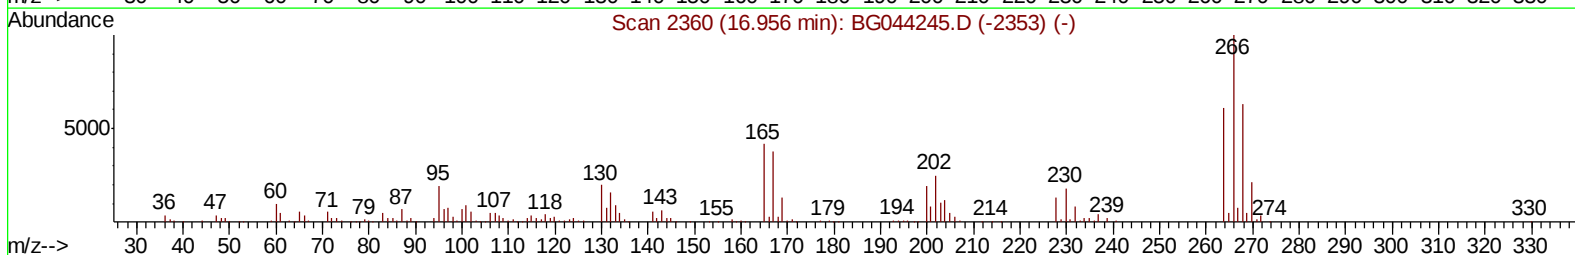
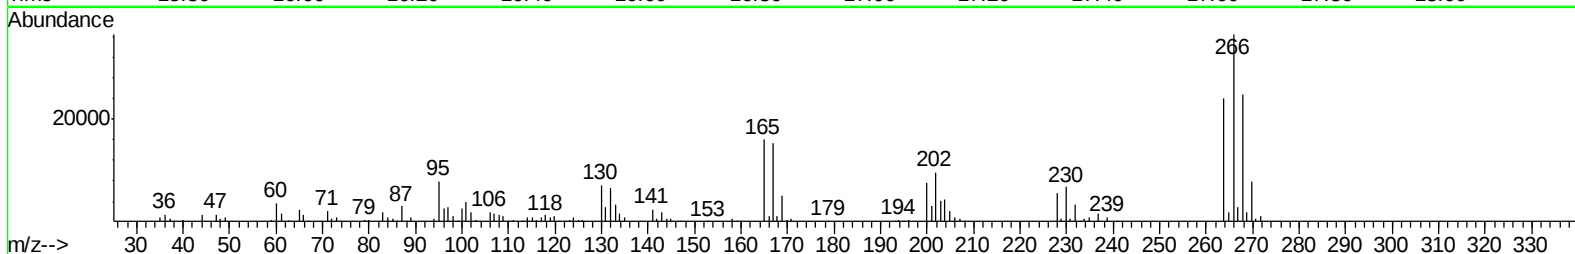


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG020620\  
 Data File : BG044317.D  
 Acq On : 6 Feb 2020 11:06  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 22:26:58 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jan 30 16:05:09 2020  
 Response via : Initial Calibration

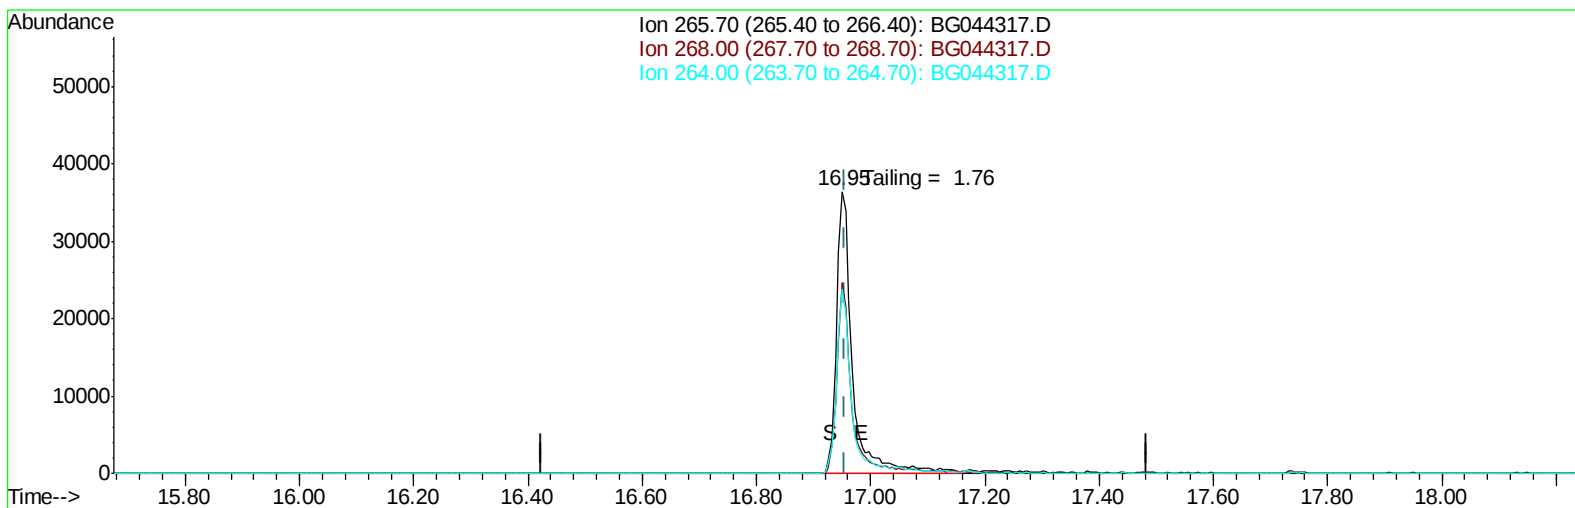

TIC: BG044317.D

(70) Pentachlorophenol (C)




16.950min (-0.005) 18378.78ng

response 69536

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.20 | 67.77 |
| 264.00 | 60.90 | 65.59 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG020620\  
 Data File : BG044317.D  
 Acq On : 6 Feb 2020 11:06  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 22:26:58 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jan 30 16:05:09 2020  
 Response via : Initial Calibration

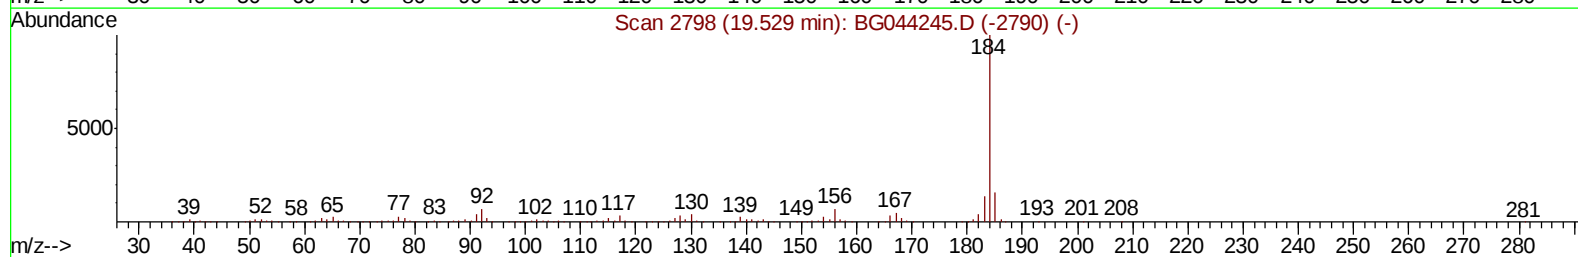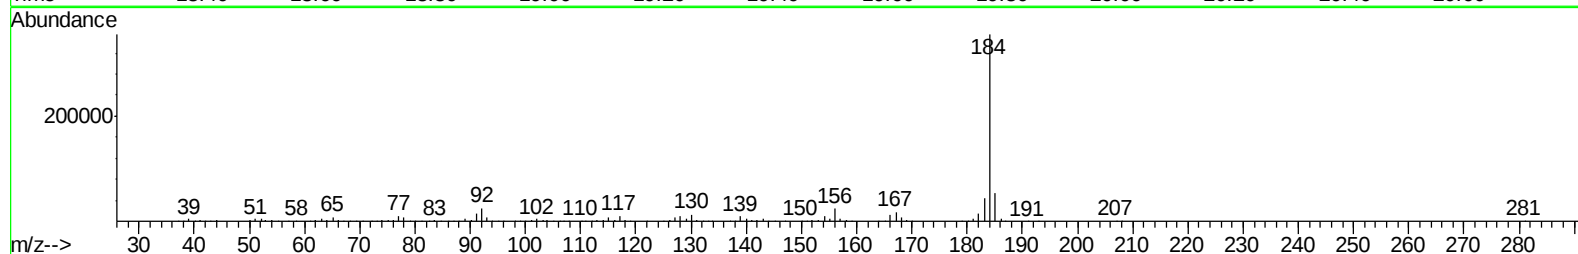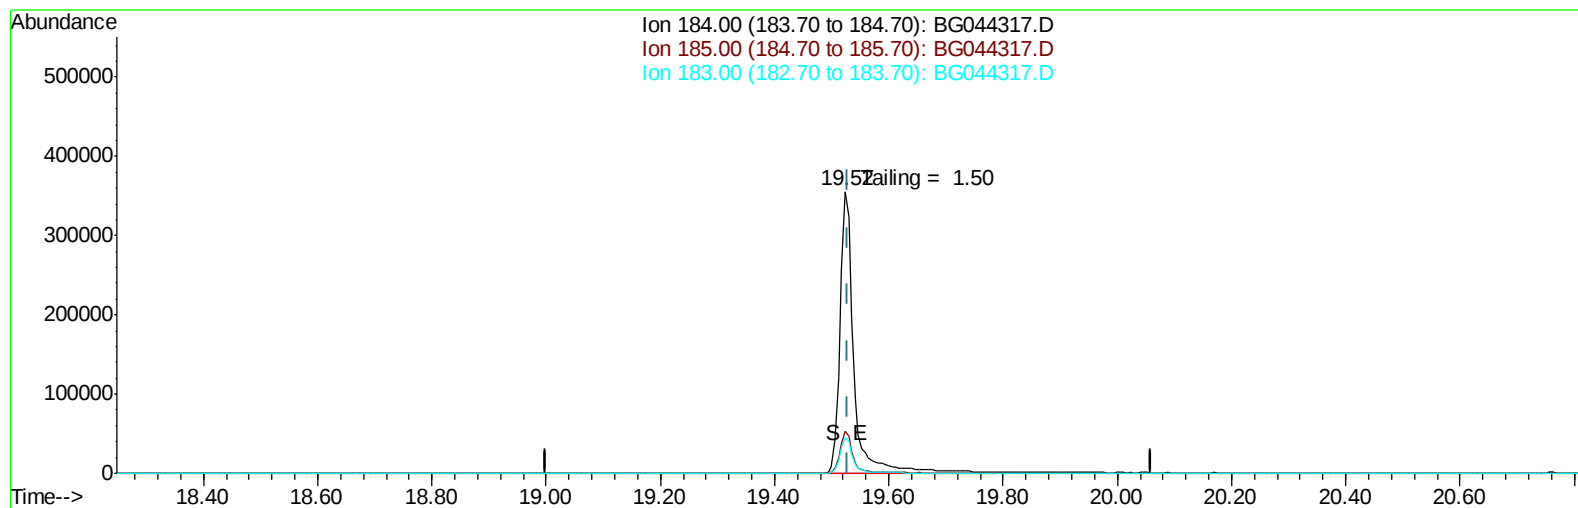

TIC: BG044317.D

(77) Benzidine

19.523min (-0.006) 0.00ng

response 600402

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.10 | 14.94 |
| 183.00 | 13.50 | 12.69 |
| 0.00   | 0.00  | 0.00  |