


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG020620\
 Data File : BG044317.D
 Acq On : 6 Feb 2020 11:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 30 16:05:09 2020

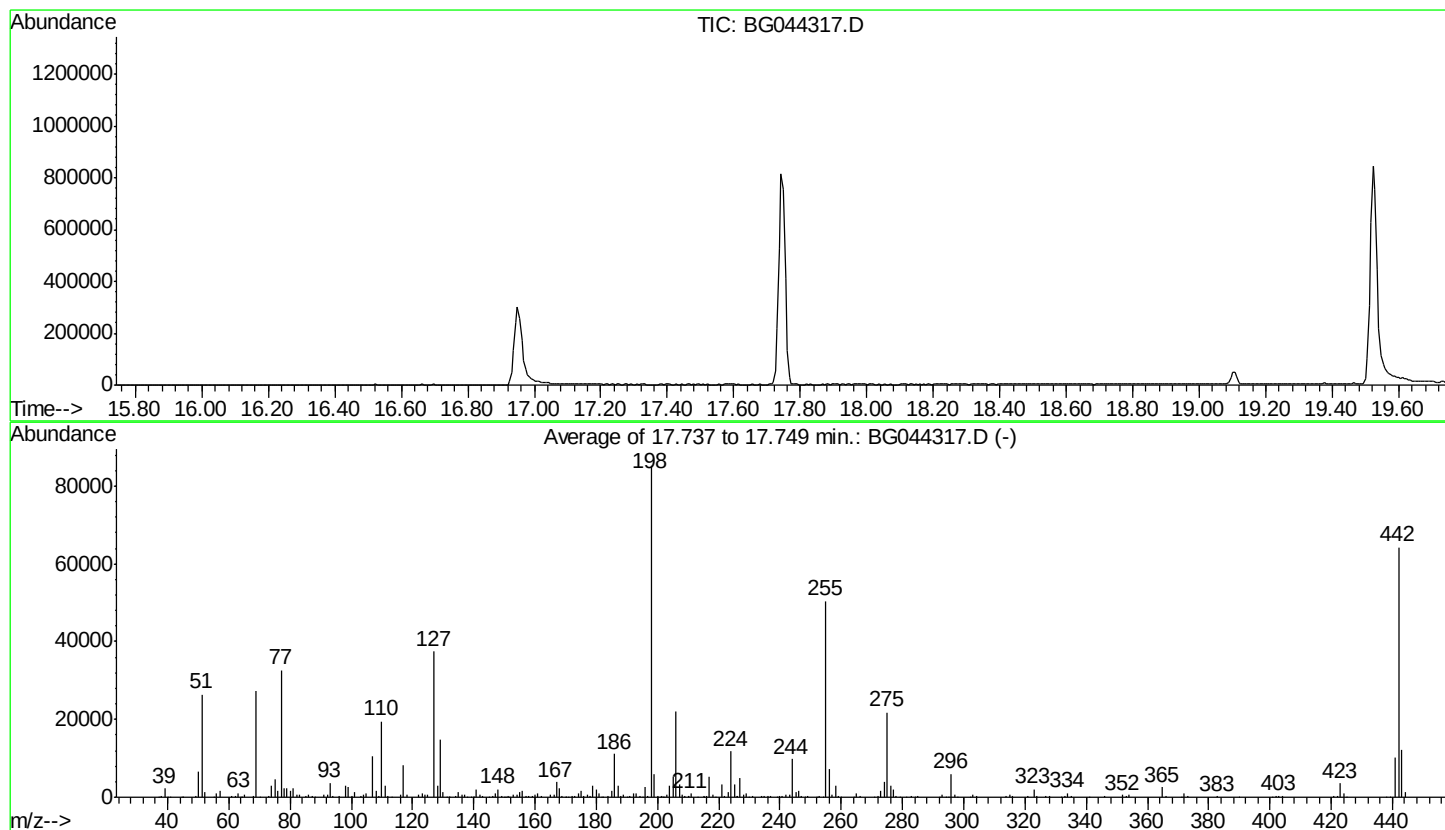

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.9	26336	PASS
68	69	0.00	2	1.3	356	PASS
69	198	0.00	100	32.1	27352	PASS
70	69	0.00	2	0.6	168	PASS
127	198	10	80	43.9	37408	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	85253	PASS
199	198	5	9	6.9	5916	PASS
275	198	10	60	25.6	21788	PASS
365	198	1	100	3.0	2593	PASS
441	198	0.01	100	12.1	10336	PASS
442	198	50	100	75.3	64218	PASS
443	442	15	24	19.1	12292	PASS