
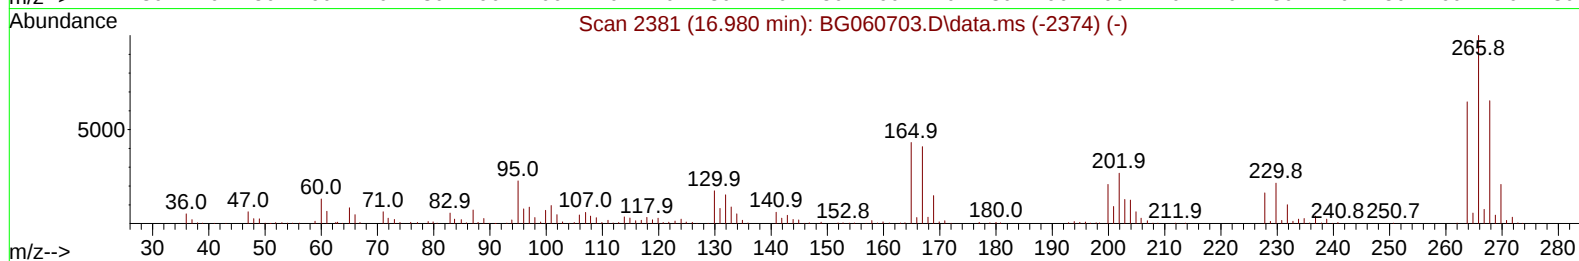
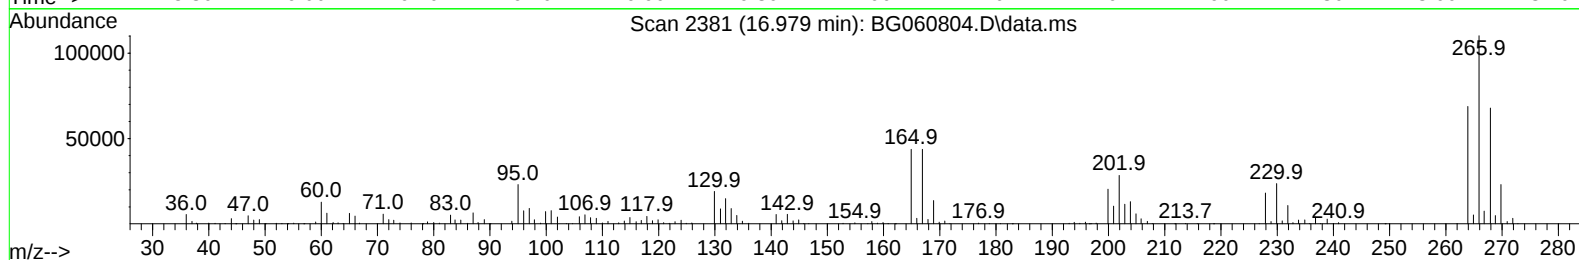


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040624\
Data File : BG060804.D
Acq On : 6 Apr 2024 9:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 10:35:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

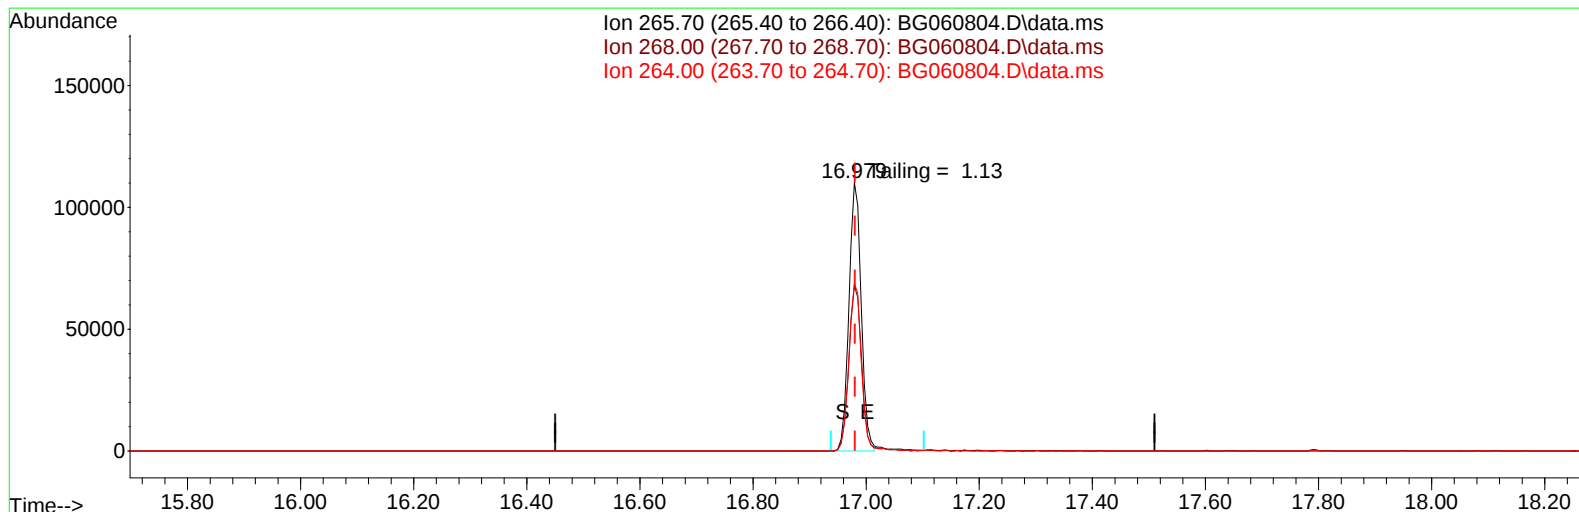

TIC: BG060804.D\data.ms

(70) Pentachlorophenol (C)




16.979min (-0.001) 29873.47 ng

response 169944

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	61.58
264.00	64.70	62.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040624\
Data File : BG060804.D
Acq On : 6 Apr 2024 9:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 10:35:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

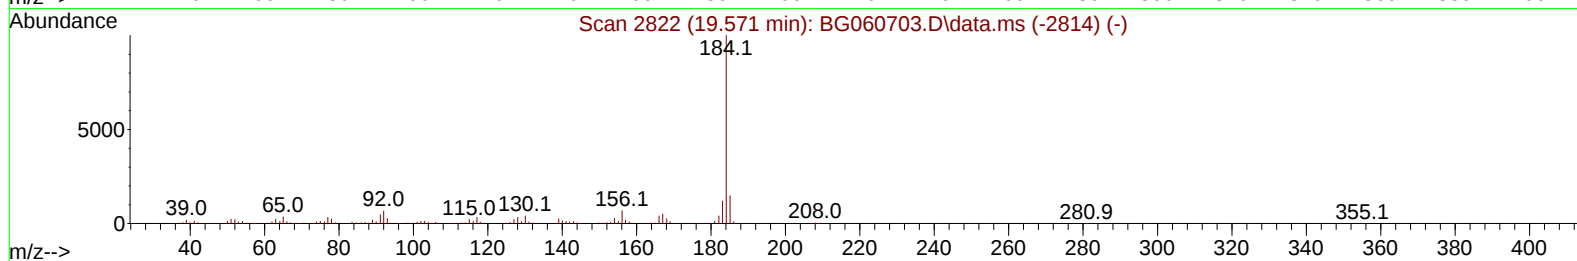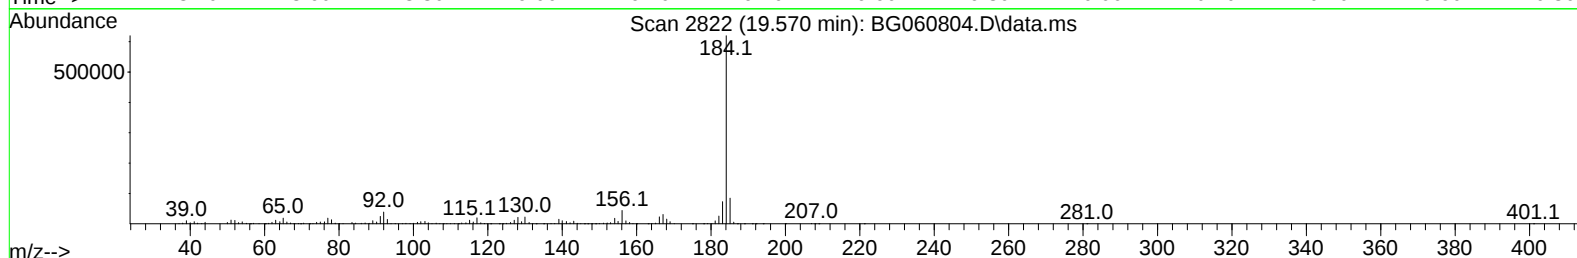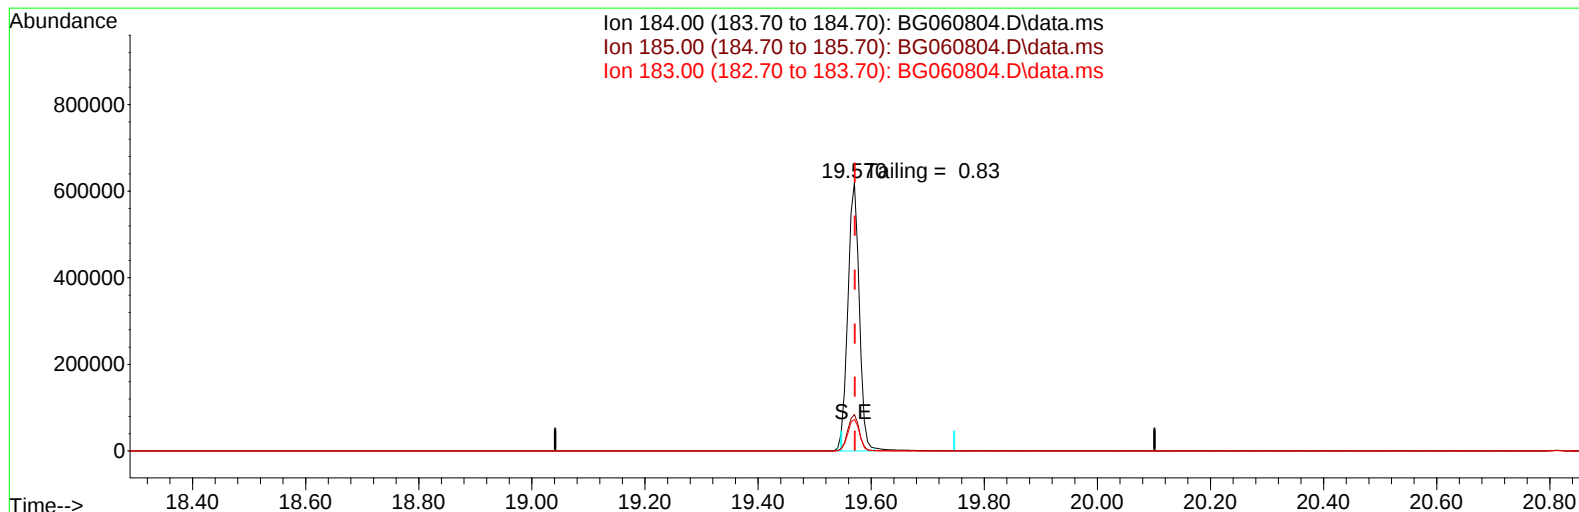

TIC: BG060804.D\data.ms

(77) Benzidine**19.570min (-0.001) 606421.48 ng****response 862293**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.64
183.00	11.90	11.80
0.00	0.00	0.00