
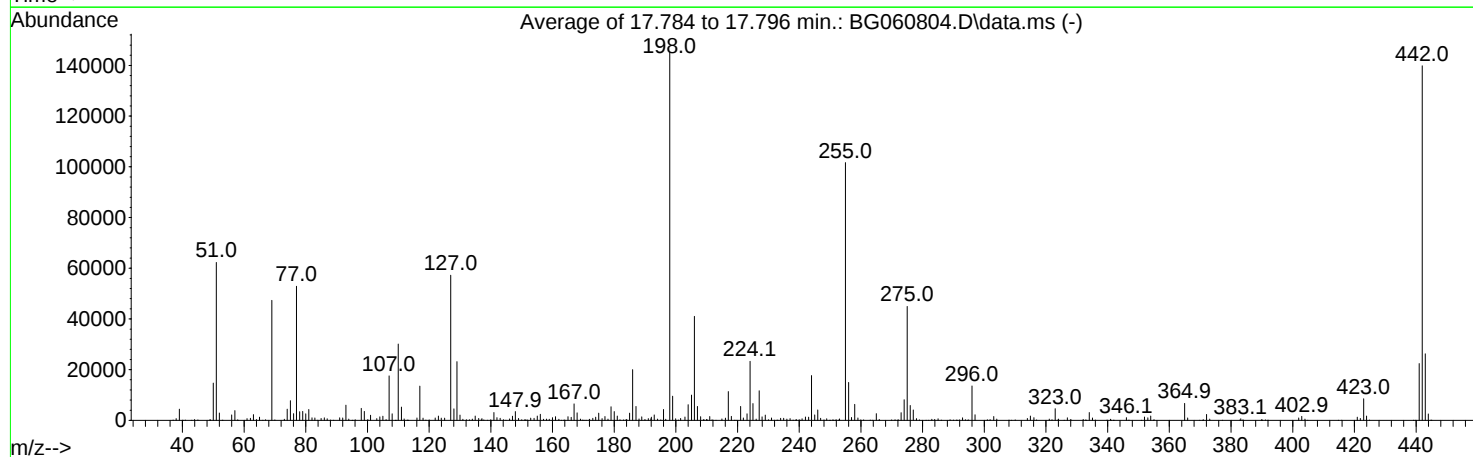


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040624\
Data File : BG060804.D
Acq On : 6 Apr 2024 9:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 30 03:12:26 2024

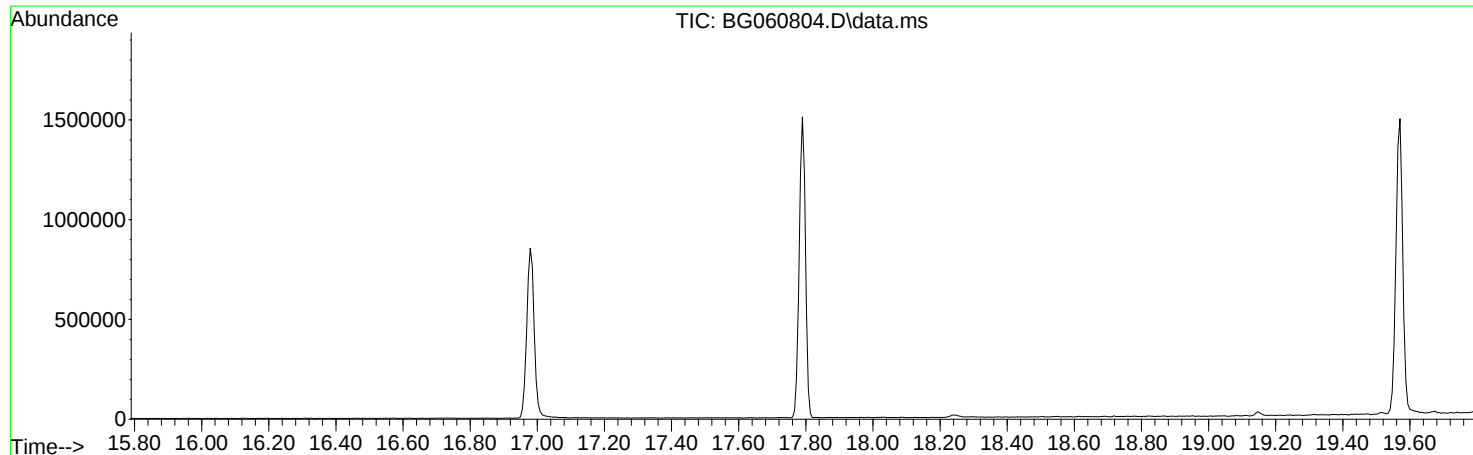




AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.9	62299	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.6	47354	PASS
70	69	0.00	2	0.4	176	PASS
127	198	10	80	39.4	57211	PASS
197	198	0.00	2	0.3	424	PASS
198	198	100	100	100.0	145088	PASS
199	198	5	9	6.6	9504	PASS
275	198	10	60	31.0	44947	PASS
365	198	1	100	4.6	6723	PASS
441	198	0.01	100	15.5	22428	PASS
442	442	50	100	100.0	139824	PASS
443	442	15	24	18.8	26237	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040624\
Data File : BG060804.D
Acq On : 6 Apr 2024 9:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 06 10:35:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

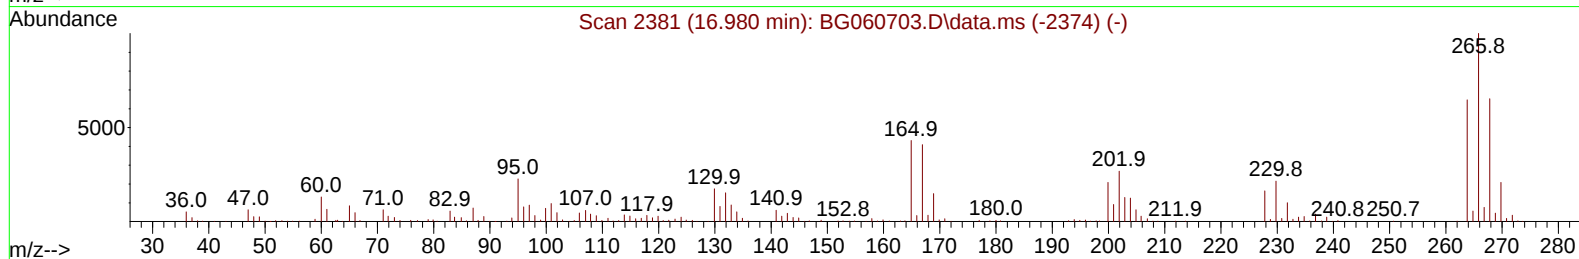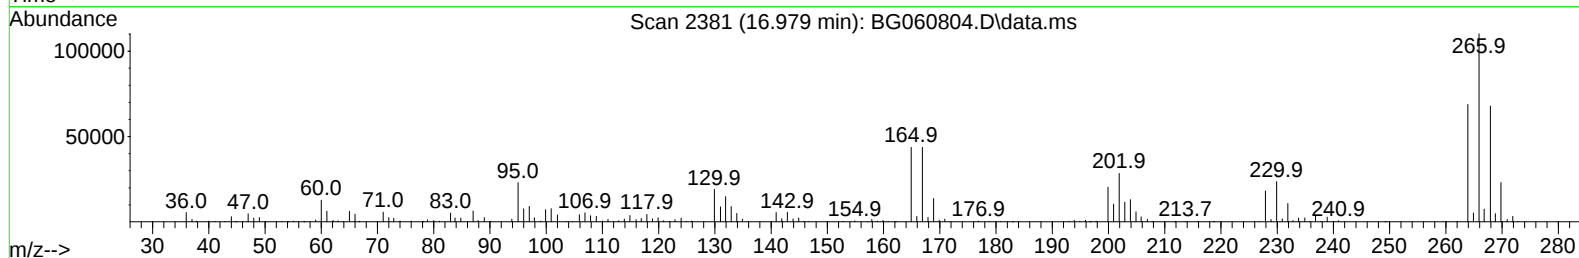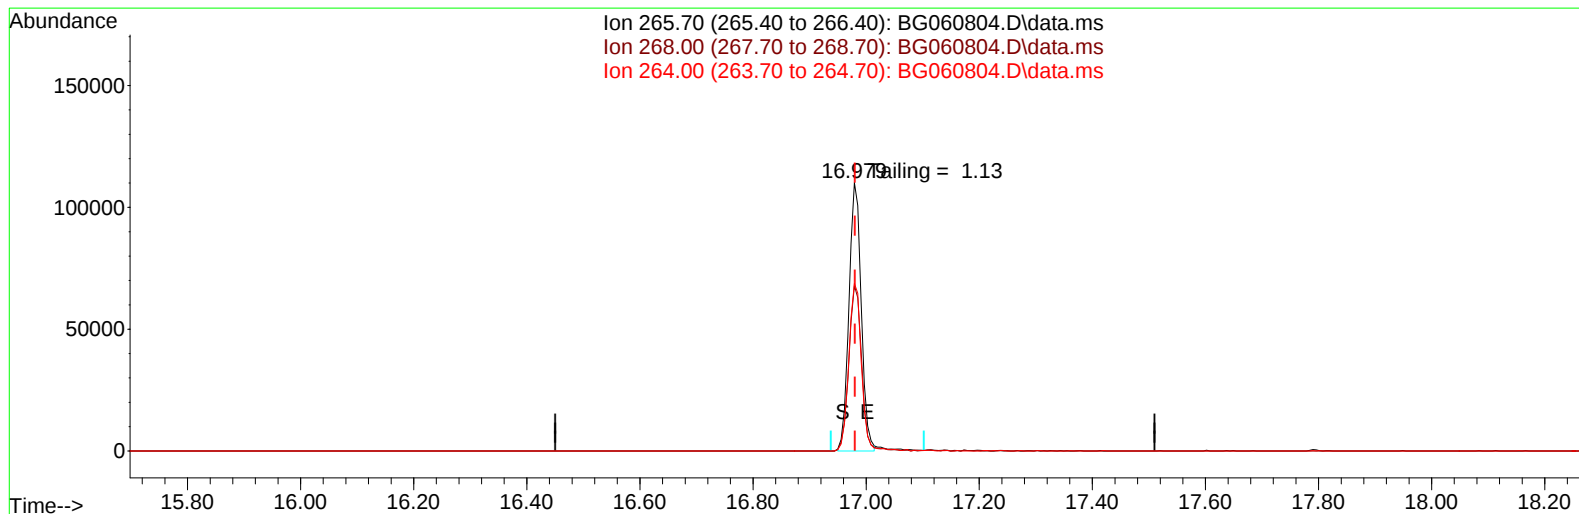

TIC: BG060804.D\data.ms

(70) Pentachlorophenol (C)

16.979min (-0.001) 29873.47 ng




response 169944

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	61.58
264.00	64.70	62.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040624\
Data File : BG060804.D
Acq On : 6 Apr 2024 9:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 06 10:35:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

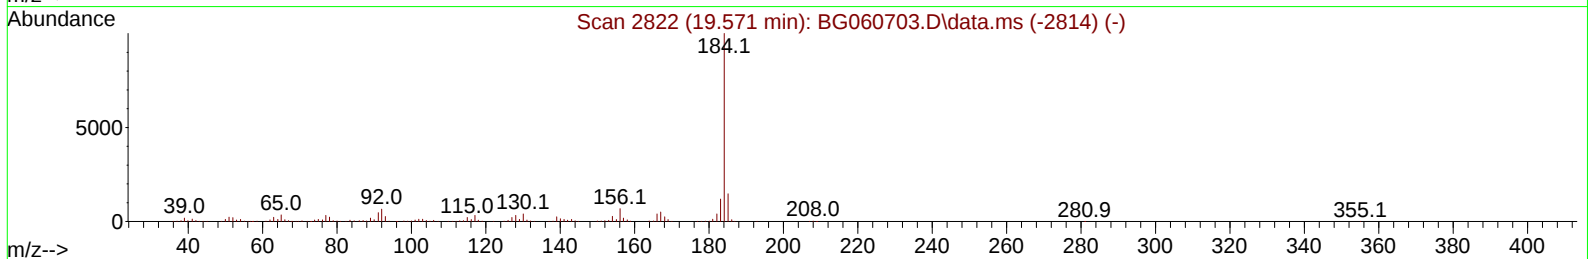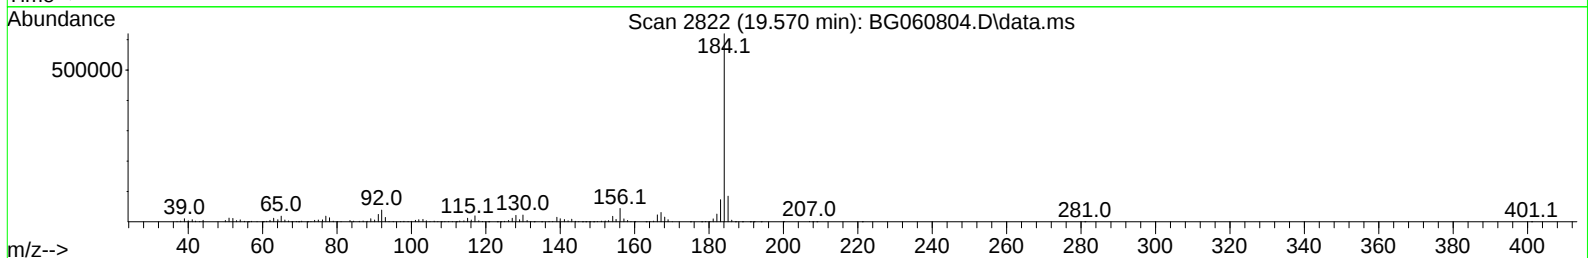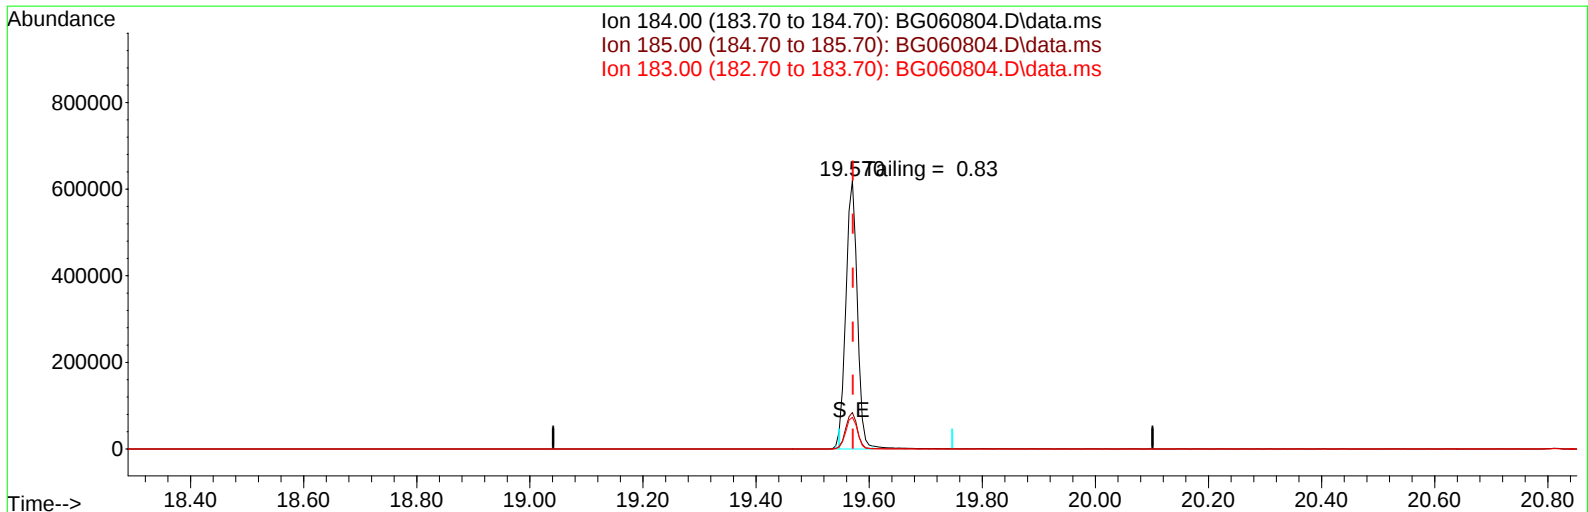

TIC: BG060804.D\data.ms

(77) Benzidine

19.570min (-0.001) 606421.48 ng

response 862293

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.64
183.00	11.90	11.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/6/2024	BNA_G	<u>BG060804.D</u>
Compound Name	Response	Retention Time
DDT	475434	20.81
DDD	14736	20.369
DDE	1678	19.864
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16414	491848	3.34

Instrument :
BNA_G
ClientSampleId :
DFTPP