

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
 Data File : BG054056.D
 Acq On : 25 Jun 2022 11:28
 Operator : CG/JU
 Sample : PB145713BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK713

Quant Time: Jun 27 01:44:59 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 15:29:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.073	152	20950	20.000	ng/u1	0.00
20) Naphthalene-d8	10.882	136	97559	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.695	164	80431	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.439	188	203446	20.000	ng/u1	0.00
79) Chrysene-d12	21.710	240	220674	20.000	ng/u1	0.00
88) Perylene-d12	24.965	264	216948	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.490	96	3258	7.399	ng/uL	-0.02
4) Pyridine-d5	3.908	84	44897	37.489	ng/u1	0.00
7) Phenol-d5	7.227	99	61296	40.840	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.392	67	35585	39.305	ng/u1	0.00
11) 2-Chlorophenol-d4	7.603	132	46811	39.112	ng/u1	0.00
15) 4-Methylphenol-d8	8.772	113	53656	41.928	ng/u1	0.00
21) Nitrobenzene-d5	9.231	128	24178	33.389	ng/u1	0.00
24) 2-Nitrophenol-d4	9.959	143	27785	36.112	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.500	165	60425	35.497	ng/u1	0.00
31) 4-Chloroaniline-d4	11.011	131	76766	35.696	ng/u1	0.00
46) Dimethylphthalate-d6	14.096	166	218486	34.530	ng/u1	0.00
49) Acenaphthylene-d8	14.389	160	241430	35.090	ng/u1	0.00
54) 4-Nitrophenol-d4	14.883	143	27830	32.122	ng/u1	0.00
60) Fluorene-d10	15.688	176	192584	33.884	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.800	200	32316	29.118	ng/u1	0.00
73) Anthracene-d10	17.539	188	329082	35.817	ng/u1	0.00
81) Pyrene-d10	19.824	212	424500	36.894	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.748	264	405697	37.047	ng/u1	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.772	70	1336	1.324 ng/u1#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054056.D
Acq On : 25 Jun 2022 11:28
Operator : CG/JU
Sample : PB145713BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK713


Quant Time: Jun 27 01:44:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 15:29:13 2022
Response via : Initial Calibration

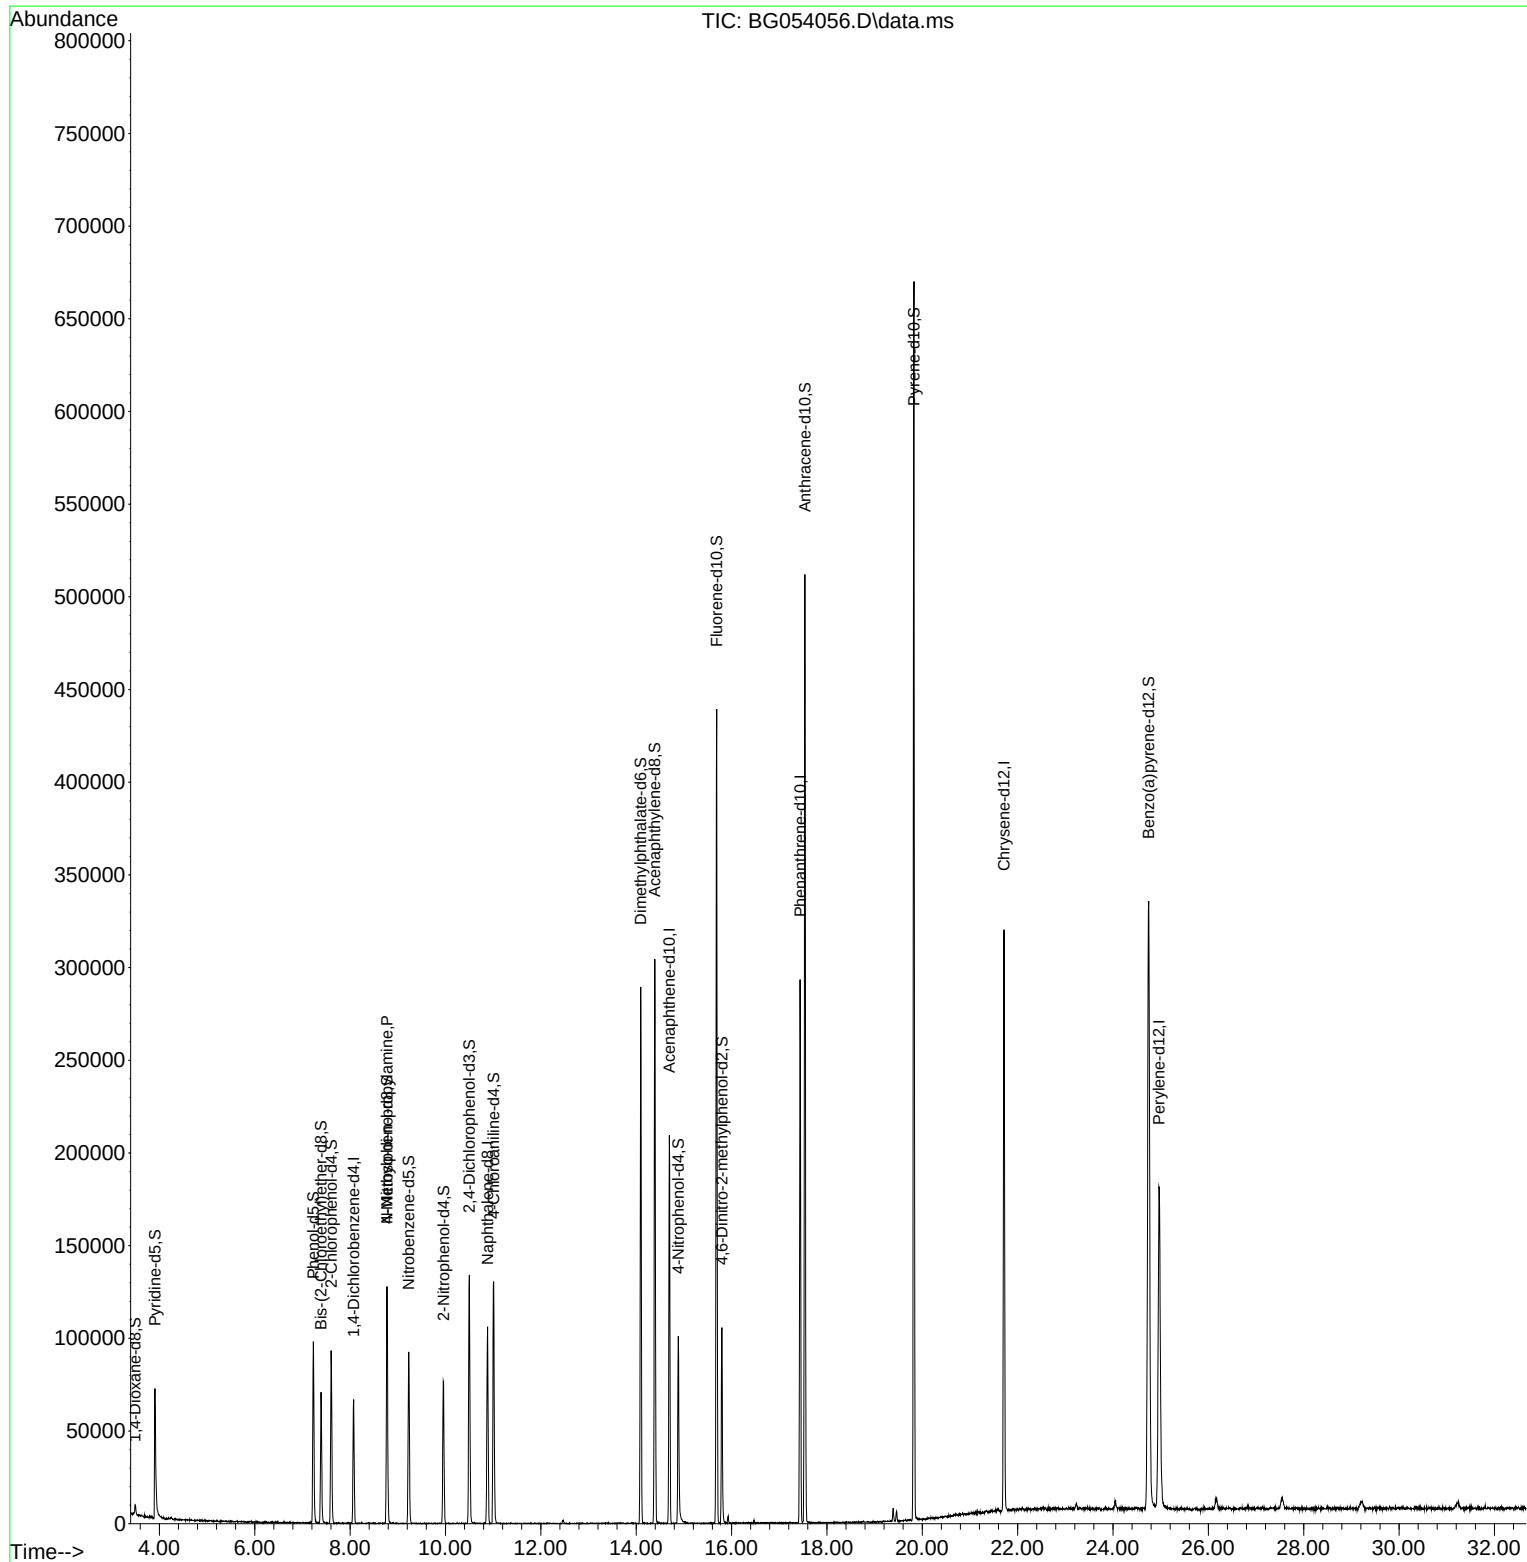

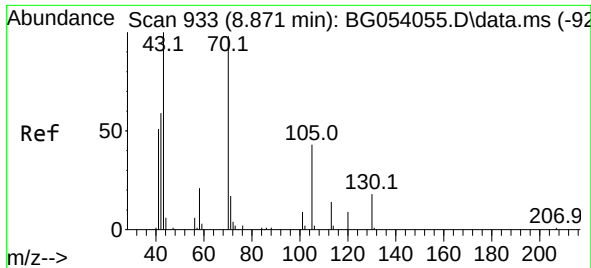

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.324 ng/ul
 RT: 8.772 min Scan# 91
 Delta R.T. -0.109 min
 Lab File: BG054056.D
 Acq: 25 Jun 2022 11:28

Instrument :
 BNA_G
 ClientSampleId :
 SBLK713

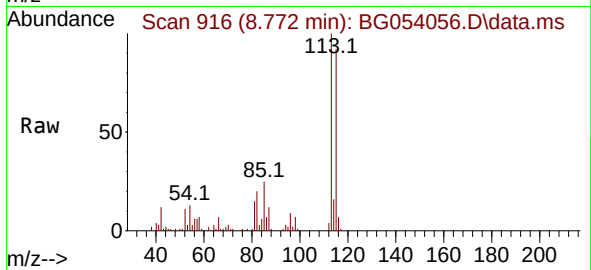

Tgt Ion:	70	Resp:	1336
Ion	Ratio	Lower	Upper
70	100		
42	401.7	50.2	75.4#
101	0.0	7.1	10.7#
130	0.0	15.5	23.3#

