

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
 Data File : BG054070.D
 Acq On : 25 Jun 2022 20:36
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020575

Quant Time: Jun 27 01:46:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 15:29:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.075	152	24085	20.000	ng/u1	0.00
20) Naphthalene-d8	10.878	136	111195	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.697	164	89430	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.441	188	225957	20.000	ng/u1	0.00
79) Chrysene-d12	21.712	240	239270	20.000	ng/u1	0.00
88) Perylene-d12	24.967	264	239347	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.493	96	4336	8.566	ng/uL	-0.01
4) Pyridine-d5	3.910	84	28268	20.531	ng/u1	0.00
7) Phenol-d5	7.229	99	38143	22.106	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.394	67	23363	22.446	ng/u1	0.00
11) 2-Chlorophenol-d4	7.605	132	29642	21.543	ng/u1	0.00
15) 4-Methylphenol-d8	8.775	113	34377	23.366	ng/u1	0.00
21) Nitrobenzene-d5	9.233	128	15639	18.948	ng/u1	0.00
24) 2-Nitrophenol-d4	9.956	143	17662	20.140	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.502	165	38828	20.012	ng/u1	0.00
31) 4-Chloroaniline-d4	11.007	131	49858	20.341	ng/u1	0.00
46) Dimethylphthalate-d6	14.098	166	127458	18.117	ng/u1	0.00
49) Acenaphthylene-d8	14.392	160	143953	18.817	ng/u1	0.00
54) 4-Nitrophenol-d4	14.885	143	18591	19.299	ng/u1	0.00
60) Fluorene-d10	15.684	176	116740	18.473	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.796	200	21925	17.787	ng/u1	0.00
73) Anthracene-d10	17.541	188	191782	18.794	ng/u1	0.00
81) Pyrene-d10	19.820	212	245053	19.643	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.744	264	230669	19.093	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.528	88	4708	8.523	ng/uL#	79
5) Pyridine	3.927	79	30531	21.383	ng/u1	95
6) Benzaldehyde	7.206	77	22469	25.572	ng/u1	90
8) Phenol	7.253	94	40739	22.628	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.482	93	29812	21.860	ng/u1	92
12) 2-Chlorophenol	7.635	128	30818	21.937	ng/u1	95
13) 2-Methylphenol	8.510	108	32400	23.183	ng/u1	94
14) 2,2'-oxybis(1-Chloropr...	8.598	45	48749	24.065	ng/u1	100
16) Acetophenone	8.892	105	50513	22.201	ng/u1	96
17) N-Nitroso-di-n-propyla...	8.874	70	26435	22.791	ng/u1	98
18) 4-Methylphenol	8.839	108	35701	23.879	ng/u1	96
19) Hexachloroethane	9.162	117	12255	20.586	ng/u1	93
22) Nitrobenzene	9.274	77	37914	19.286	ng/u1	92
23) Isophorone	9.797	82	74034	19.423	ng/u1	99
25) 2-Nitrophenol	9.991	139	18057	19.637	ng/u1	91
26) 2,4-Dimethylphenol	10.044	107	41293	20.565	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.279	93	44747	20.854	ng/u1	98
29) 2,4-Dichlorophenol	10.525	162	37764	19.463	ng/u1	98
30) Naphthalene	10.931	128	106661	19.337	ng/u1	99
32) 4-Chloroaniline	11.031	127	49749	20.468	ng/u1	96
33) Hexachlorobutadiene	11.225	225	28834	15.215	ng/u1	92
34) Caprolactam	11.777	113	11474	19.817	ng/u1	90
35) 4-Chloro-3-methylphenol	12.153	107	40951	21.947	ng/u1	96
36) 2-Methylnaphthalene	12.529	142	78936	19.345	ng/u1	96


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
 Data File : BG054070.D
 Acq On : 25 Jun 2022 20:36
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020575

Quant Time: Jun 27 01:46:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 15:29:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.746	142	79466	19.528	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.899	216	59420	16.346	ng/ul	97
40) Hexachlorocyclopentadiene	12.882	237	34491	16.918	ng/ul	96
41) 2,4,6-Trichlorophenol	13.134	196	34780	18.435	ng/ul	95
42) 2,4,5-Trichlorophenol	13.205	196	37939	17.788	ng/ul	98
43) 1,1'-Biphenyl	13.534	154	119234	19.236	ng/ul	98
44) 2-Chloronaphthalene	13.575	162	94547	18.368	ng/ul	99
45) 2-Nitroaniline	13.775	65	27972	21.601	ng/ul	97
47) Dimethylphthalate	14.145	163	123170	18.215	ng/ul	99
48) 2,6-Dinitrotoluene	14.262	165	26090	19.184	ng/ul	97
50) Acenaphthylene	14.421	152	151359	19.269	ng/ul	99
51) 3-Nitroaniline	14.591	138	23821	21.577	ng/ul#	93
52) Acenaphthene	14.762	153	100152	19.093	ng/ul	100
53) 2,4-Dinitrophenol	14.797	184	10196	16.183	ng/ul#	57
55) 4-Nitrophenol	14.897	109	16363	17.328	ng/ul	94
56) Dibenzofuran	15.097	168	151572	18.885	ng/ul	95
57) 2,4-Dinitrotoluene	15.050	165	38095	19.311	ng/ul#	97
58) 2,3,4,6-Tetrachlorophenol	15.320	232	33751	18.211	ng/ul	96
59) Diethylphthalate	15.502	149	124988	18.851	ng/ul	100
61) Fluorene	15.743	166	123591	18.907	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.731	204	70452	16.950	ng/ul	96
63) 4-Nitroaniline	15.749	138	22207	20.919	ng/ul	92
66) 4,6-Dinitro-2-methylph...	15.813	198	20937	17.695	ng/ul#	97
67) N-Nitrosodiphenylamine	15.943	169	111830	20.244	ng/ul	97
68) 4-Bromophenyl-phenylether	16.624	248	49343	17.581	ng/ul	98
69) Hexachlorobenzene	16.748	284	54458	16.555	ng/ul	98
70) Atrazine	16.889	200	49389	18.203	ng/ul	97
71) Pentachlorophenol	17.094	266	23051	16.532	ng/ul	93
72) Phenanthrene	17.482	178	217035	19.387	ng/ul	99
74) Anthracene	17.570	178	219931	19.494	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.499	216	63634	16.534	ng/ul	95
76) Pentachlorobenzene	15.020	250	59934	16.932	ng/ul	98
77) Carbazole	17.840	167	189933	20.419	ng/ul	99
78) Di-n-butylphthalate	18.399	149	224556	21.204	ng/ul	99
80) Fluoranthene	19.491	202	284176	20.405	ng/ul	97
82) Pyrene	19.850	202	278804	20.136	ng/ul	99
83) Butylbenzylphthalate	20.731	149	99056	23.739	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.607	252	99470	20.089	ng/ul	95
85) Benzo(a)anthracene	21.695	228	286619	19.434	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.601	149	142913	23.438	ng/ul	99
87) Chrysene	21.759	228	272536	19.262	ng/ul	100
89) Di-n-octyl phthalate	22.823	149	243018	23.642	ng/ul	100
90) Benzo(b)fluoranthene	23.933	252	294945	19.957	ng/ul	98
91) Benzo(k)fluoranthene	23.998	252	270878	19.141	ng/ul	98
93) Benzo(a)pyrene	24.815	252	278212	19.542	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	28.681	276	324183	18.927	ng/ul	97
95) Dibenzo(a,h)anthracene	28.745	278	271055	18.804	ng/ul	99
96) Benzo(g,h,i)perylene	29.838	276	271407	18.767	ng/ul	96





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
 1,4-Dioxane
 Concen: 8.523 ng/uL
 RT: 3.528 min Scan# 24
 Delta R.T. -0.013 min
 Lab File: BG054070.D
 Acq: 25 Jun 2022 20:36




Instrument :
 BNA_G
 ClientSampleId :
 SST020575


Tgt Ion: 88 Resp: 4708
 Ion Ratio Lower Upper
 88 100
 43 31.1 48.1 72.1#
 58 81.1 59.8 89.6



#5
 Pyridine
 Concen: 21.383 ng/uL
 RT: 3.927 min Scan# 92
 Delta R.T. -0.007 min
 Lab File: BG054070.D
 Acq: 25 Jun 2022 20:36

Tgt Ion: 79 Resp: 30531
 Ion Ratio Lower Upper
 79 100
 52 86.9 75.4 113.2
 51 44.2 35.2 52.8









#6
Benzaldehyde
Concen: 25.572 ng/ul
RT: 7.206 min Scan# 61
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion: 77 Resp: 22469
Ion Ratio Lower Upper
77 100
105 106.6 79.7 119.5
106 101.7 71.0 106.4



#8
Phenol
Concen: 22.628 ng/ul
RT: 7.253 min Scan# 658
Delta R.T. -0.002 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion: 94 Resp: 40739
Ion Ratio Lower Upper
94 100
65 32.1 24.1 36.1
66 40.3 32.5 48.7



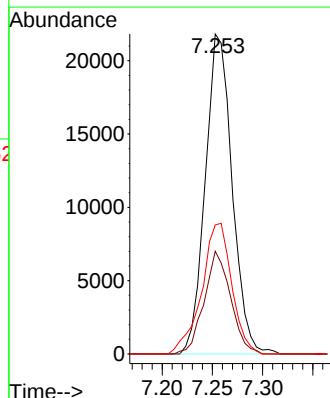





#10
Bis(2-Chloroethyl)ether
Concen: 21.860 ng/ul
RT: 7.482 min Scan# 697
Delta R.T. -0.013 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion: 93	Resp:	29812
Ion Ratio	Lower	Upper
93	100	
63	81.7	72.3 108.5
95	32.7	29.4 44.0



#12
2-Chlorophenol
Concen: 21.937 ng/ul
RT: 7.635 min Scan# 723
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion: 128	Resp:	30818
Ion Ratio	Lower	Upper
128	100	
64	48.0	41.4 62.2
130	31.2	27.0 40.6




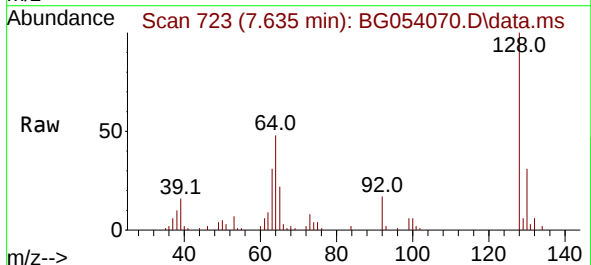




#13
2-Methylphenol
Concen: 23.183 ng/ul
RT: 8.510 min Scan# 81
Delta R.T. -0.002 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:108 Resp: 32400
Ion Ratio Lower Upper
108 100
107 88.6 75.8 113.8

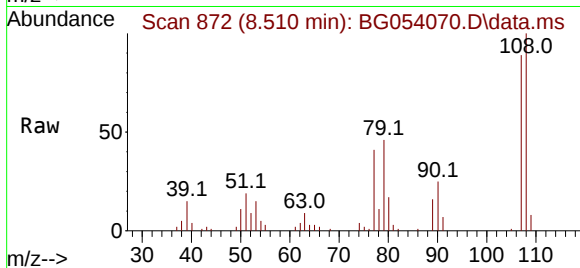

#14
2,2'-oxybis(1-Chloropropane)
Concen: 24.065 ng/ul
RT: 8.598 min Scan# 887
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion: 45 Resp: 48749
Ion Ratio Lower Upper
45 100
77 12.7 10.2 15.4
79 9.9 8.1 12.1




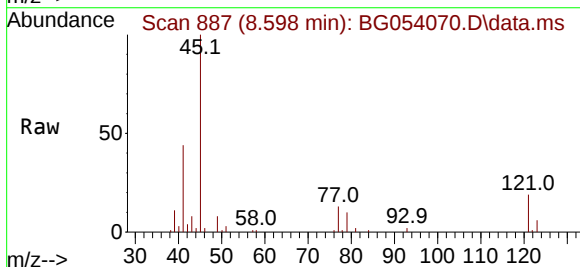




#16
Acetophenone
Concen: 22.201 ng/ul
RT: 8.892 min Scan# 913
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:105 Resp: 50513
Ion Ratio Lower Upper
105 100
77 80.7 61.0 91.6
51 27.9 22.8 34.2



#17
N-Nitroso-di-n-propylamine
Concen: 22.791 ng/ul
RT: 8.874 min Scan# 934
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion: 70 Resp: 26435
Ion Ratio Lower Upper
70 100
42 62.3 50.2 75.4
101 8.0 7.1 10.7
130 17.2 15.5 23.3



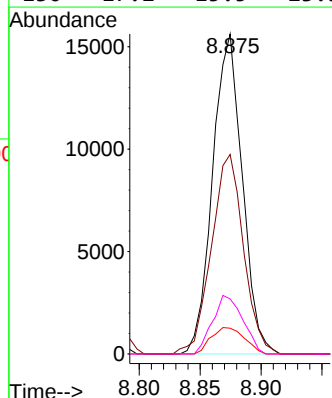





#18
4-Methylphenol
Concen: 23.879 ng/ul
RT: 8.839 min Scan# 91
Delta R.T. -0.002 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:108 Resp: 35701
Ion Ratio Lower Upper
108 100
107 109.0 90.7 136.1



#19
Hexachloroethane
Concen: 20.586 ng/ul
RT: 9.162 min Scan# 983
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:117 Resp: 12255
Ion Ratio Lower Upper
117 100
201 134.1 117.4 176.0
199 81.9 64.0 96.0









#22
Nitrobenzene
Concen: 19.286 ng/ul
RT: 9.274 min Scan# 1002
Delta R.T. -0.002 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion: 77 Resp: 37914
Ion Ratio Lower Upper
77 100
123 45.0 31.2 46.8
65 11.7 10.5 15.7



#23
Isophorone
Concen: 19.423 ng/ul
RT: 9.797 min Scan# 1091
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion: 82 Resp: 74034
Ion Ratio Lower Upper
82 100
95 8.1 6.1 9.1
138 17.5 13.6 20.4




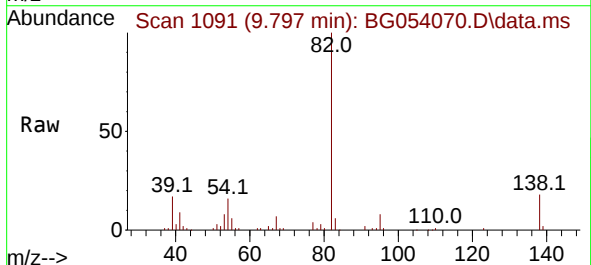




#25
2-Nitrophenol
Concen: 19.637 ng/ul
RT: 9.991 min Scan# 1124
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:139 Resp: 18057
Ion Ratio Lower Upper
139 100
65 49.7 47.7 71.5
109 34.6 27.1 40.7

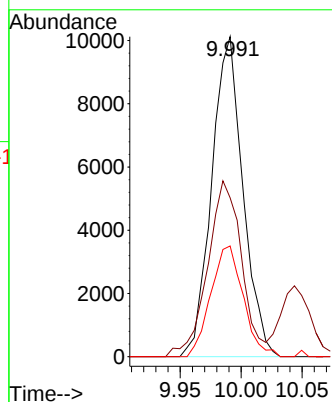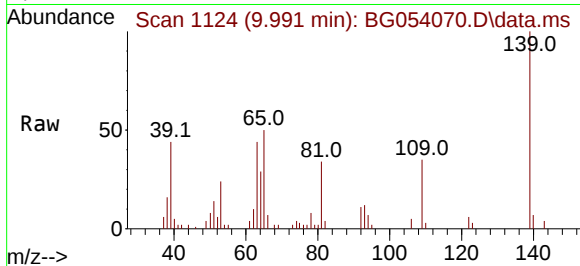

#26
2,4-Dimethylphenol
Concen: 20.565 ng/ul
RT: 10.044 min Scan# 1133
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:107 Resp: 41293
Ion Ratio Lower Upper
107 100
121 48.3 39.9 59.9
122 82.9 66.7 100.1

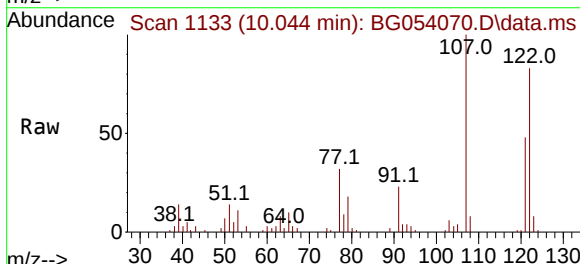



#27

Bis(2-Chloroethoxy)methane

Concen: 20.854 ng/ul

RT: 10.279 min Scan# 1172

Delta R.T. -0.007 min

Lab File: BG054070.D

Acq: 25 Jun 2022 20:36

Instrument :

BNA_G

ClientSampleId :

SSTD020575





Tgt Ion: 93 Resp: 44747

Ion Ratio Lower Upper

93 100

95 32.3 26.5 39.7

123 10.2 8.8 13.2

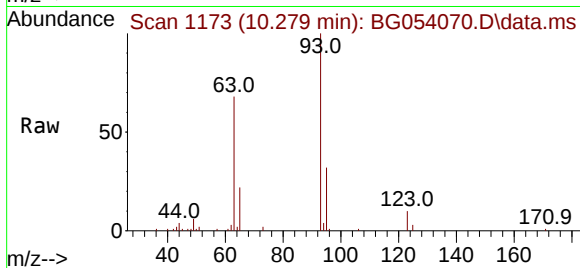

#29

2,4-Dichlorophenol

Concen: 19.463 ng/ul

RT: 10.525 min Scan# 1215

Delta R.T. -0.007 min

Lab File: BG054070.D

Acq: 25 Jun 2022 20:36




Tgt Ion: 162 Resp: 37764


Ion Ratio Lower Upper

162 100

164 62.3 50.9 76.3

98 33.7 28.5 42.7




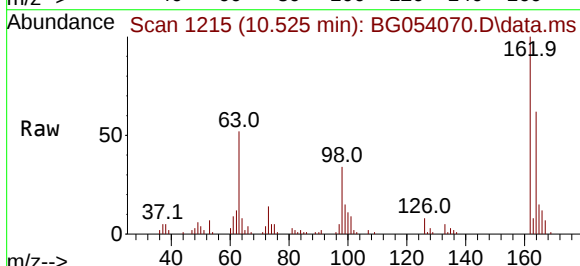




#30
Naphthalene
Concen: 19.337 ng/ul
RT: 10.931 min Scan# 1284
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:128 Resp: 106661
Ion Ratio Lower Upper
128 100
129 11.5 9.0 13.6
127 13.0 11.1 16.7



#32
4-Chloroaniline
Concen: 20.468 ng/ul
RT: 11.031 min Scan# 1301
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:127 Resp: 49749
Ion Ratio Lower Upper
127 100
129 29.5 25.4 38.2









#33
Hexachlorobutadiene
Concen: 15.215 ng/ul
RT: 11.225 min Scan# 11
Delta R.T. -0.002 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:225 Resp: 28834
Ion Ratio Lower Upper
225 100
223 57.8 50.2 75.2
227 57.0 51.8 77.6



#34
Caprolactam
Concen: 19.817 ng/ul
RT: 11.777 min Scan# 1428
Delta R.T. -0.013 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:113 Resp: 11474
Ion Ratio Lower Upper
113 100
55 204.7 167.8 251.6
56 135.3 127.6 191.4


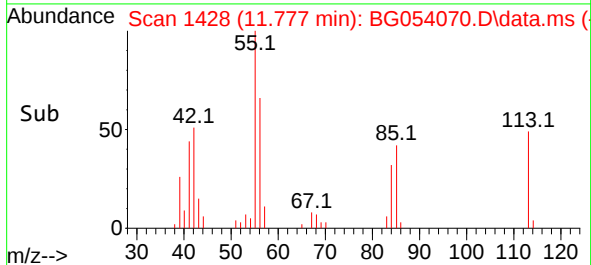






#35
4-Chloro-3-methylphenol
Concen: 21.947 ng/ul
RT: 12.153 min Scan# 1491
Delta R.T. -0.002 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:	107	Resp:	40951
Ion	Ratio	Lower	Upper
107	100		
144	25.9	21.3	31.9
142	76.5	65.0	97.4

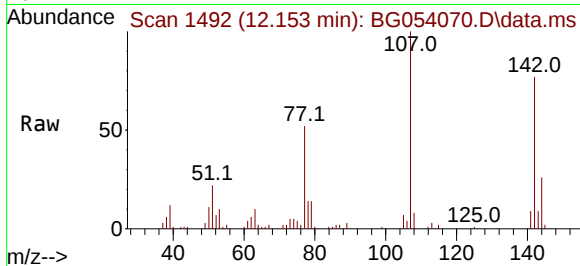

#36
2-Methylnaphthalene
Concen: 19.345 ng/ul
RT: 12.529 min Scan# 1556
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:	142	Resp:	78936
Ion	Ratio	Lower	Upper
142	100		
141	91.3	76.3	114.5




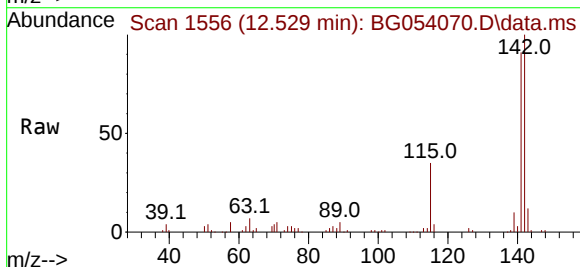


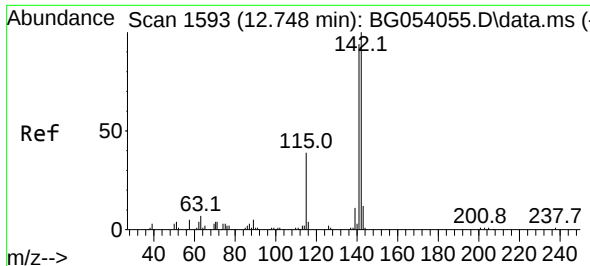

#37
1-Methylnaphthalene
Concen: 19.528 ng/ul
RT: 12.746 min Scan# 11
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:142 Resp: 79466
Ion Ratio Lower Upper
142 100
141 93.1 73.4 110.2
116 4.2 3.2 4.8

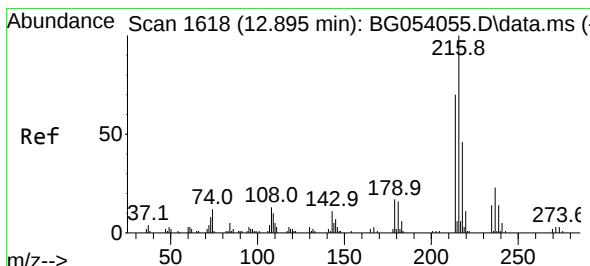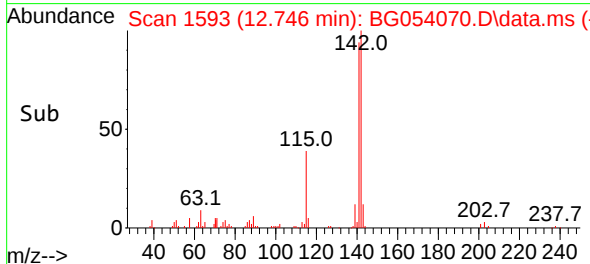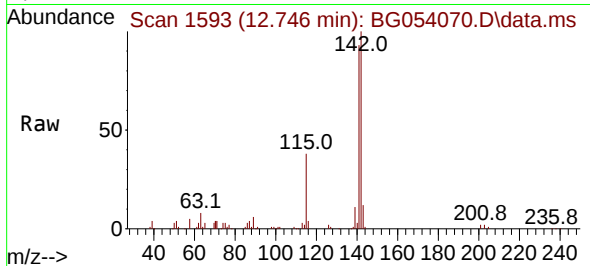

#39
1,2,4,5-Tetrachlorobenzene
Concen: 16.346 ng/ul
RT: 12.899 min Scan# 1619
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:216 Resp: 59420
Ion Ratio Lower Upper
216 100
214 74.7 58.1 87.1
179 17.0 14.8 22.2
108 11.5 10.4 15.6


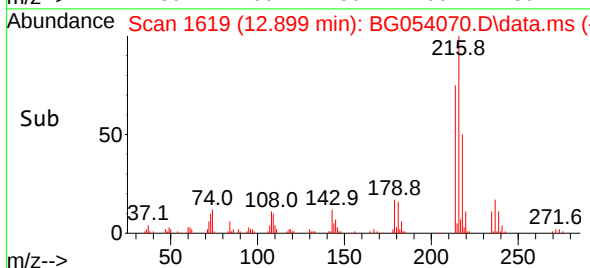
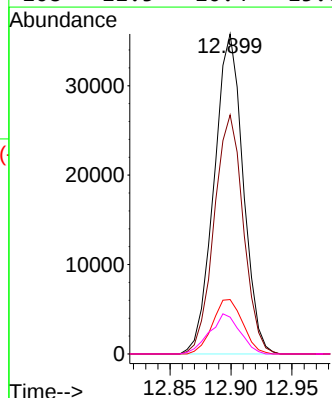
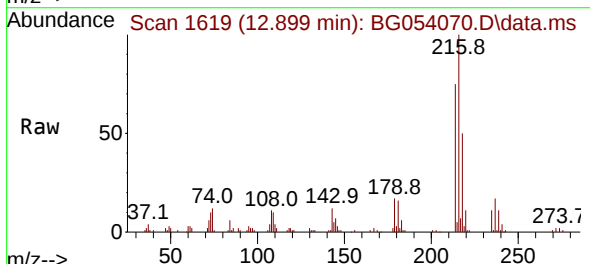




#40
Hexachlorocyclopentadiene
Concen: 16.918 ng/ul
RT: 12.882 min Scan# 1616
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:237 Resp: 34491
Ion Ratio Lower Upper
237 100
235 55.8 47.0 70.6
272 12.7 8.6 12.8



#41
2,4,6-Trichlorophenol
Concen: 18.435 ng/ul
RT: 13.134 min Scan# 1659
Delta R.T. -0.002 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:196 Resp: 34780
Ion Ratio Lower Upper
196 100
198 96.4 81.9 122.9
200 33.4 25.7 38.5

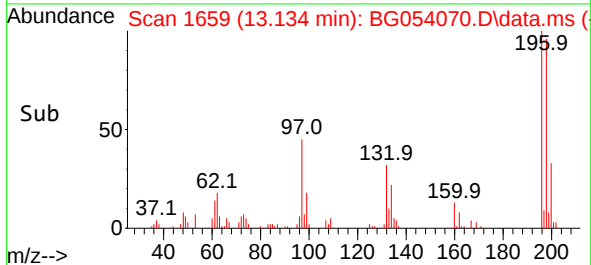



#42
2,4,5-Trichlorophenol
Concen: 17.788 ng/ul
RT: 13.205 min Scan# 1
Delta R.T. -0.002 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36





Instrument :

BNA_G

ClientSampleId :




SSTD020575


Tgt Ion:196 Resp: 37939
Ion Ratio Lower Upper
196 100
198 96.3 76.3 114.5
200 33.9 25.5 38.3



#43
1,1'-Biphenyl
Concen: 19.236 ng/ul
RT: 13.534 min Scan# 1727
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:154 Resp: 119234
Ion Ratio Lower Upper
154 100
153 39.5 32.7 49.1
76 10.6 9.0 13.6


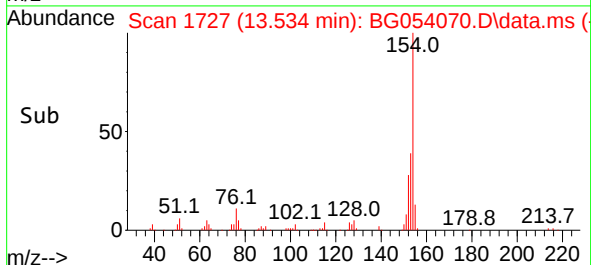
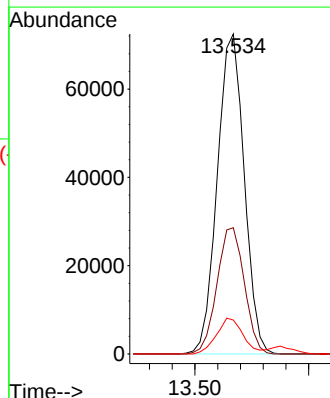





#44
2-Chloronaphthalene
Concen: 18.368 ng/ul
RT: 13.575 min Scan# 1734
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:162 Resp: 94547
Ion Ratio Lower Upper
162 100
164 32.5 25.7 38.5
127 35.8 28.3 42.5

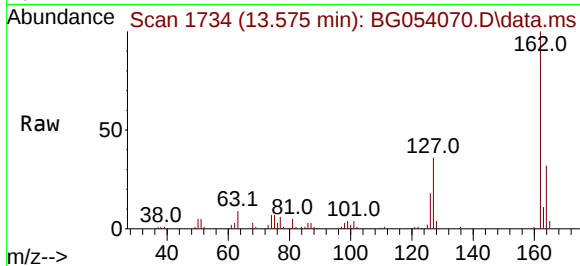

#45
2-Nitroaniline
Concen: 21.601 ng/ul
RT: 13.775 min Scan# 1768
Delta R.T. -0.002 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion: 65 Resp: 27972
Ion Ratio Lower Upper
65 100
92 62.8 52.2 78.4
138 100.8 79.0 118.4




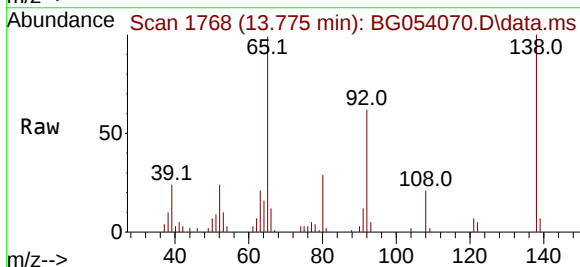




#47
Dimethylphthalate
Concen: 18.215 ng/ul
RT: 14.145 min Scan# 1831
Delta R.T. -0.002 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:163 Resp: 123170
Ion Ratio Lower Upper
163 100
194 4.1 3.7 5.5
164 10.0 7.9 11.9

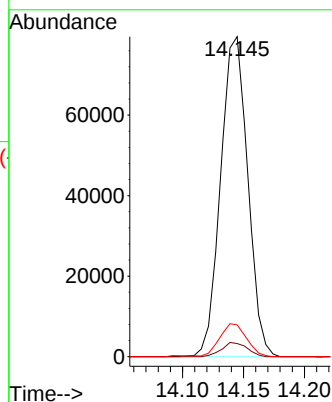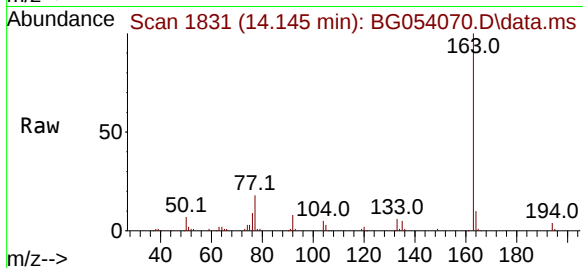

#48
2,6-Dinitrotoluene
Concen: 19.184 ng/ul
RT: 14.262 min Scan# 1851
Delta R.T. -0.002 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:165 Resp: 26090
Ion Ratio Lower Upper
165 100
89 53.9 44.7 67.1
121 19.1 16.9 25.3



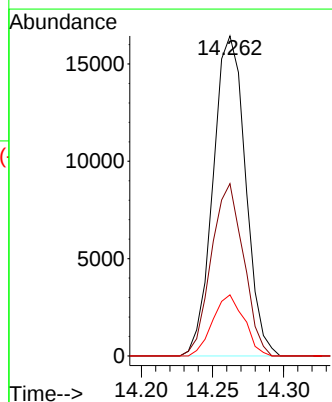
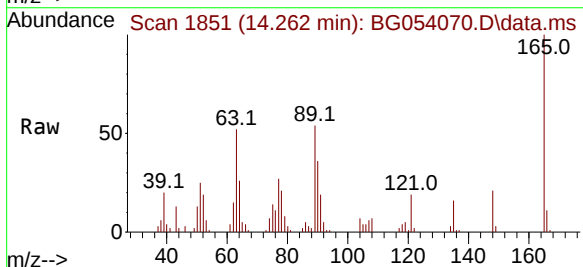




#50
Acenaphthylene
Concen: 19.269 ng/ul
RT: 14.421 min Scan# 11
Delta R.T. -0.002 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:152 Resp: 151359
Ion Ratio Lower Upper
152 100
151 20.3 16.2 24.2
153 13.5 10.5 15.7



#51
3-Nitroaniline
Concen: 21.577 ng/ul
RT: 14.591 min Scan# 1907
Delta R.T. -0.002 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:138 Resp: 23821
Ion Ratio Lower Upper
138 100
108 10.0 17.8 26.6#
92 114.4 94.2 141.4


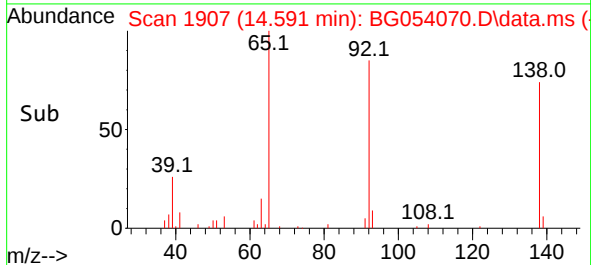






#52
Acenaphthene
Concen: 19.093 ng/ul
RT: 14.762 min Scan# 1936
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:153 Resp: 100152
Ion Ratio Lower Upper
153 100
152 46.3 37.5 56.3
154 85.8 68.8 103.2



#53
2,4-Dinitrophenol
Concen: 16.183 ng/ul
RT: 14.797 min Scan# 1942
Delta R.T. -0.002 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:184 Resp: 10196
Ion Ratio Lower Upper
184 100
63 53.1 34.7 52.1#
154 52.5 87.3 130.9#









#55
4-Nitrophenol
Concen: 17.328 ng/ul
RT: 14.897 min Scan# 1959
Delta R.T. 0.004 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:	109	Resp:	16363
Ion	Ratio	Lower	Upper
109	100		
139	116.8	92.9	139.3
65	134.4	97.8	146.6

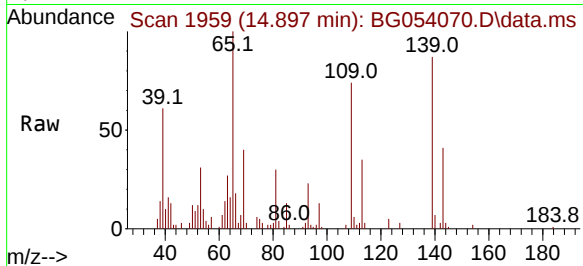

#56
Dibenzofuran
Concen: 18.885 ng/ul
RT: 15.097 min Scan# 1993
Delta R.T. -0.002 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:	168	Resp:	151572
Ion	Ratio	Lower	Upper
168	100		
139	32.4	28.2	42.2




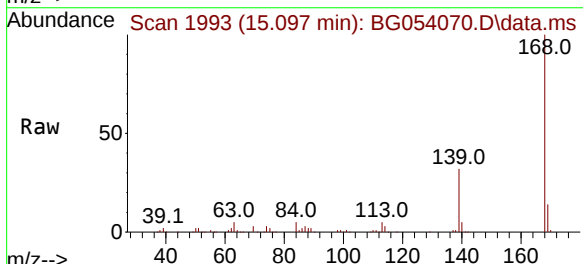




#57
2,4-Dinitrotoluene
Concen: 19.311 ng/ul
RT: 15.050 min Scan# 1984
Delta R.T. -0.002 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:165 Resp: 38095
Ion Ratio Lower Upper
165 100
63 39.6 33.0 49.4
182 1.9 2.8 4.2#



#58
2,3,4,6-Tetrachlorophenol
Concen: 18.211 ng/ul
RT: 15.320 min Scan# 2031
Delta R.T. -0.002 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:232 Resp: 33751
Ion Ratio Lower Upper
232 100
131 30.7 27.5 41.3
130 2.3 1.8 2.8
166 25.6 20.7 31.1



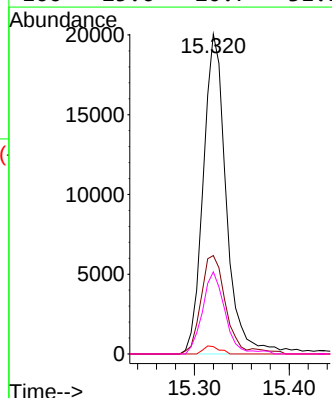





#59
Diethylphthalate
Concen: 18.851 ng/ul
RT: 15.502 min Scan# 2062
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:149 Resp: 124988
Ion Ratio Lower Upper
149 100
177 23.8 18.9 28.3
150 13.1 10.6 15.8



#61
Fluorene
Concen: 18.907 ng/ul
RT: 15.743 min Scan# 2103
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:166 Resp: 123591
Ion Ratio Lower Upper
166 100
165 101.3 81.7 122.5
167 13.8 11.0 16.4




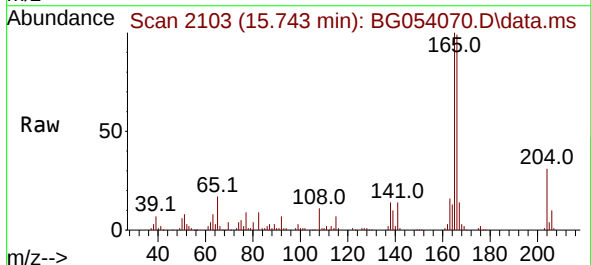




#62
4-Chlorophenyl-phenylether
Concen: 16.950 ng/ul
RT: 15.731 min Scan# 2101
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:204 Resp: 70452
Ion Ratio Lower Upper
204 100
206 32.6 27.1 40.7
141 47.3 40.7 61.1



#63
4-Nitroaniline
Concen: 20.919 ng/ul
RT: 15.749 min Scan# 2104
Delta R.T. -0.002 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:138 Resp: 22207
Ion Ratio Lower Upper
138 100
92 50.4 42.0 63.0
108 88.1 79.0 118.6









#66
4,6-Dinitro-2-methylphenol
Concen: 17.695 ng/ul
RT: 15.813 min Scan# 2115
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:198 Resp: 20937
Ion Ratio Lower Upper
198 100
182 5.2 3.4 5.0#
77 19.9 14.7 22.1

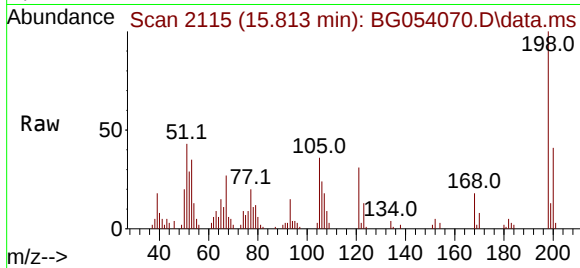

#67
N-Nitrosodiphenylamine
Concen: 20.244 ng/ul
RT: 15.943 min Scan# 2137
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:169 Resp: 111830
Ion Ratio Lower Upper
169 100
168 66.8 51.0 76.4
167 37.4 28.7 43.1




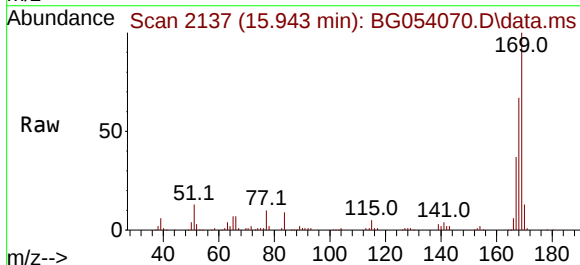




#68
4-Bromophenyl-phenylether
Concen: 17.581 ng/ul
RT: 16.624 min Scan# 21
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:248 Resp: 49343
Ion Ratio Lower Upper
248 100
250 100.3 78.2 117.2
141 56.9 46.7 70.1

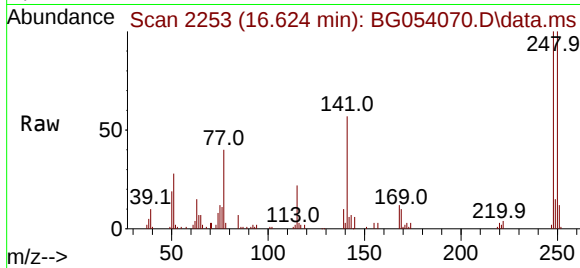

#69
Hexachlorobenzene
Concen: 16.555 ng/ul
RT: 16.748 min Scan# 2274
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:284 Resp: 54458
Ion Ratio Lower Upper
284 100
142 24.2 20.8 31.2
249 33.4 27.4 41.0




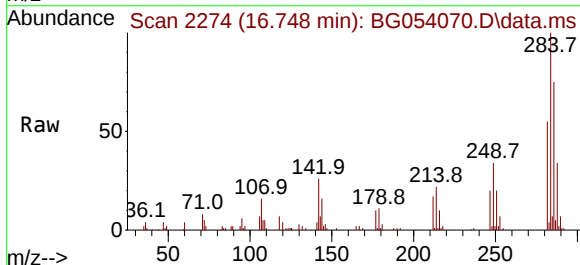




#70
 Atrazine
 Concen: 18.203 ng/ul
 RT: 16.889 min Scan# 21
 Delta R.T. -0.002 min
 Lab File: BG054070.D
 Acq: 25 Jun 2022 20:36




Instrument :
 BNA_G
 ClientSampleId :
 SST020575


Tgt Ion:200 Resp: 49389
 Ion Ratio Lower Upper
 200 100
 173 23.2 19.8 29.6
 215 50.7 38.8 58.2

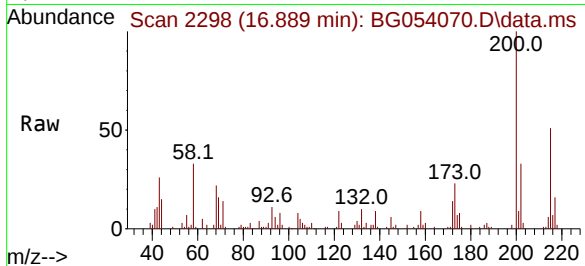

#71
 Pentachlorophenol
 Concen: 16.532 ng/ul
 RT: 17.094 min Scan# 2333
 Delta R.T. -0.002 min
 Lab File: BG054070.D
 Acq: 25 Jun 2022 20:36

Tgt Ion:266 Resp: 23051
 Ion Ratio Lower Upper
 266 100
 264 71.1 56.8 85.2
 268 71.4 48.0 72.0




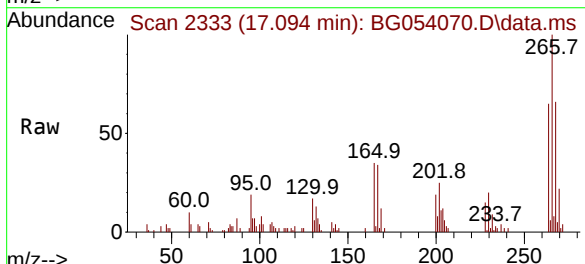




#72
Phenanthrene
Concen: 19.387 ng/ul
RT: 17.482 min Scan# 217035
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:178 Resp: 217035
Ion Ratio Lower Upper
178 100
179 15.0 12.6 19.0
176 19.1 15.7 23.5



#74
Anthracene
Concen: 19.494 ng/ul
RT: 17.570 min Scan# 2414
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:178 Resp: 219931
Ion Ratio Lower Upper
178 100
179 14.7 12.4 18.6
176 18.9 14.6 22.0


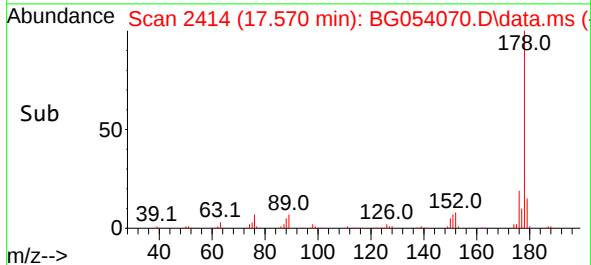






#75
1,2,3,4-Tetrachlorobenzene
Concen: 16.534 ng/uL
RT: 13.499 min Scan# 11
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:216 Resp: 63634
Ion Ratio Lower Upper
216 100
214 73.2 64.2 96.4
218 49.1 39.0 58.4



#76
Pentachlorobenzene
Concen: 16.932 ng/uL
RT: 15.020 min Scan# 1980
Delta R.T. -0.002 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:250 Resp: 59934
Ion Ratio Lower Upper
250 100
248 59.3 47.7 71.5
252 65.0 50.0 75.0









#77
 Carbazole
 Concen: 20.419 ng/ul
 RT: 17.840 min Scan# 2459
 Delta R.T. -0.002 min
 Lab File: BG054070.D
 Acq: 25 Jun 2022 20:36




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020575


Tgt Ion:167 Resp: 189933
 Ion Ratio Lower Upper
 167 100
 166 23.0 18.2 27.2
 139 10.9 9.0 13.6



#78
 Di-n-butylphthalate
 Concen: 21.204 ng/ul
 RT: 18.399 min Scan# 2555
 Delta R.T. -0.007 min
 Lab File: BG054070.D
 Acq: 25 Jun 2022 20:36

Tgt Ion:149 Resp: 224556
 Ion Ratio Lower Upper
 149 100
 150 9.1 7.1 10.7
 104 4.8 4.2 6.2




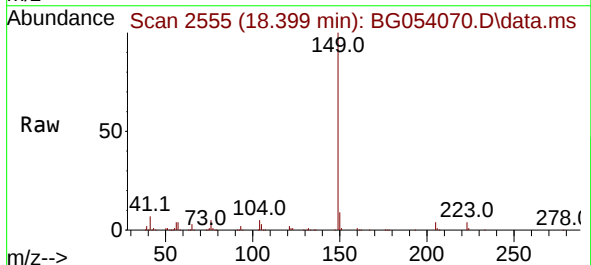




#80
 Fluoranthene
 Concen: 20.405 ng/u1
 RT: 19.491 min Scan# 21
 Delta R.T. -0.002 min
 Lab File: BG054070.D
 Acq: 25 Jun 2022 20:36




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020575


Tgt Ion:202 Resp: 284176
 Ion Ratio Lower Upper
 202 100
 101 7.4 6.6 9.8
 100 6.1 5.8 8.8



#82
 Pyrene
 Concen: 20.136 ng/u1
 RT: 19.850 min Scan# 2802
 Delta R.T. -0.007 min
 Lab File: BG054070.D
 Acq: 25 Jun 2022 20:36

Tgt Ion:202 Resp: 278804
 Ion Ratio Lower Upper
 202 100
 101 9.6 7.3 10.9
 100 8.0 6.2 9.4







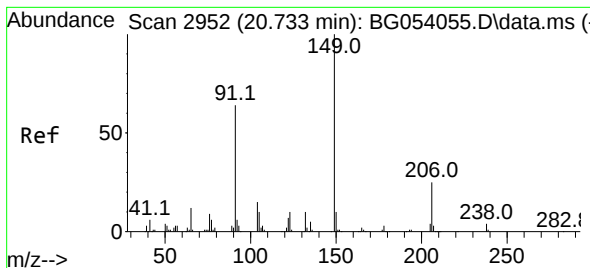

#83
 Butylbenzylphthalate
 Concen: 23.739 ng/ul
 RT: 20.731 min Scan# 2952
 Delta R.T. -0.007 min
 Lab File: BG054070.D
 Acq: 25 Jun 2022 20:36




Instrument :
 BNA_G
 ClientSampleId :
 SST020575


Tgt Ion:	149	Resp:	99056
Ion	Ratio	Lower	Upper
149	100		
91	66.4	54.0	81.0
206	25.6	19.5	29.3

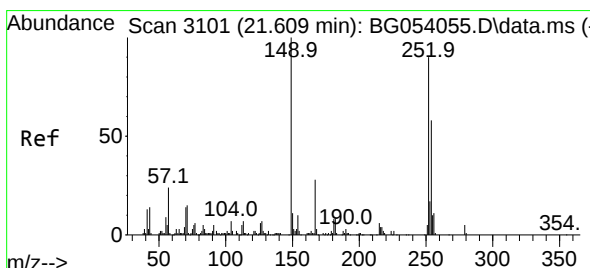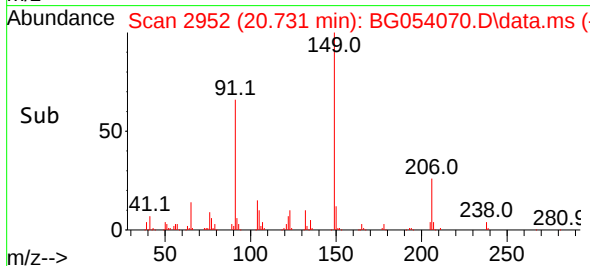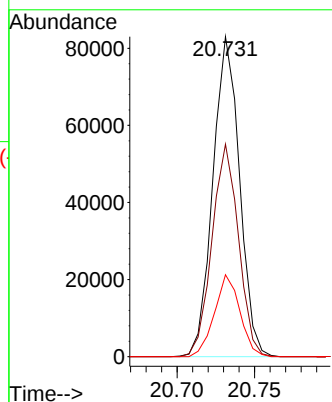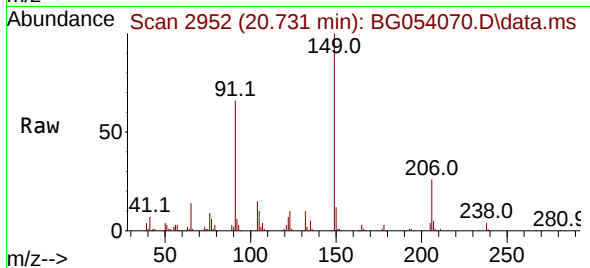

#84
 3,3'-Dichlorobenzidine
 Concen: 20.089 ng/ul
 RT: 21.607 min Scan# 3101
 Delta R.T. -0.007 min
 Lab File: BG054070.D
 Acq: 25 Jun 2022 20:36

Tgt Ion:	252	Resp:	99470
Ion	Ratio	Lower	Upper
252	100		
254	66.3	49.6	74.4
126	7.6	6.0	9.0


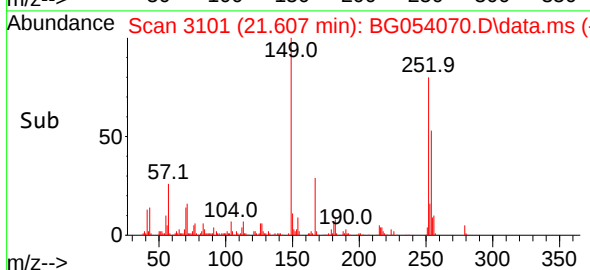

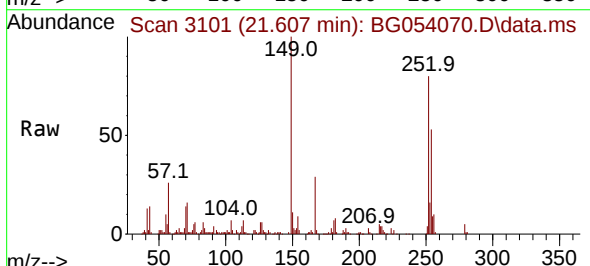




#85
Benzo(a)anthracene
Concen: 19.434 ng/ul
RT: 21.695 min Scan# 3116
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:228 Resp: 286619
Ion Ratio Lower Upper
228 100
229 20.0 16.5 24.7
226 27.0 22.1 33.1

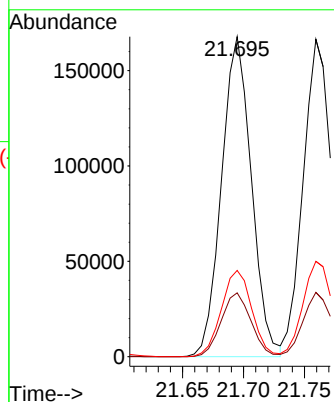

#86
Bis(2-ethylhexyl)phthalate
Concen: 23.438 ng/ul
RT: 21.601 min Scan# 3100
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:149 Resp: 142913
Ion Ratio Lower Upper
149 100
167 26.4 21.7 32.5
279 4.9 3.9 5.9



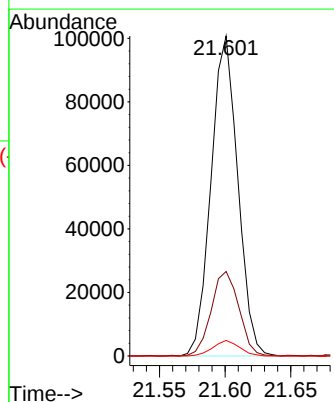



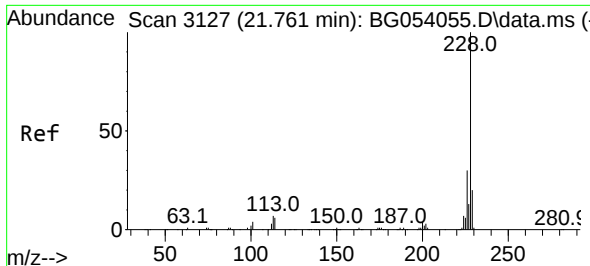

#87
Chrysene
Concen: 19.262 ng/ul
RT: 21.759 min Scan# 3127
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:228 Resp: 272536
Ion Ratio Lower Upper
228 100
226 30.0 24.2 36.4
229 20.2 16.3 24.5

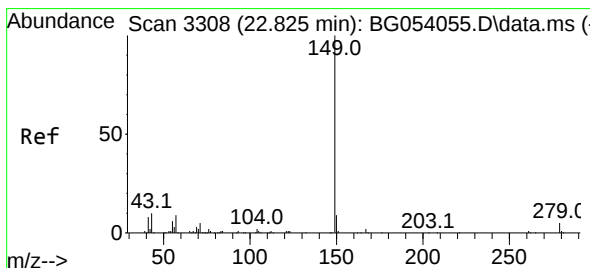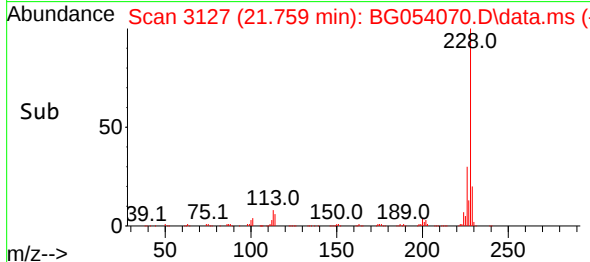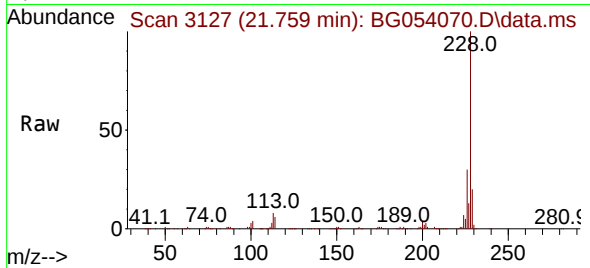

#89
Di-n-octyl phthalate
Concen: 23.642 ng/ul
RT: 22.823 min Scan# 3308
Delta R.T. -0.013 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:149 Resp: 243018


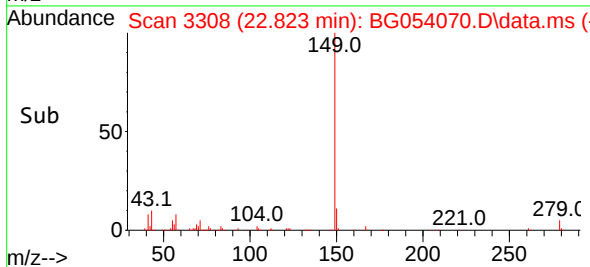

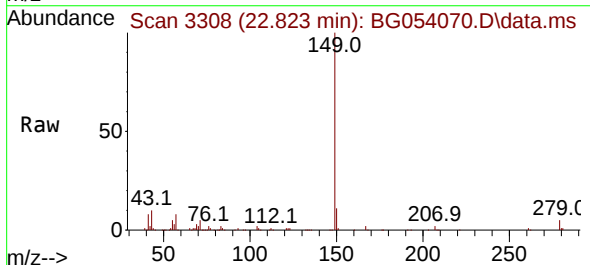




#90
Benzo(b)fluoranthene
Concen: 19.957 ng/ul
RT: 23.933 min Scan# 3497
Delta R.T. -0.007 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36




Instrument :
BNA_G
ClientSampleId :
SSTD020575


Tgt Ion:252 Resp: 294945
Ion Ratio Lower Upper
252 100
253 21.7 18.2 27.4
125 6.6 6.1 9.1



#91
Benzo(k)fluoranthene
Concen: 19.141 ng/ul
RT: 23.998 min Scan# 3508
Delta R.T. -0.019 min
Lab File: BG054070.D
Acq: 25 Jun 2022 20:36

Tgt Ion:252 Resp: 270878
Ion Ratio Lower Upper
252 100
253 21.1 17.4 26.2
125 7.3 5.4 8.0





#93

Benzo(a)pyrene

Concen: 19.542 ng/ul

RT: 24.815 min Scan# 3647

Delta R.T. -0.013 min

Lab File: BG054070.D

Acq: 25 Jun 2022 20:36

Instrument :

BNA_G

ClientSampleId :

SSTD020575





Tgt Ion:252 Resp: 278212

Ion Ratio Lower Upper

252 100

253 22.2 17.6 26.4

125 7.4 6.8 10.2

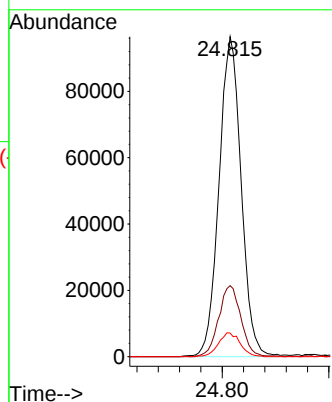

#94

Indeno(1,2,3-cd)pyrene

Concen: 18.927 ng/ul

RT: 28.681 min Scan# 4305

Delta R.T. -0.019 min

Lab File: BG054070.D

Acq: 25 Jun 2022 20:36




Tgt Ion:276 Resp: 324183


Ion Ratio Lower Upper

276 100

138 12.4 10.1 15.1

277 22.7 19.9 29.9









#95
 Dibenzo(a,h)anthracene
 Concen: 18.804 ng/ul
 RT: 28.745 min Scan# 41
 Delta R.T. -0.019 min
 Lab File: BG054070.D
 Acq: 25 Jun 2022 20:36

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020575

Tgt Ion:278 Resp: 271055
 Ion Ratio Lower Upper
 278 100
 139 10.5 8.6 13.0
 279 24.6 19.4 29.0

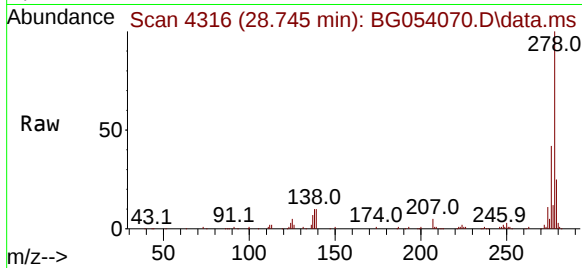

#96
 Benzo(g,h,i)perylene
 Concen: 18.767 ng/ul
 RT: 29.838 min Scan# 4502
 Delta R.T. -0.019 min
 Lab File: BG054070.D
 Acq: 25 Jun 2022 20:36

Tgt Ion:276 Resp: 271407
 Ion Ratio Lower Upper
 276 100
 138 12.3 11.3 16.9
 277 25.1 18.6 27.8

