

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062622\
 Data File : BG054073.D
 Acq On : 26 Jun 2022 15:16
 Operator : CG/JU
 Sample : PB145765TB
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB145765TB

Quant Time: Jun 27 00:29:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 27 00:27:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.071	152	23917	20.000	ng	0.00
21) Naphthalene-d8	10.879	136	106774	20.000	ng	0.00
39) Acenaphthene-d10	14.693	164	87285	20.000	ng	0.00
64) Phenanthrene-d10	17.436	188	227313	20.000	ng	0.00
76) Chrysene-d12	21.714	240	249220	20.000	ng	0.00
86) Perylene-d12	24.969	264	248653	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.638	112	197448	157.839	ng	0.00
7) Phenol-d6	7.231	99	276758	163.086	ng	0.00
23) Nitrobenzene-d5	9.228	82	174337	91.755	ng	0.00
42) 2,4,6-Tribromophenol	16.179	330	161915	115.457	ng	0.00
45) 2-Fluorobiphenyl	13.324	172	509819	84.934	ng	0.00
79) Terphenyl-d14	20.045	244	1117478	90.309	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062622\
Data File : BG054073.D
Acq On : 26 Jun 2022 15:16
Operator : CG/JU
Sample : PB145765TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB145765TB

Quant Time: Jun 27 00:29:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration




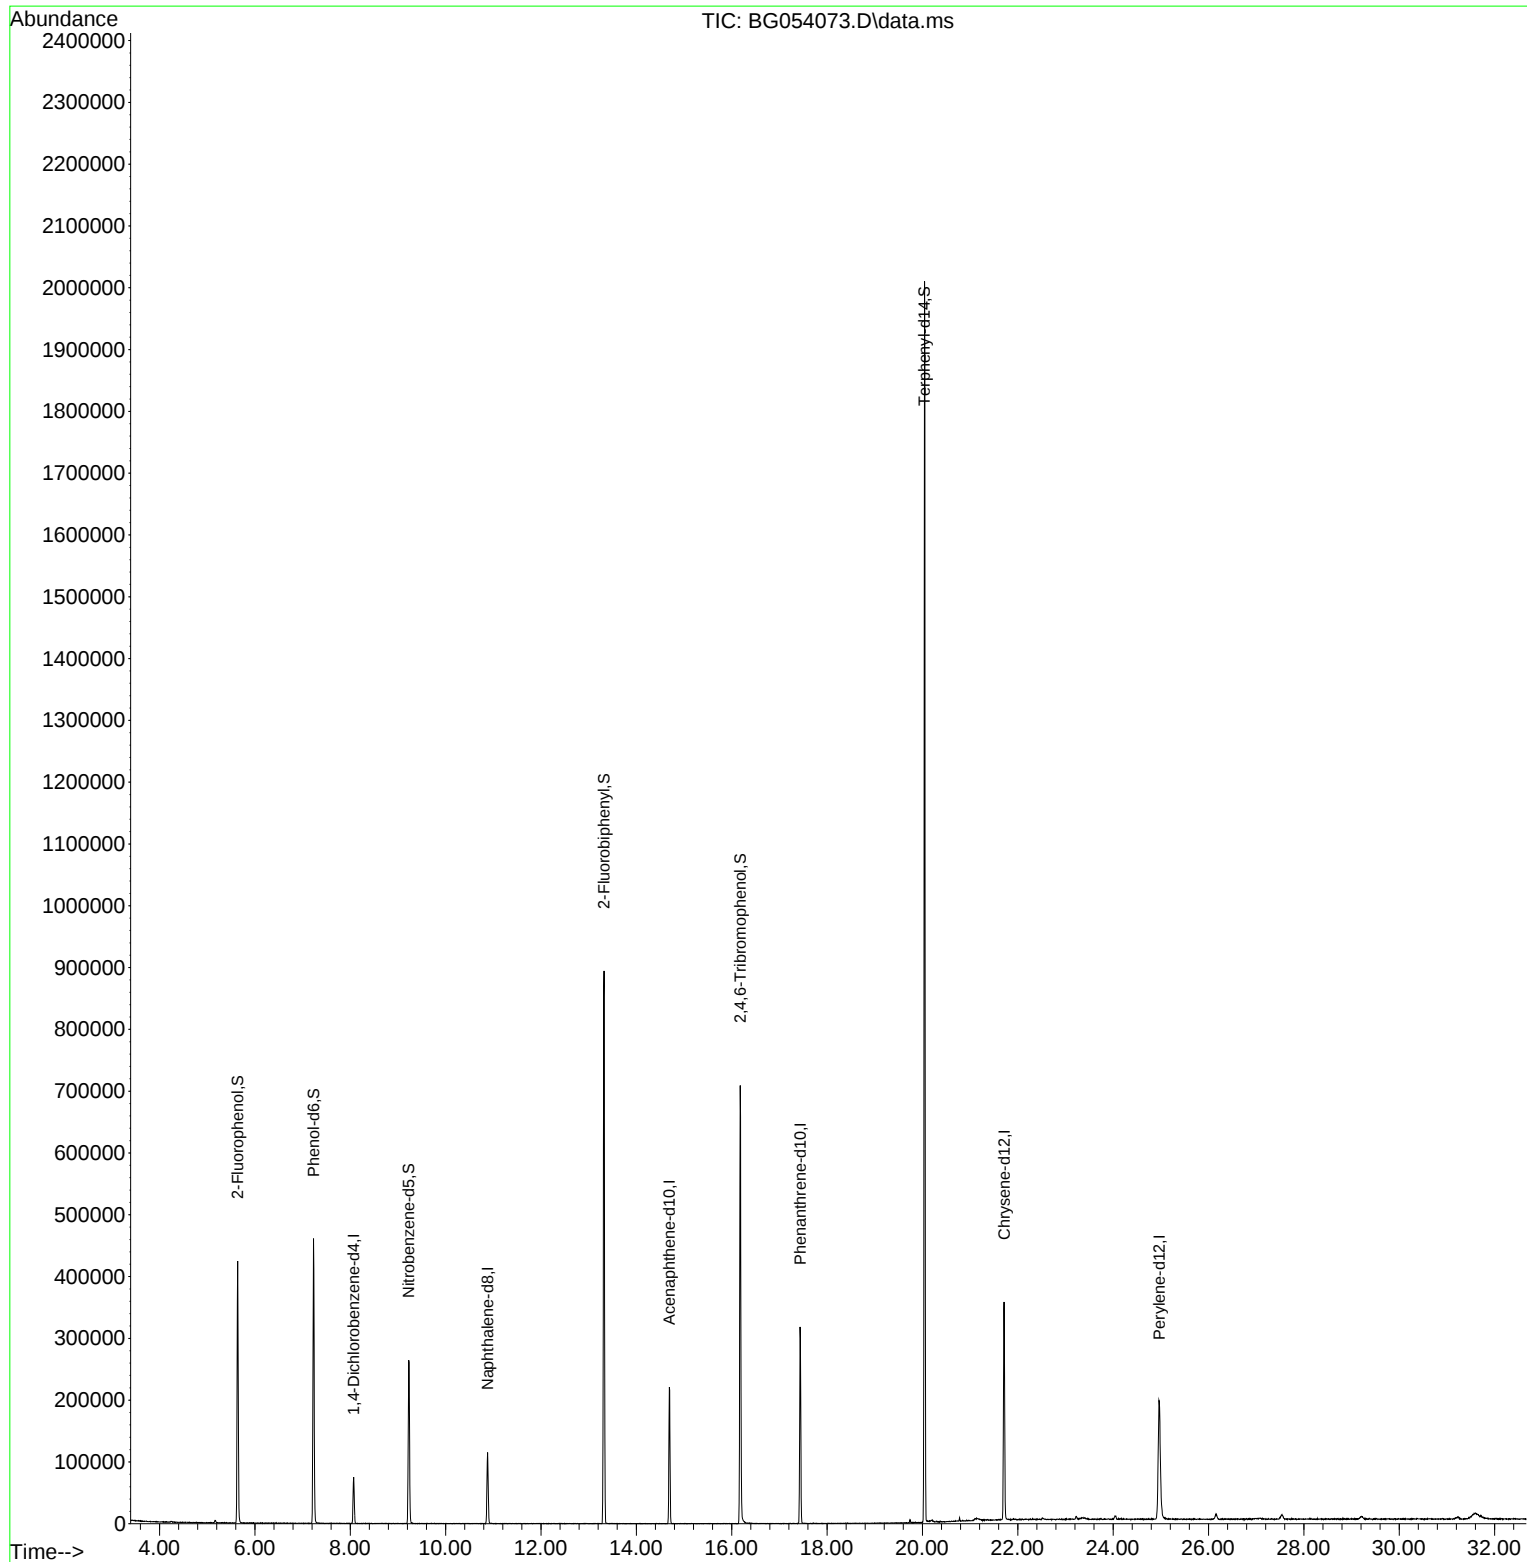


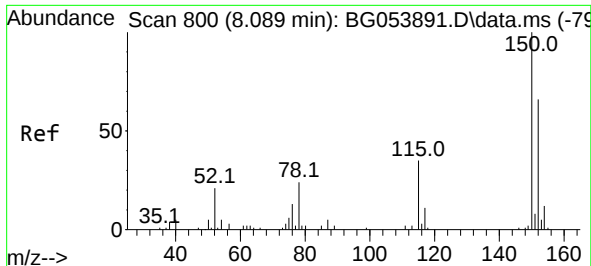

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.071 min Scan# 79
Delta R.T. 0.001 min
Lab File: BG054073.D
Acq: 26 Jun 2022 15:16




Instrument :
BNA_G
ClientSampleId :
PB145765TB


Tgt Ion:152 Resp: 23917
Ion Ratio Lower Upper
152 100
150 154.8 131.6 197.4
115 58.2 50.9 76.3

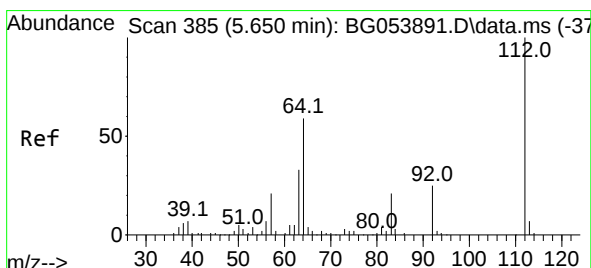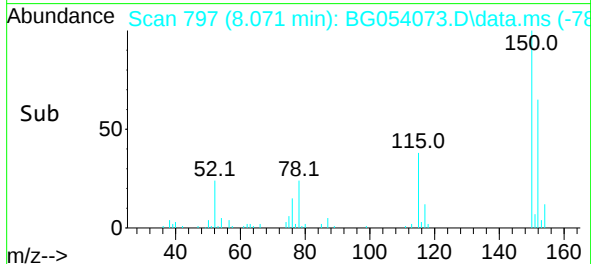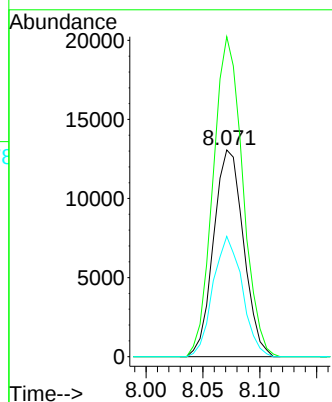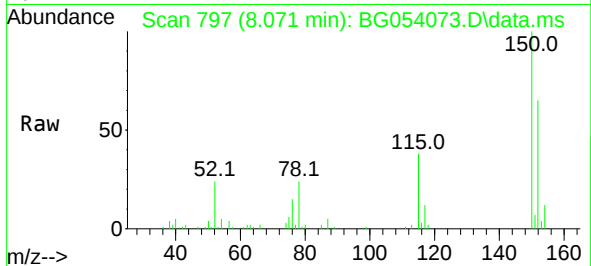

#5
2-Fluorophenol
Concen: 157.839 ng
RT: 5.638 min Scan# 383
Delta R.T. 0.001 min
Lab File: BG054073.D
Acq: 26 Jun 2022 15:16

Tgt Ion:112 Resp: 197448
Ion Ratio Lower Upper
112 100
64 63.6 55.1 82.7
63 34.0 30.4 45.6


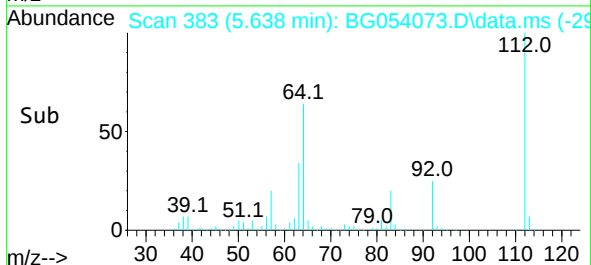
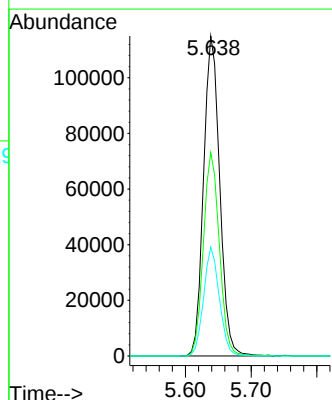
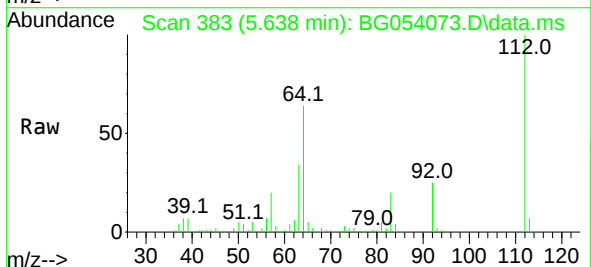


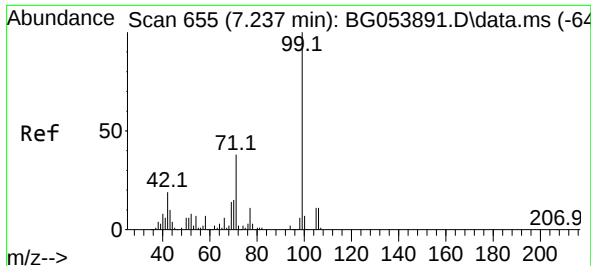

#7
Phenol-d6
Concen: 163.086 ng
RT: 7.231 min Scan# 61
Delta R.T. 0.001 min
Lab File: BG054073.D
Acq: 26 Jun 2022 15:16




Instrument :
BNA_G
ClientSampleId :
PB145765TB


Tgt Ion: 99 Resp: 276758
Ion Ratio Lower Upper
99 100
42 20.0 17.0 25.6
71 37.6 33.8 50.8

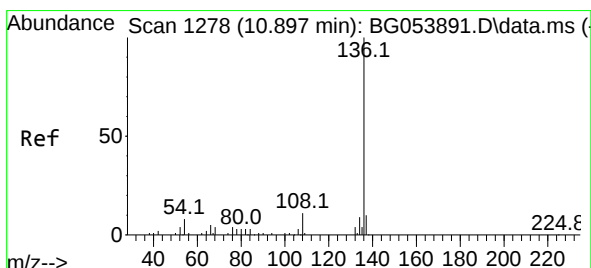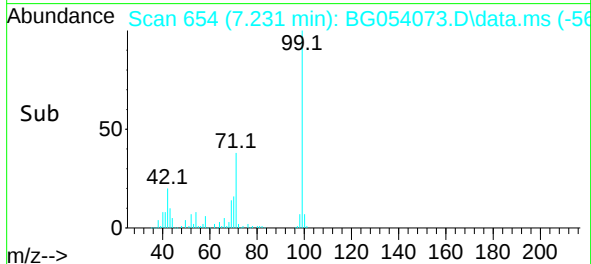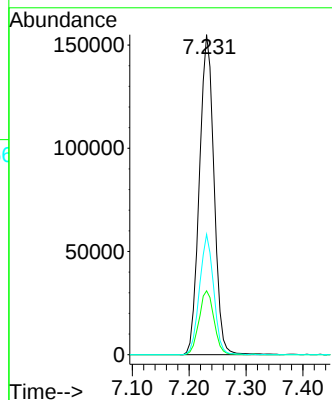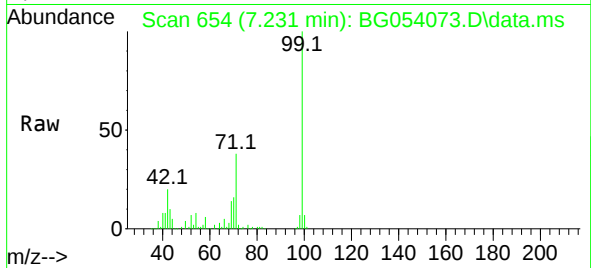

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.879 min Scan# 1275
Delta R.T. 0.001 min
Lab File: BG054073.D
Acq: 26 Jun 2022 15:16

Tgt Ion: 136 Resp: 106774
Ion Ratio Lower Upper
136 100
137 11.1 8.5 12.7
54 8.9 7.4 11.2
68 6.8 4.9 7.3

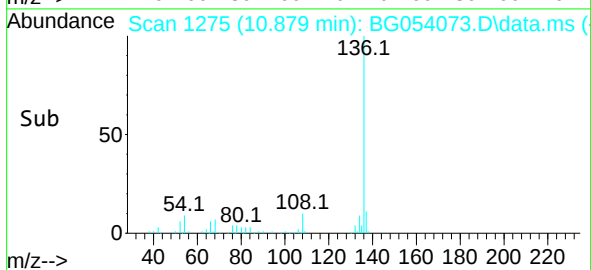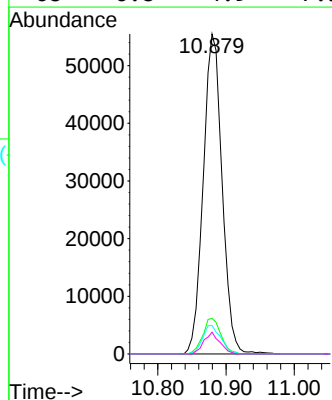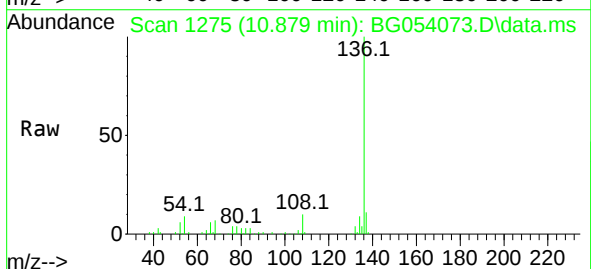

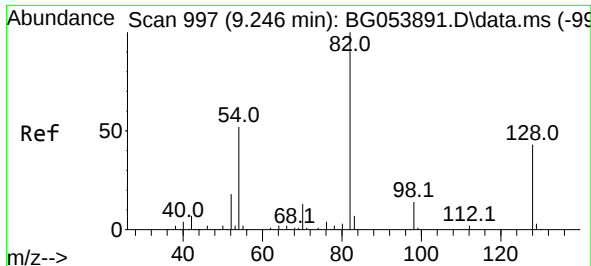

#23

Nitrobenzene-d5

Concen: 91.755 ng

RT: 9.228 min Scan# 994

Delta R.T. -0.005 min

Lab File: BG054073.D

Acq: 26 Jun 2022 15:16

Instrument :

BNA_G

ClientSampleId :

PB145765TB





Tgt Ion: 82 Resp: 174337

Ion Ratio Lower Upper

82 100

128 39.9 27.9 41.9

54 52.5 41.2 61.8

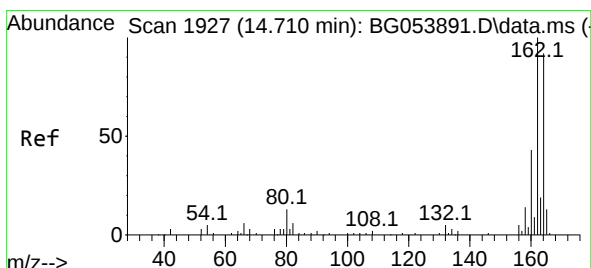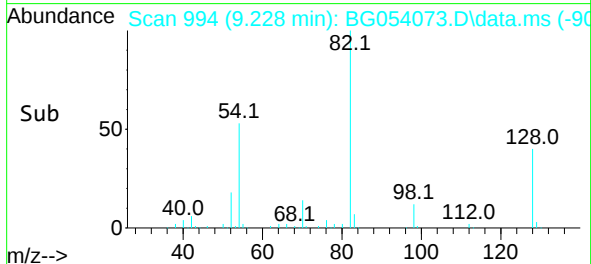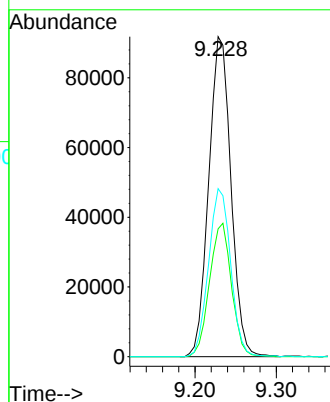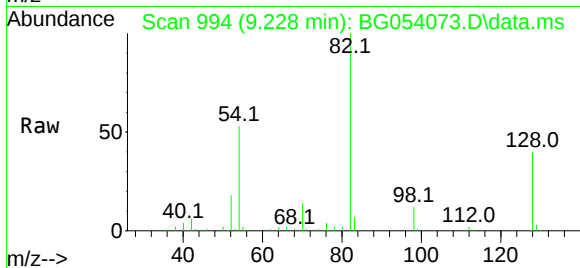

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.693 min Scan# 1924

Delta R.T. -0.005 min

Lab File: BG054073.D

Acq: 26 Jun 2022 15:16




Tgt Ion: 164 Resp: 87285


Ion Ratio Lower Upper

164 100

162 105.8 82.3 123.5

160 46.9 34.2 51.2


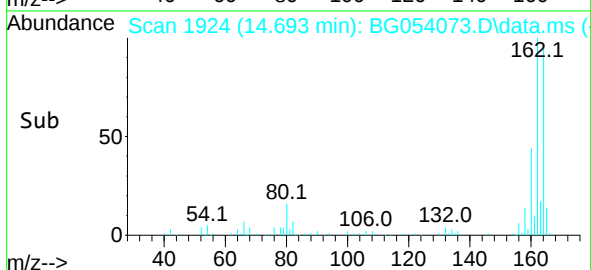
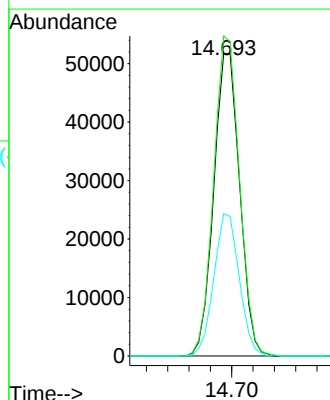
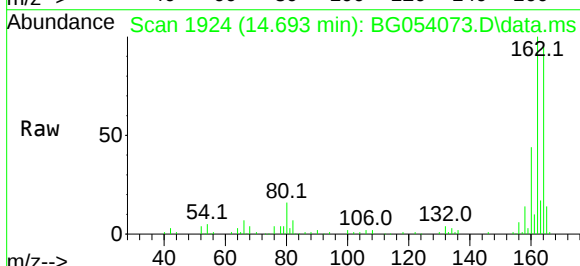


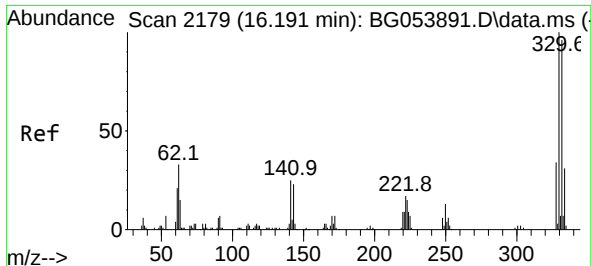

#42
 2,4,6-Tribromophenol
 Concen: 115.457 ng
 RT: 16.179 min Scan# 2179
 Delta R.T. -0.005 min
 Lab File: BG054073.D
 Acq: 26 Jun 2022 15:16




Instrument :
 BNA_G
 ClientSampleId :
 PB145765TB


Tgt Ion:330 Resp: 161915
 Ion Ratio Lower Upper
 330 100
 332 96.8 76.0 114.0
 141 28.6 27.1 40.7

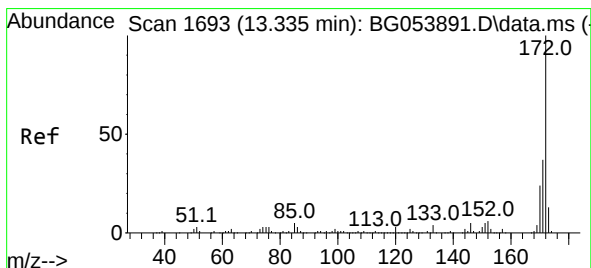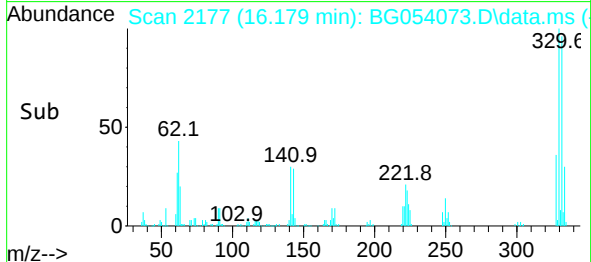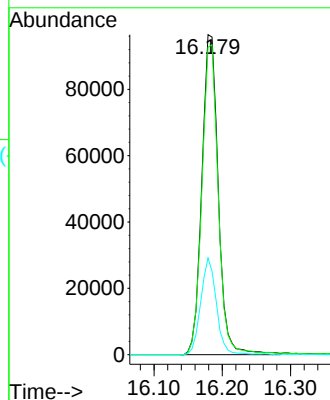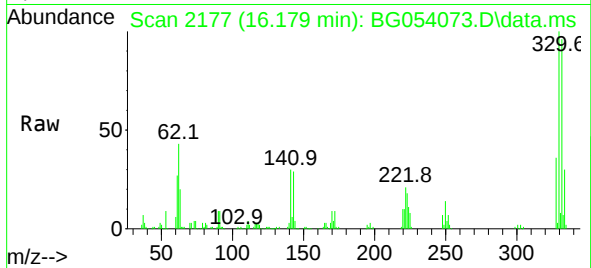

#45
 2-Fluorobiphenyl
 Concen: 84.934 ng
 RT: 13.324 min Scan# 1691
 Delta R.T. 0.001 min
 Lab File: BG054073.D
 Acq: 26 Jun 2022 15:16

Tgt Ion:172 Resp: 509819
 Ion Ratio Lower Upper
 172 100
 171 37.2 28.5 42.7
 170 25.2 18.9 28.3


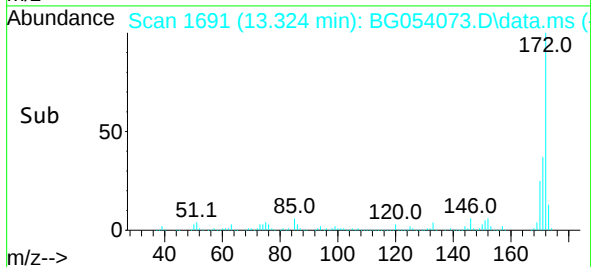
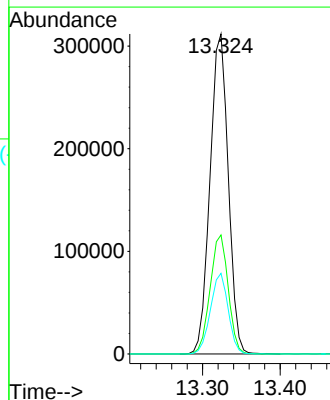
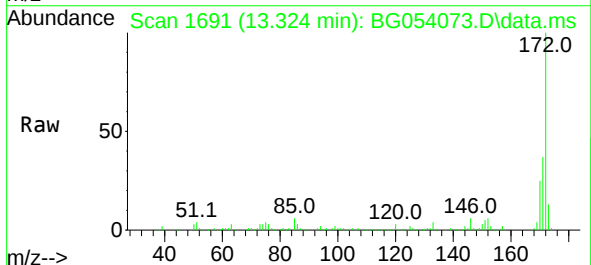


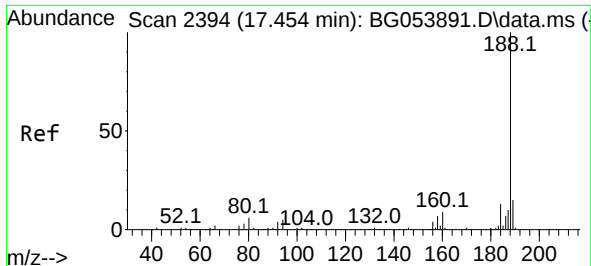

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.436 min Scan# 21
Delta R.T. -0.005 min
Lab File: BG054073.D
Acq: 26 Jun 2022 15:16




Instrument :
BNA_G
ClientSampleId :
PB145765TB


Tgt Ion:188 Resp: 227313
Ion Ratio Lower Upper
188 100
94 6.5 5.4 8.0
80 7.8 6.8 10.2

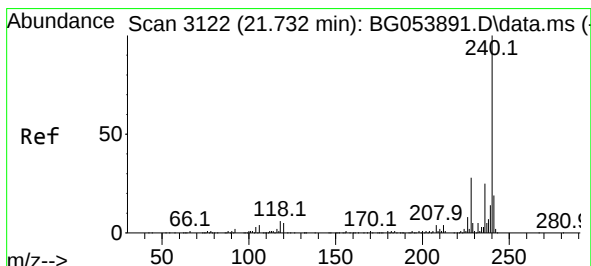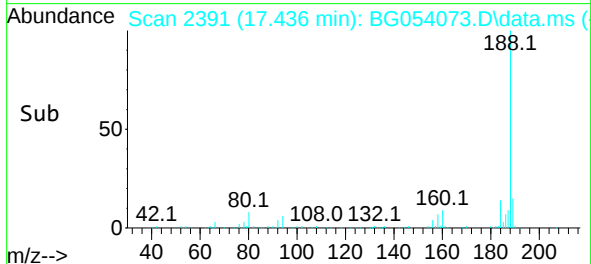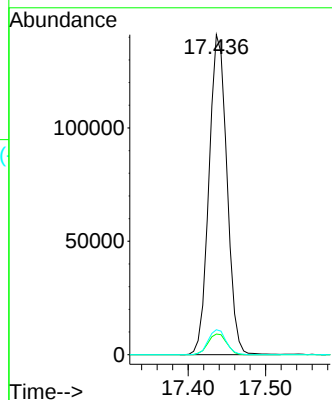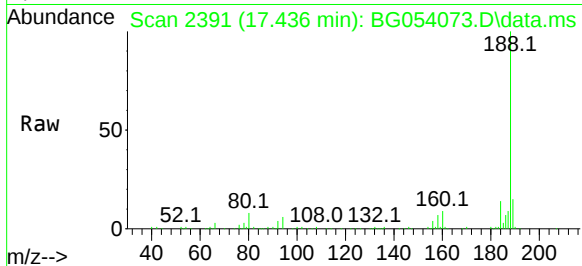

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.714 min Scan# 3119
Delta R.T. -0.005 min
Lab File: BG054073.D
Acq: 26 Jun 2022 15:16

Tgt Ion:240 Resp: 249220
Ion Ratio Lower Upper
240 100
120 6.6 4.6 7.0
236 24.4 20.2 30.4


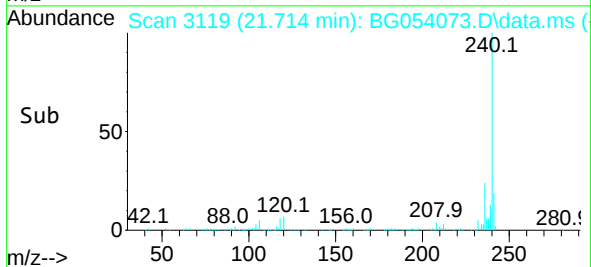
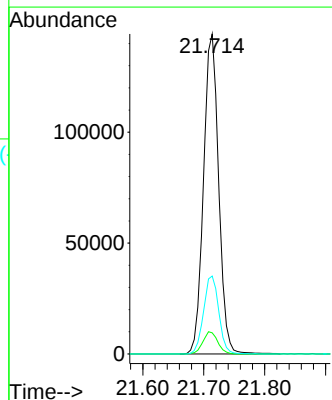
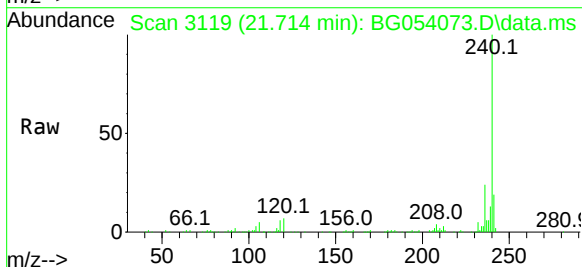


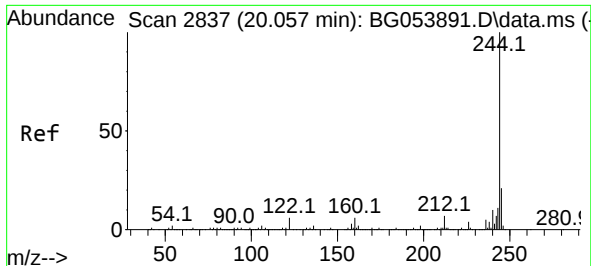

#79
 Terphenyl-d14
 Concen: 90.309 ng
 RT: 20.045 min Scan# 21
 Delta R.T. 0.001 min
 Lab File: BG054073.D
 Acq: 26 Jun 2022 15:16

Instrument :
 BNA_G
 ClientSampleId :
 PB145765TB

Tgt Ion:244 Resp: 1117478
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.5 9.7
 122 7.3 5.0 7.4

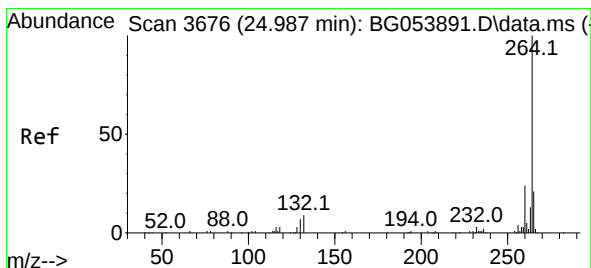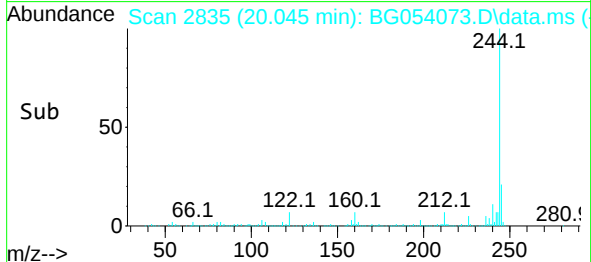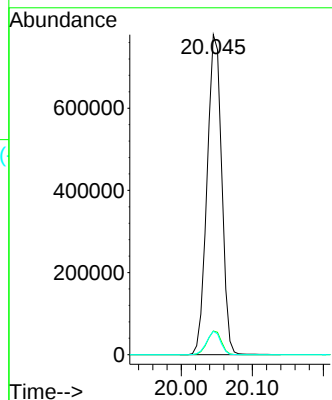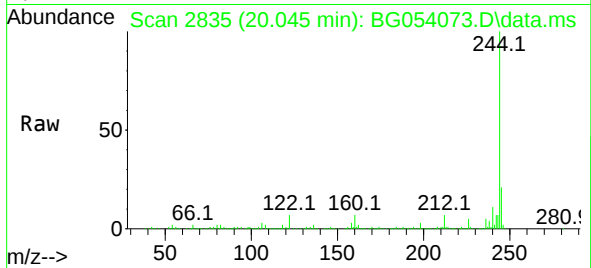

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.969 min Scan# 3673
 Delta R.T. 0.006 min
 Lab File: BG054073.D
 Acq: 26 Jun 2022 15:16

Tgt Ion:264 Resp: 248653
 Ion Ratio Lower Upper
 264 100
 260 22.8 19.0 28.6
 265 21.8 17.4 26.2

