

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062622\
 Data File : BG054083.D
 Acq On : 26 Jun 2022 21:50
 Operator : CG/JU
 Sample : N3488-15
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-14-0-2-20220623

Quant Time: Jun 27 00:33:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 27 00:27:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.071	152	28351	20.000	ng	0.00
21) Naphthalene-d8	10.880	136	113721	20.000	ng	0.00
39) Acenaphthene-d10	14.693	164	81848	20.000	ng	0.00
64) Phenanthrene-d10	17.437	188	206057	20.000	ng	0.00
76) Chrysene-d12	21.714	240	232904	20.000	ng	0.00
86) Perylene-d12	24.963	264	226820	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.639	112	173670	117.118	ng	0.00
7) Phenol-d6	7.231	99	226185	112.440	ng	0.00
23) Nitrobenzene-d5	9.229	82	152848	75.531	ng	0.00
42) 2,4,6-Tribromophenol	16.179	330	118256	89.926	ng	0.00
45) 2-Fluorobiphenyl	13.318	172	398909	70.871	ng	0.00
79) Terphenyl-d14	20.045	244	852124	73.689	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062622\
Data File : BG054083.D
Acq On : 26 Jun 2022 21:50
Operator : CG/JU
Sample : N3488-15
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-14-0-2-20220623

Quant Time: Jun 27 00:33:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration



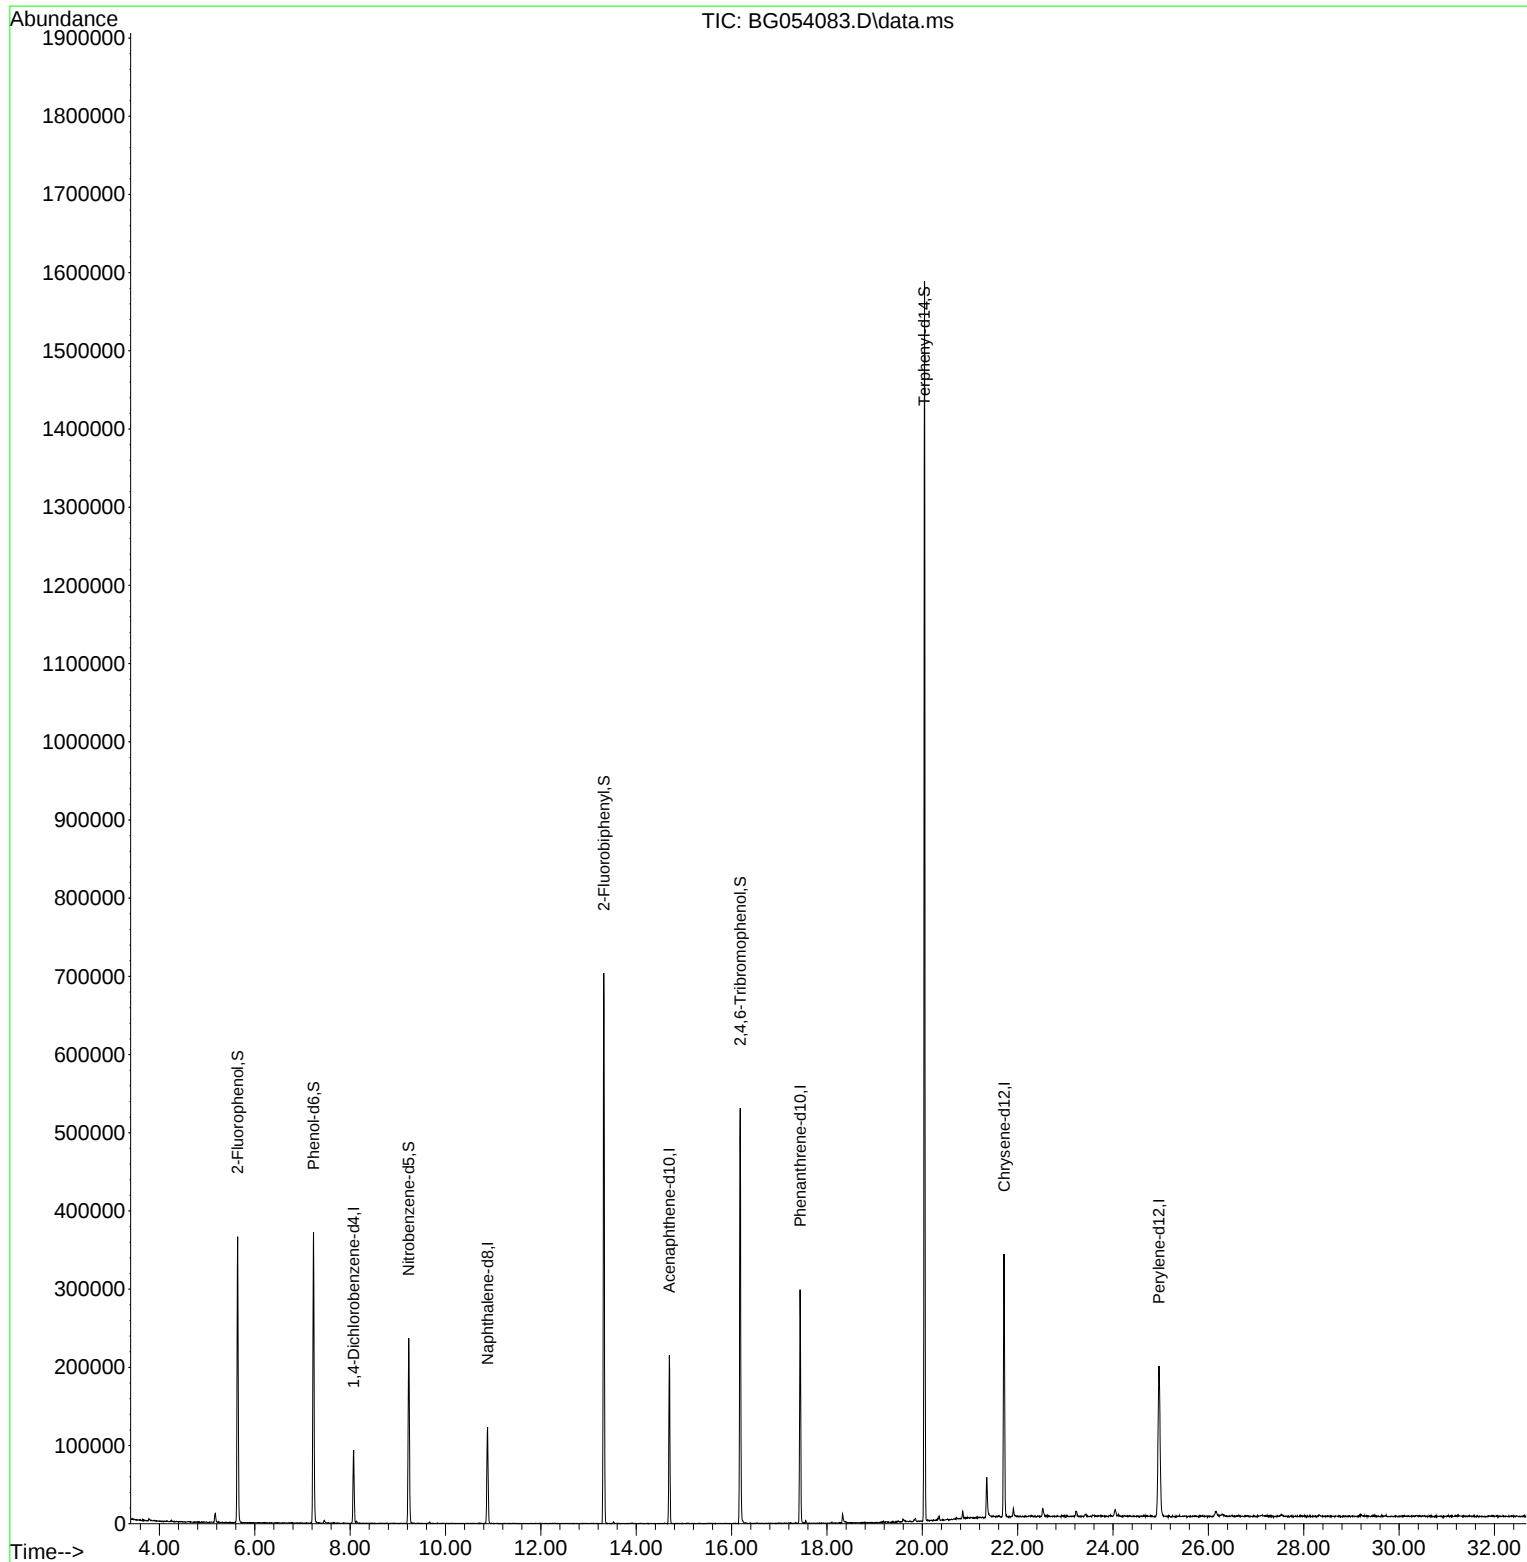




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.071 min Scan# 79
Delta R.T. 0.001 min
Lab File: BG054083.D
Acq: 26 Jun 2022 21:50




Instrument :
BNA_G
ClientSampleId :
SB-14-0-2-20220623

Tgt Ion:152 Resp: 28351
Ion Ratio Lower Upper
152 100
150 151.2 131.6 197.4
115 59.0 50.9 76.3

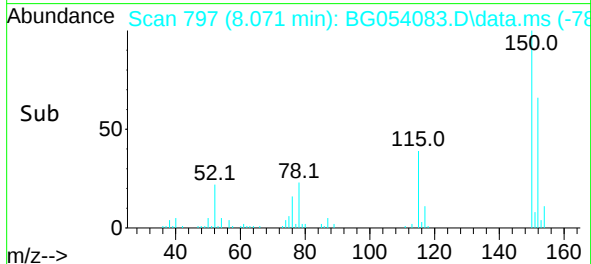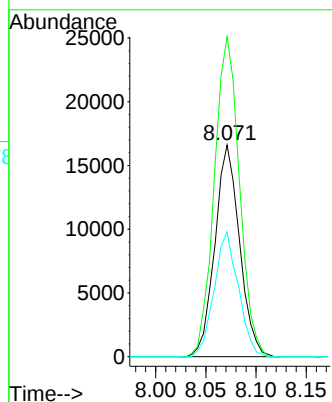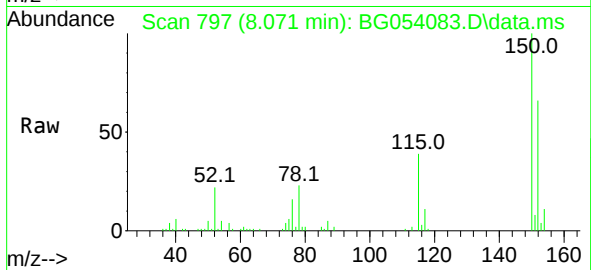

#5
2-Fluorophenol
Concen: 117.118 ng
RT: 5.639 min Scan# 383
Delta R.T. 0.001 min
Lab File: BG054083.D
Acq: 26 Jun 2022 21:50

Tgt Ion:112 Resp: 173670
Ion Ratio Lower Upper
112 100
64 64.5 55.1 82.7
63 34.4 30.4 45.6


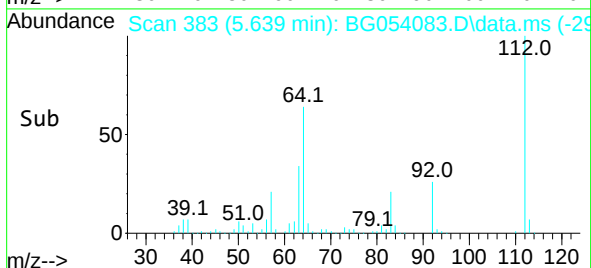

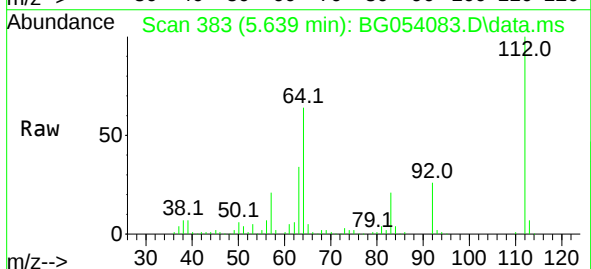




#7
Phenol-d6
Concen: 112.440 ng
RT: 7.231 min Scan# 61
Delta R.T. 0.001 min
Lab File: BG054083.D
Acq: 26 Jun 2022 21:50




Instrument :
BNA_G
ClientSampleId :
SB-14-0-2-20220623


Tgt Ion: 99 Resp: 226185
Ion Ratio Lower Upper
99 100
42 20.6 17.0 25.6
71 37.8 33.8 50.8

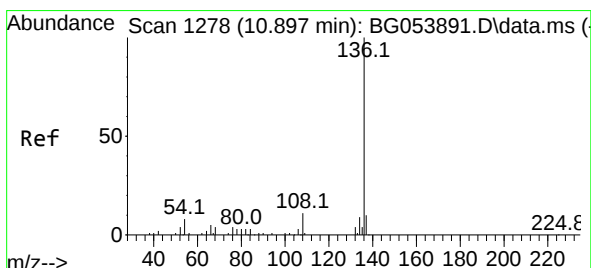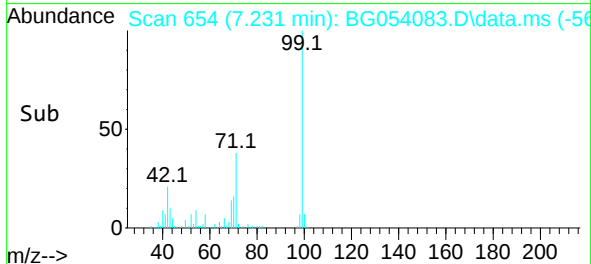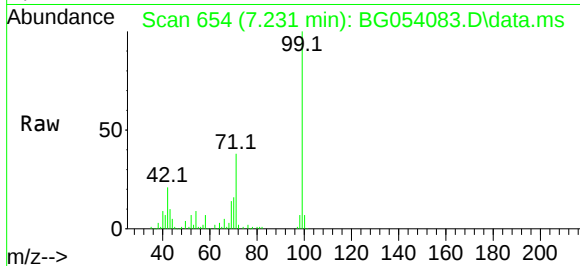

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.880 min Scan# 1275
Delta R.T. 0.001 min
Lab File: BG054083.D
Acq: 26 Jun 2022 21:50

Tgt Ion: 136 Resp: 113721
Ion Ratio Lower Upper
136 100
137 10.6 8.5 12.7
54 8.6 7.4 11.2
68 5.9 4.9 7.3

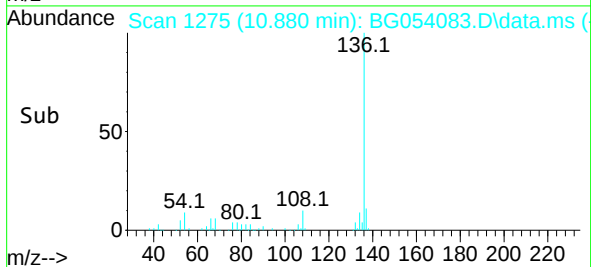

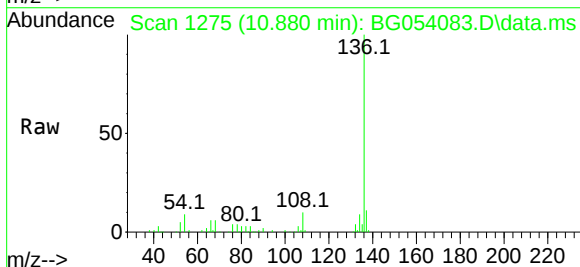


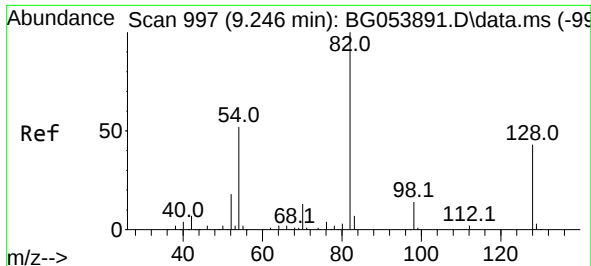

#23
 Nitrobenzene-d5
 Concen: 75.531 ng
 RT: 9.229 min Scan# 994
 Delta R.T. -0.005 min
 Lab File: BG054083.D
 Acq: 26 Jun 2022 21:50




Instrument :
 BNA_G
 ClientSampleId :
 SB-14-0-2-20220623

Tgt Ion: 82 Resp: 152848
 Ion Ratio Lower Upper
 82 100
 128 41.2 27.9 41.9
 54 53.3 41.2 61.8

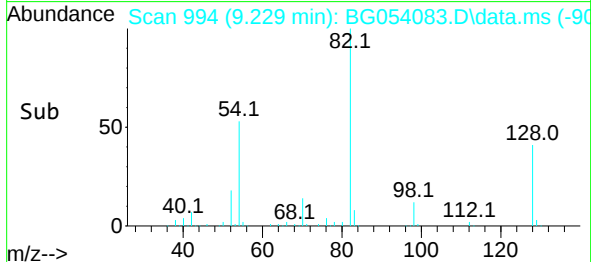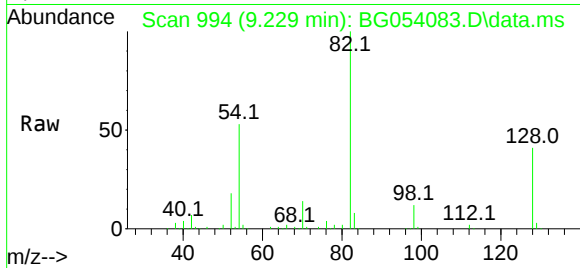

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.693 min Scan# 1924
 Delta R.T. -0.005 min
 Lab File: BG054083.D
 Acq: 26 Jun 2022 21:50


Tgt Ion: 164 Resp: 81848
 Ion Ratio Lower Upper
 164 100
 162 101.9 82.3 123.5
 160 41.1 34.2 51.2

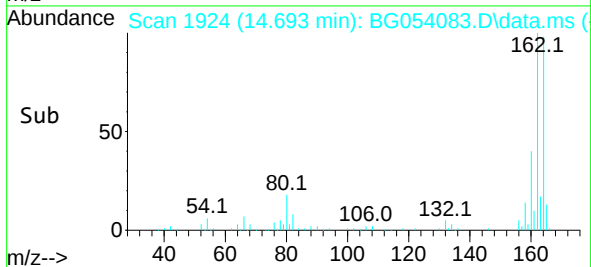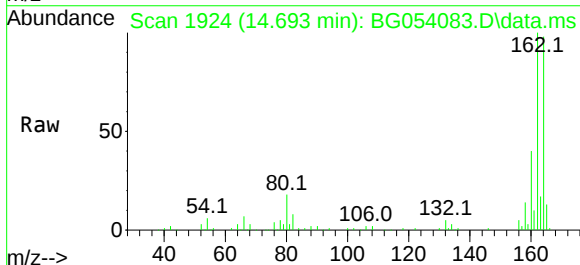






#42
2,4,6-Tribromophenol
Concen: 89.926 ng
RT: 16.179 min Scan# 2179
Delta R.T. -0.005 min
Lab File: BG054083.D
Acq: 26 Jun 2022 21:50

Instrument :
BNA_G
ClientSampleId :
SB-14-0-2-20220623



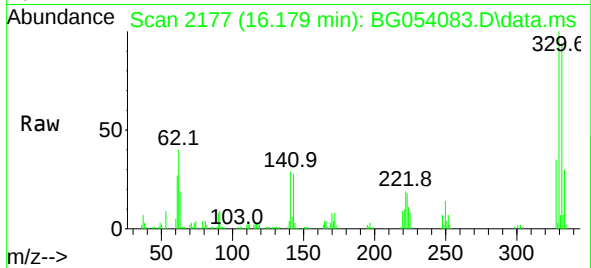



Tgt Ion:330 Resp: 118256
Ion Ratio Lower Upper
330 100
332 96.7 76.0 114.0
141 29.0 27.1 40.7

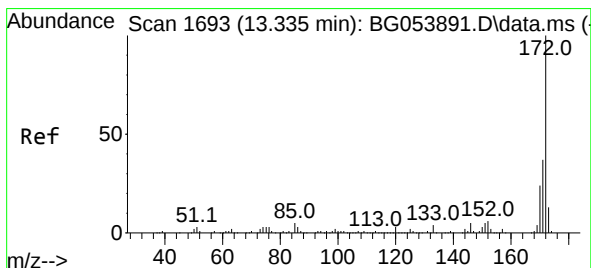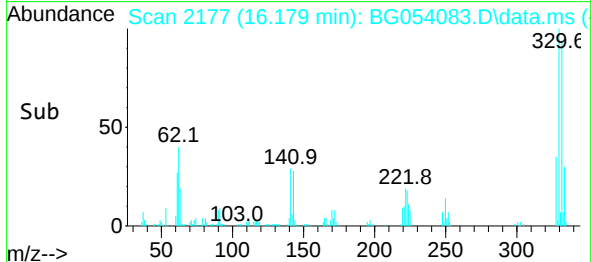

#45
2-Fluorobiphenyl
Concen: 70.871 ng
RT: 13.318 min Scan# 1690
Delta R.T. -0.005 min
Lab File: BG054083.D
Acq: 26 Jun 2022 21:50

Tgt Ion:172 Resp: 398909
Ion Ratio Lower Upper
172 100
171 37.6 28.5 42.7
170 24.2 18.9 28.3


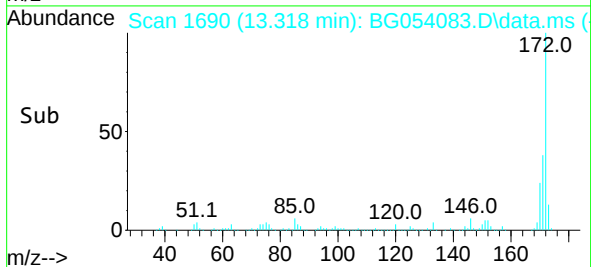

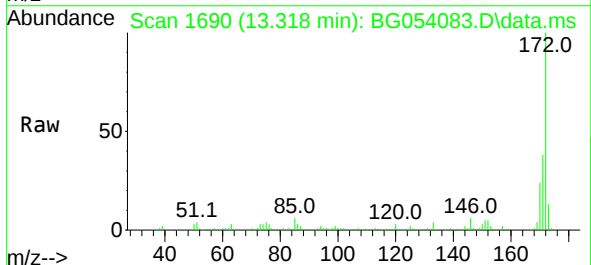


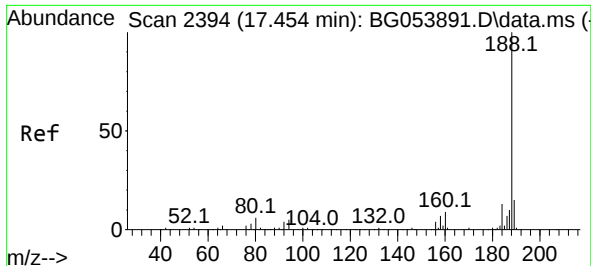

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.437 min Scan# 21
Delta R.T. -0.005 min
Lab File: BG054083.D
Acq: 26 Jun 2022 21:50




Instrument :
BNA_G
ClientSampleId :
SB-14-0-2-20220623


Tgt Ion:188 Resp: 206057
Ion Ratio Lower Upper
188 100
94 6.9 5.4 8.0
80 8.9 6.8 10.2

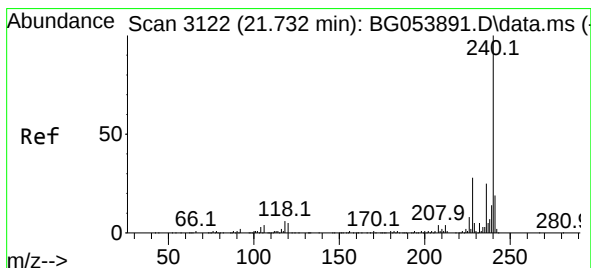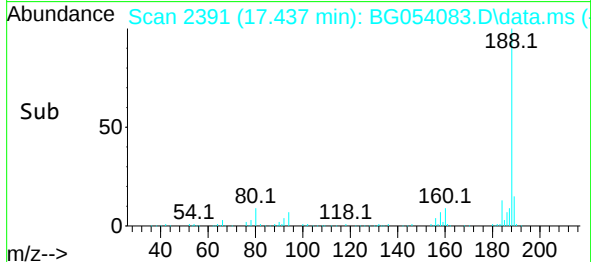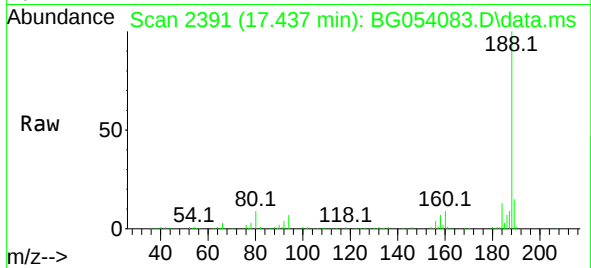

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.714 min Scan# 3119
Delta R.T. -0.005 min
Lab File: BG054083.D
Acq: 26 Jun 2022 21:50

Tgt Ion:240 Resp: 232904
Ion Ratio Lower Upper
240 100
120 6.4 4.6 7.0
236 24.5 20.2 30.4


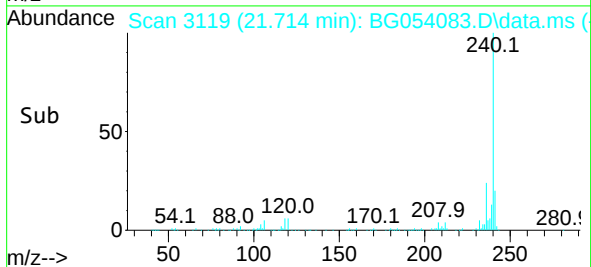

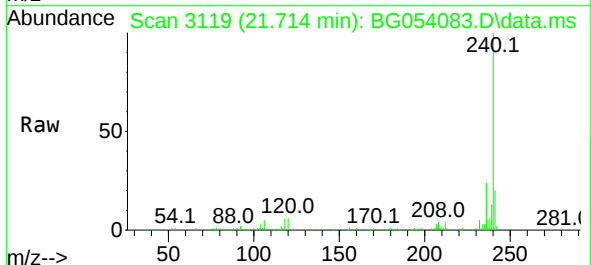


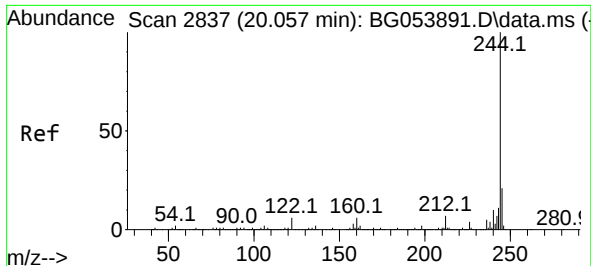

#79
 Terphenyl-d14
 Concen: 73.689 ng
 RT: 20.045 min Scan# 21
 Delta R.T. 0.001 min
 Lab File: BG054083.D
 Acq: 26 Jun 2022 21:50

Instrument :
 BNA_G
 ClientSampleId :
 SB-14-0-2-20220623

Tgt Ion:244 Resp: 852124
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.5 9.7
 122 7.2 5.0 7.4

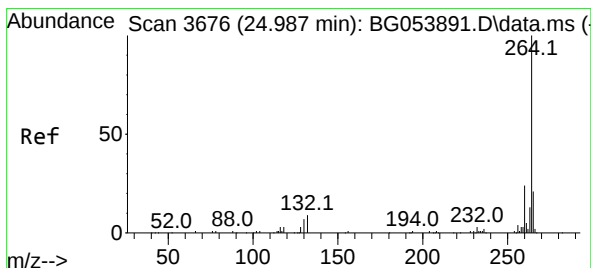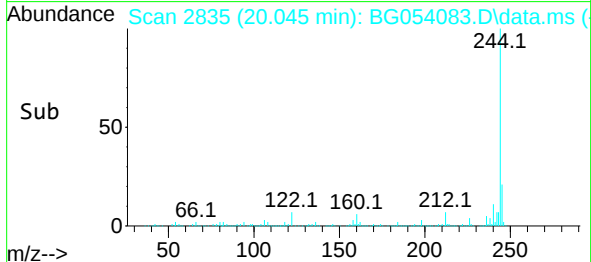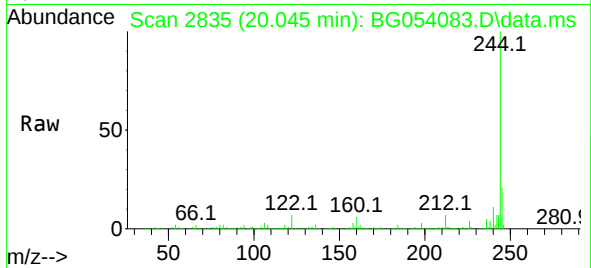

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.963 min Scan# 3672
 Delta R.T. 0.001 min
 Lab File: BG054083.D
 Acq: 26 Jun 2022 21:50

Tgt Ion:264 Resp: 226820
 Ion Ratio Lower Upper
 264 100
 260 25.3 19.0 28.6
 265 21.7 17.4 26.2

