
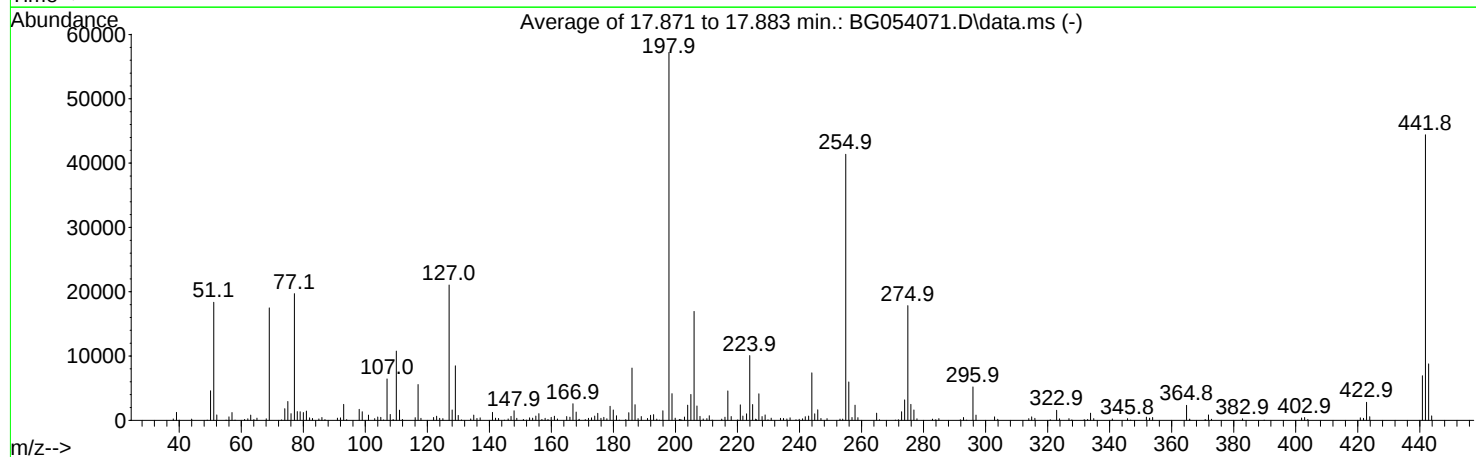


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062622\
 Data File : BG054071.D
 Acq On : 26 Jun 2022 12:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 27 00:27:54 2022

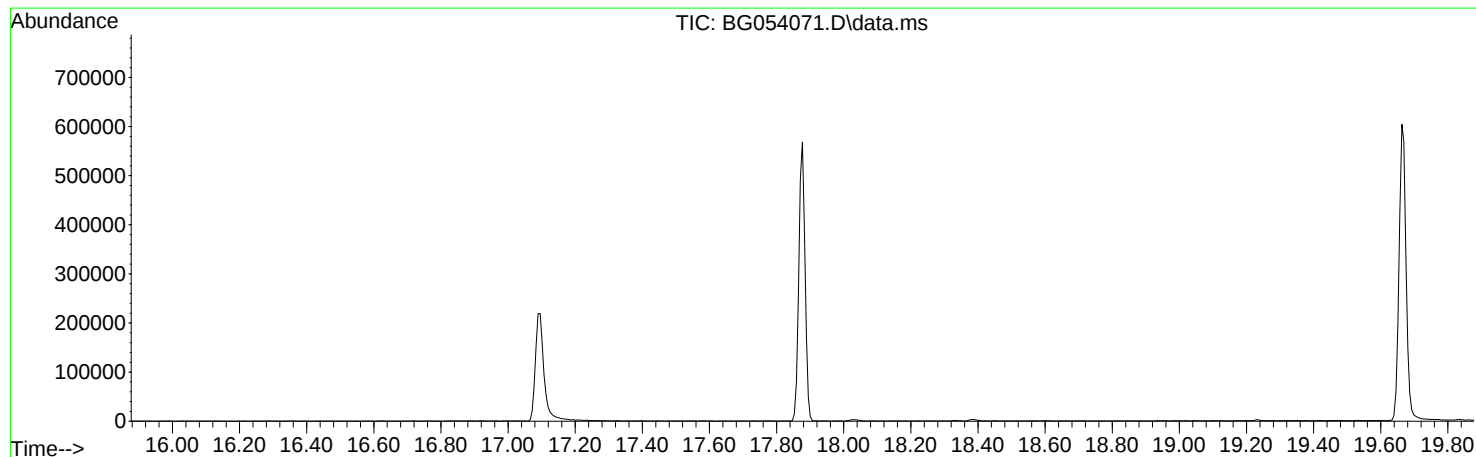




AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.1	18366	PASS
68	69	0.00	2	1.4	239	PASS
69	198	0.00	100	30.6	17485	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	36.8	21048	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	57203	PASS
199	198	5	9	7.3	4163	PASS
275	198	10	60	31.2	17830	PASS
365	198	1	100	4.1	2340	PASS
441	198	0.01	100	12.1	6942	PASS
442	442	50	100	100.0	44405	PASS
443	442	15	24	19.8	8796	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062622\
Data File : BG054071.D
Acq On : 26 Jun 2022 12:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 27 03:03:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

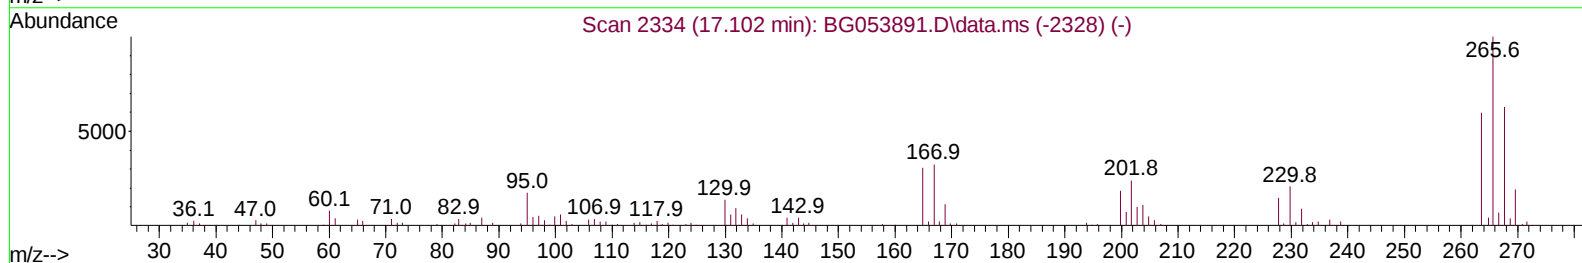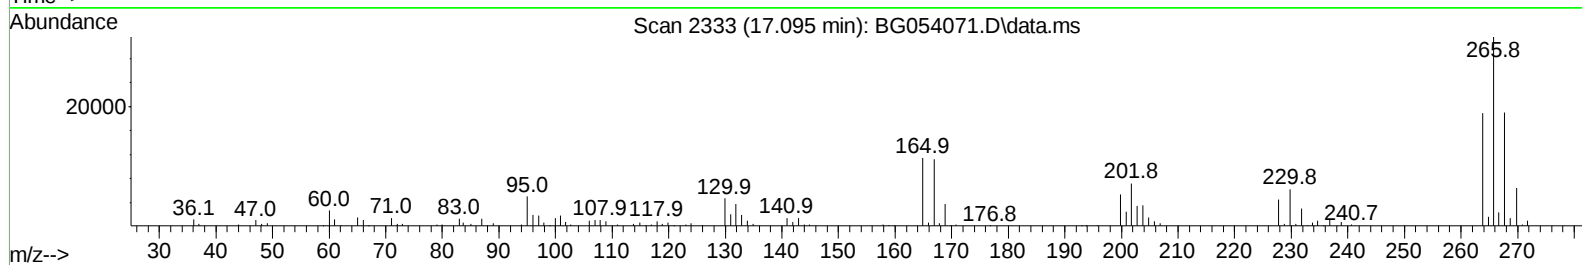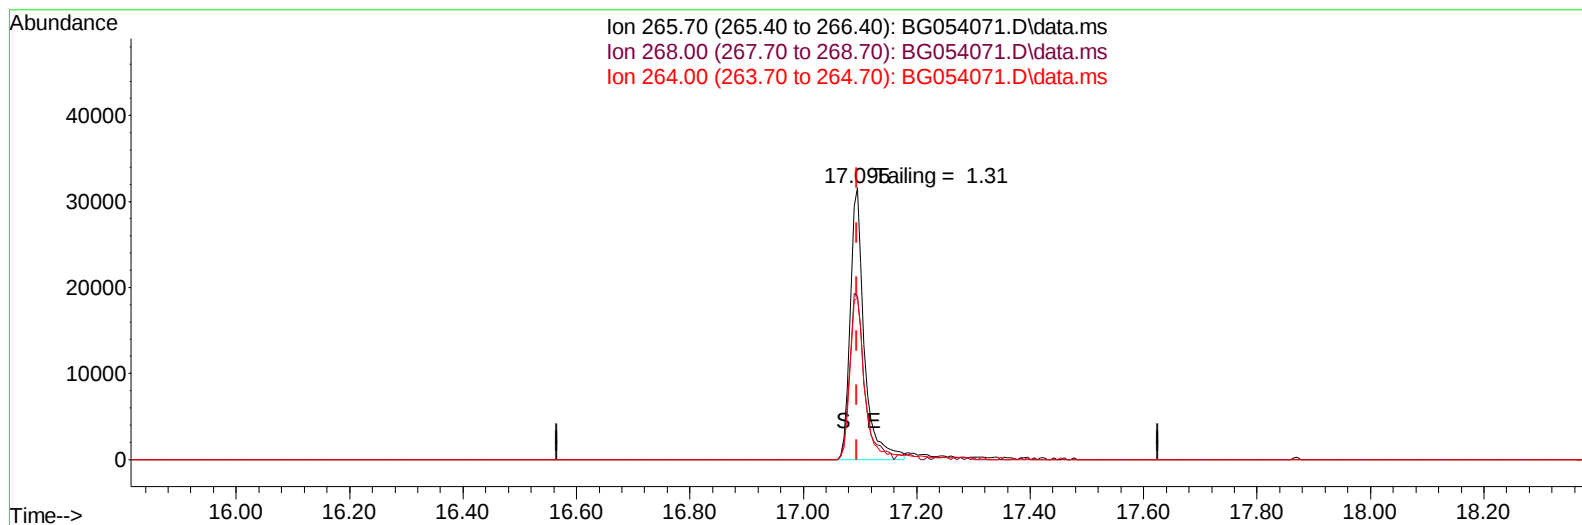

TIC: BG054071.D\data.ms

(70) Pentachlorophenol (C)

17.095min (+ 0.000) 28830.68 ng




response 54721

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	64.74
264.00	66.20	59.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062622\
Data File : BG054071.D
Acq On : 26 Jun 2022 12:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 27 03:03:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

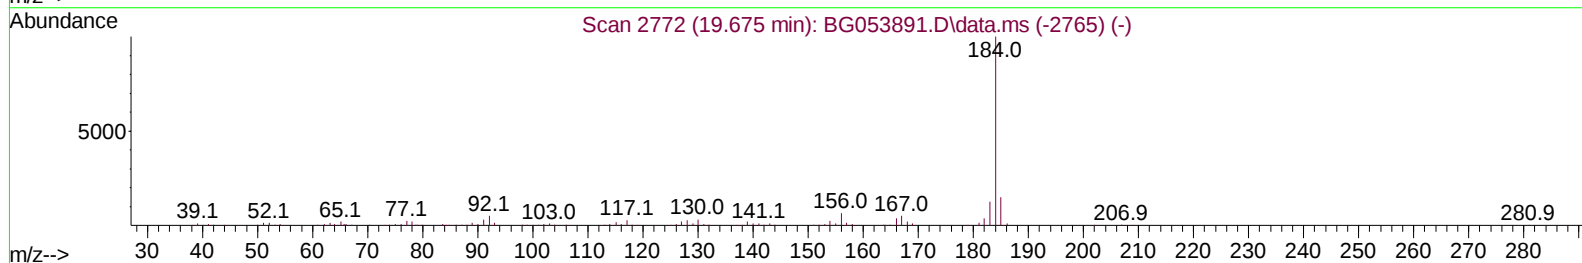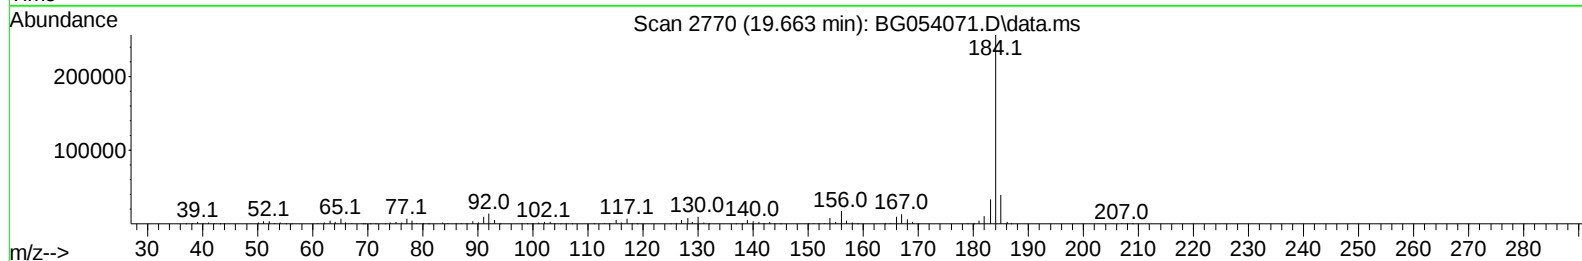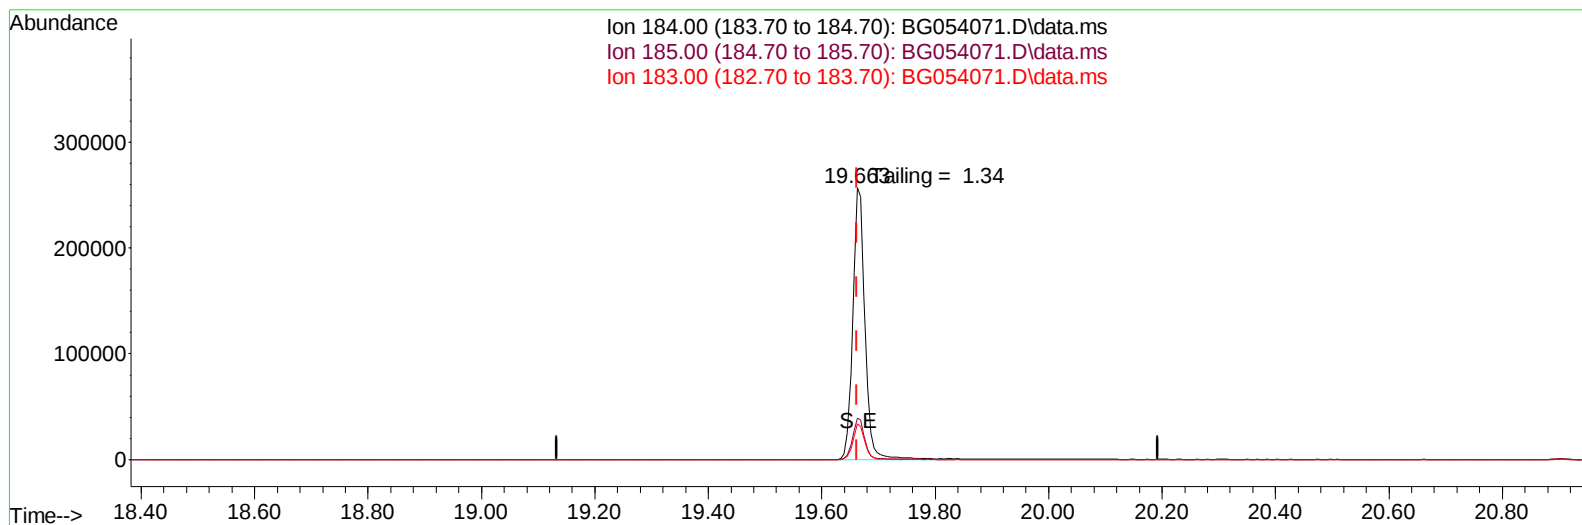

TIC: BG054071.D\data.ms

(77) Benzidine

19.663min (+ 0.000) 0.00 ng

response 383826

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.28
183.00	11.10	13.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/26/2022	BNA_G	<u>BG054071.D</u>
Compound Name	Response	Retention Time
DDT	210785	20.9
DDD	4343	20.46
DDE	0	19.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4343	215128	2.02

Instrument :
BNA_G
ClientSampleId :
DFTPP