
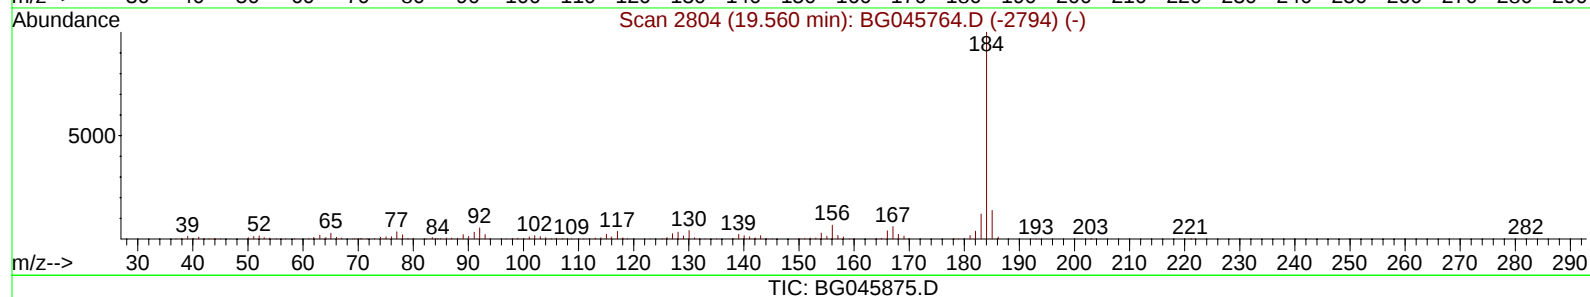
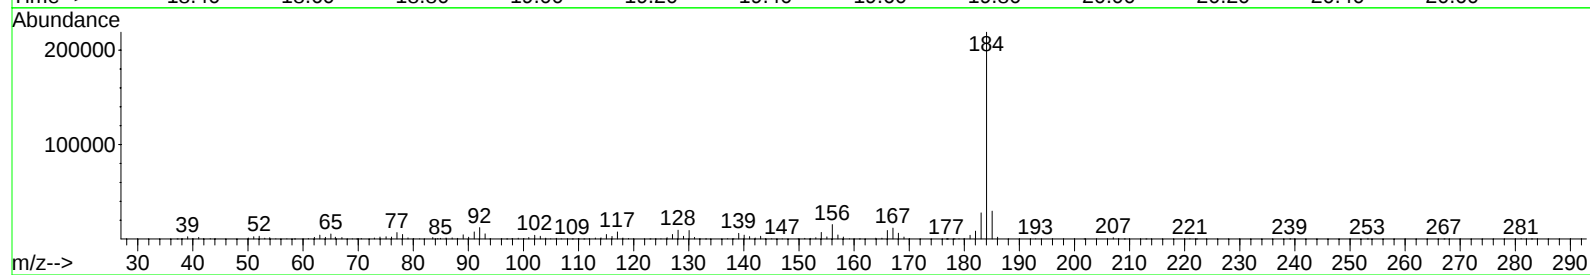


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062920\
 Data File : BG045875.D
 Acq On : 29 Jun 2020 14:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 18:11:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 25 15:44:32 2020
 Response via : Initial Calibration

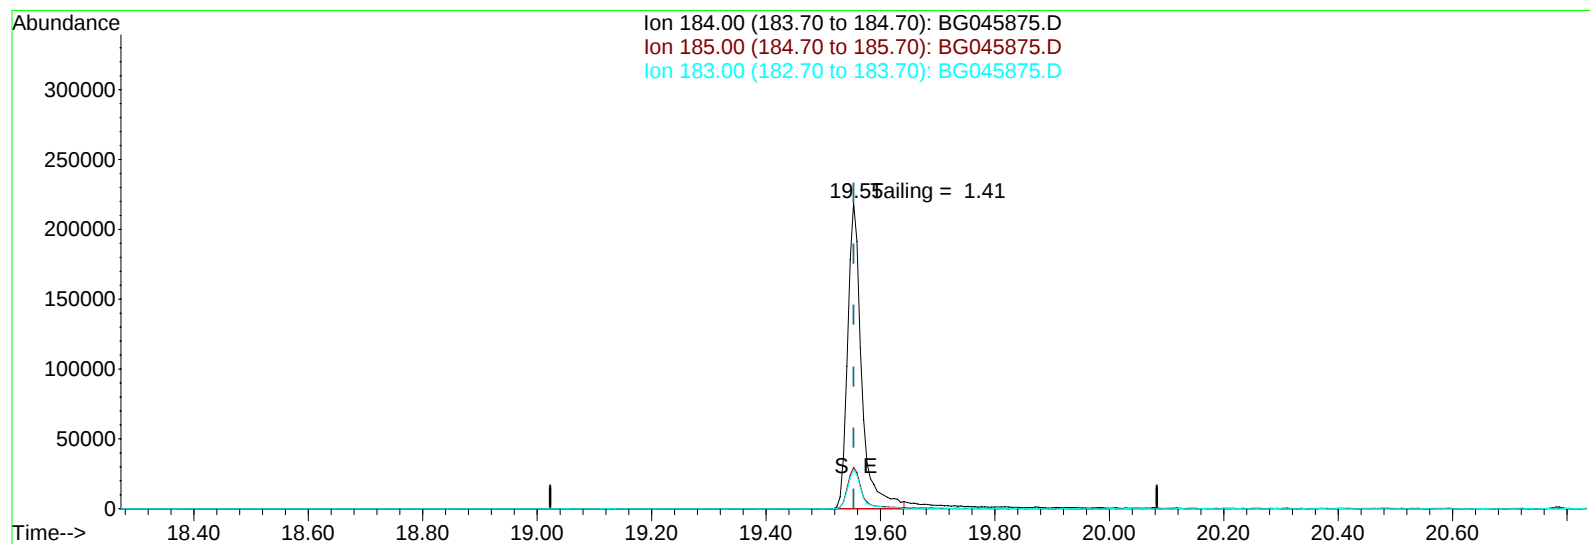

(77) Benzidine




19.553min (+0.000) 115068.29ng

response 394869

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.55
183.00	12.10	12.69
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062920\
Data File : BG045875.D
Acq On : 29 Jun 2020 14:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 18:11:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 25 15:44:32 2020
Response via : Initial Calibration

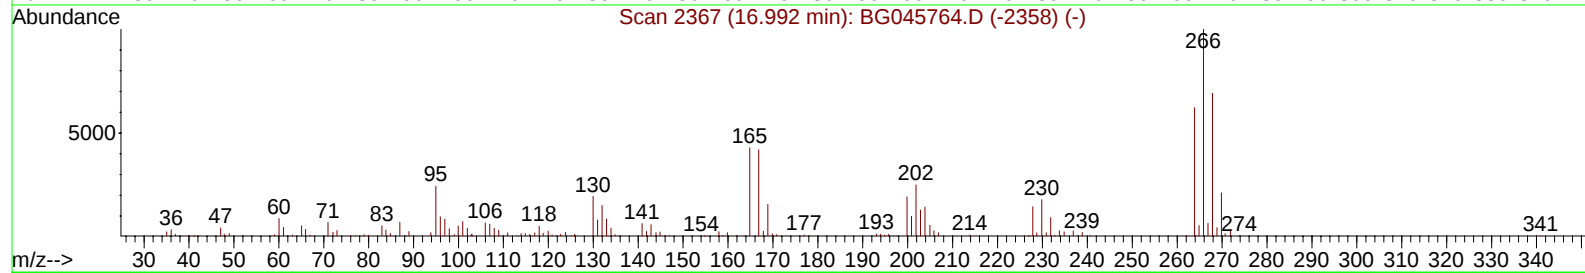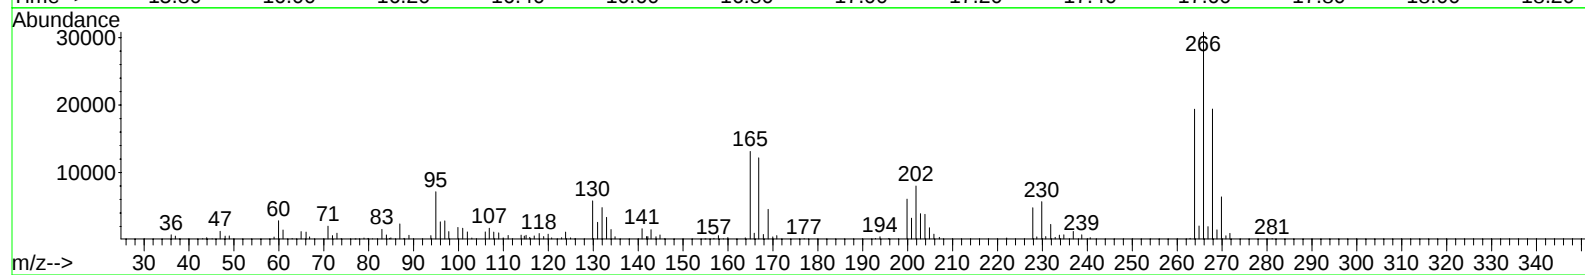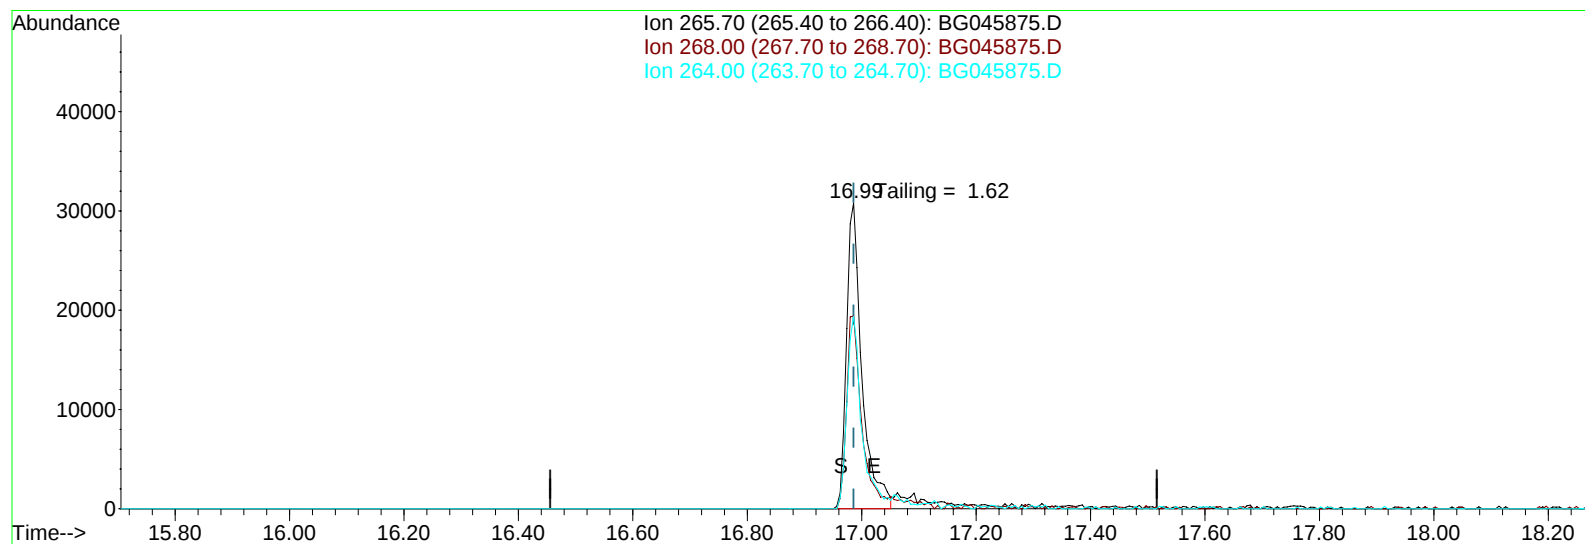

TIC: BG045875.D

(70) Pentachlorophenol (C)

16.986min (+0.000) 108182.73ng

response 58008

Ion	Exp%	Act%
265.70	100	100
268.00	69.20	63.04
264.00	62.20	62.94
0.00	0.00	0.00