
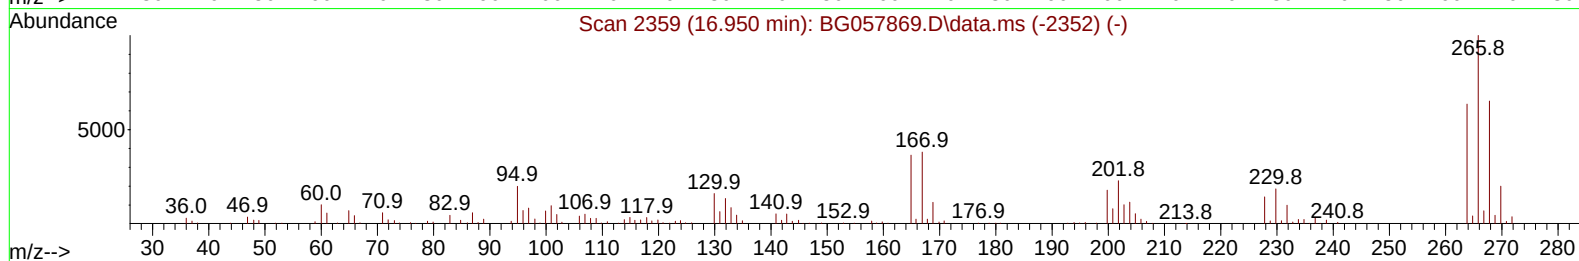
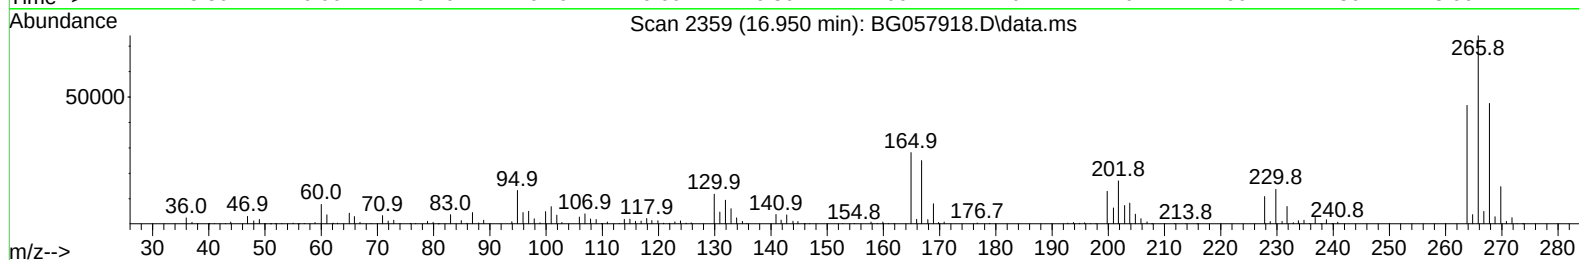


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG063023\
Data File : BG057918.D
Acq On : 30 Jun 2023 14:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 18:00:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 01:12:33 2023
Response via : Initial Calibration

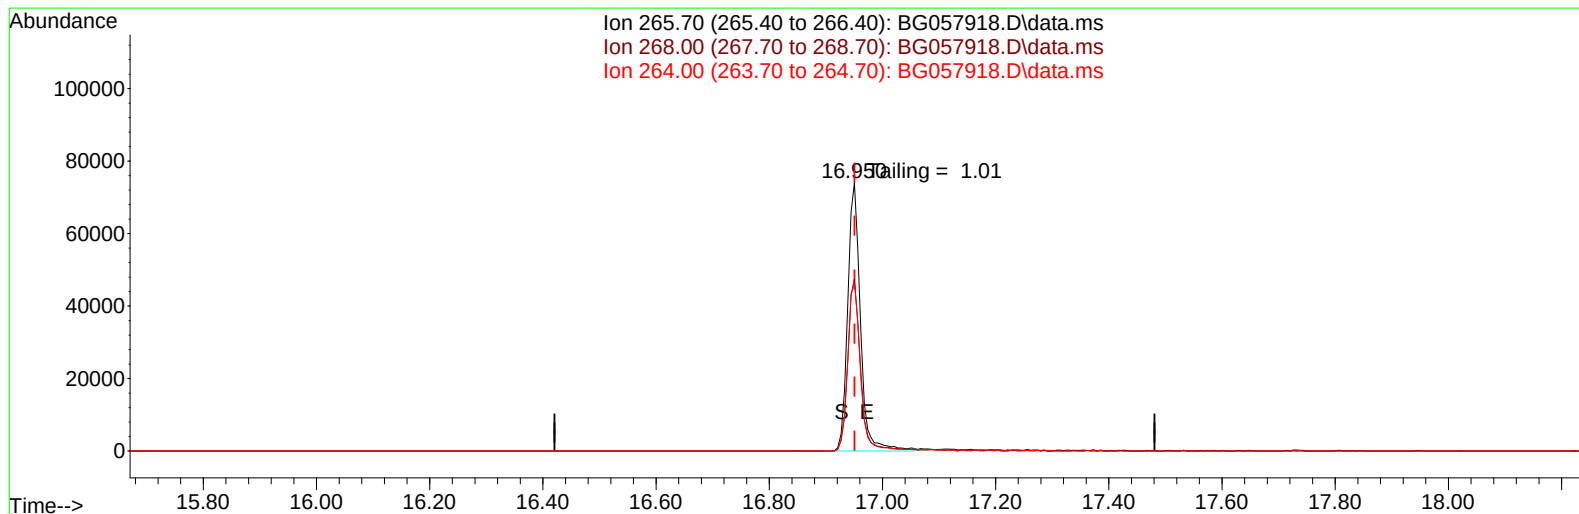

TIC: BG057918.D\data.ms

(70) Pentachlorophenol (C)




16.950min (-0.000) 193742.80 ng

response 115611

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	64.06
264.00	63.60	63.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG063023\
 Data File : BG057918.D
 Acq On : 30 Jun 2023 14:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 18:00:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 28 01:12:33 2023
 Response via : Initial Calibration

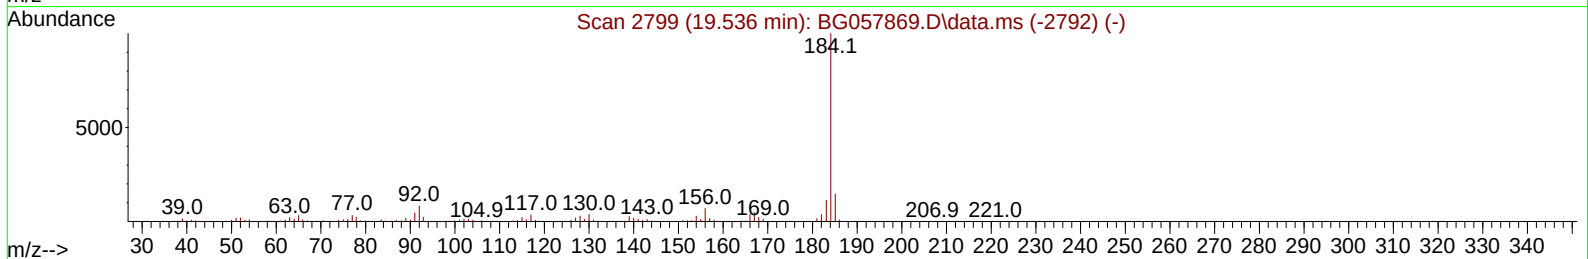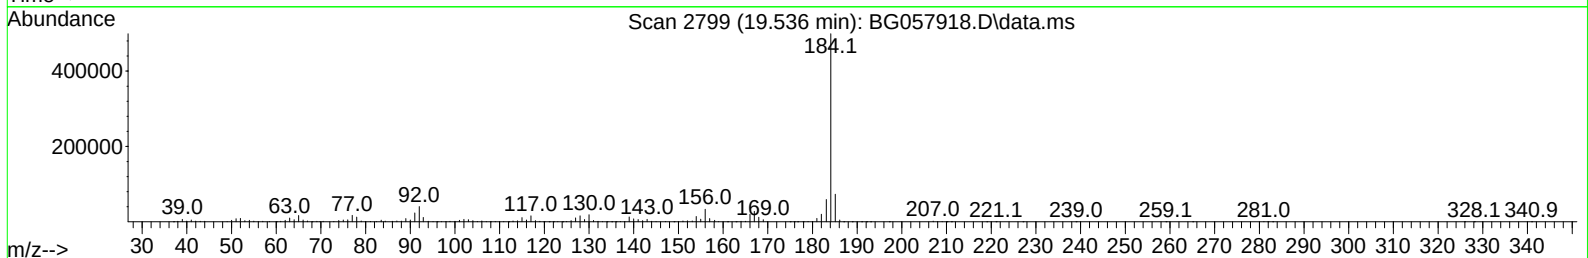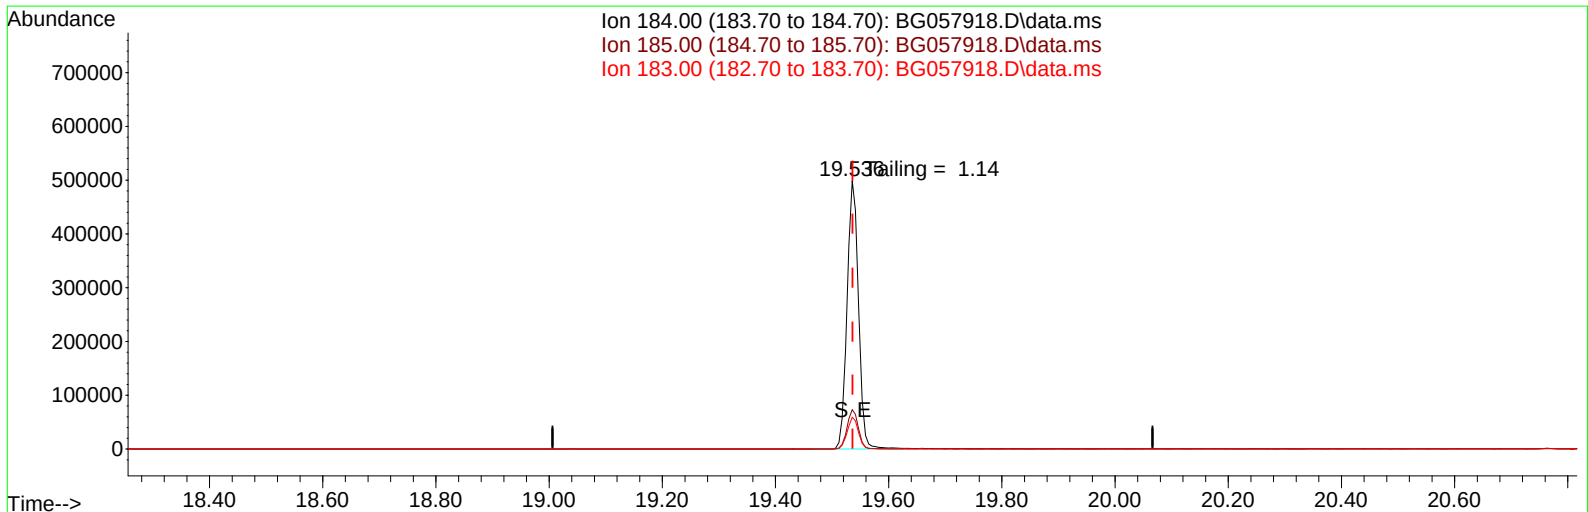

TIC: BG057918.D\data.ms

(77) Benzidine**19.536min (-0.000) 48514.75 ng****response 701134**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.66
183.00	11.20	11.88
0.00	0.00	0.00