


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG063023\
Data File : BG057918.D
Acq On : 30 Jun 2023 14:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 28 01:12:33 2023

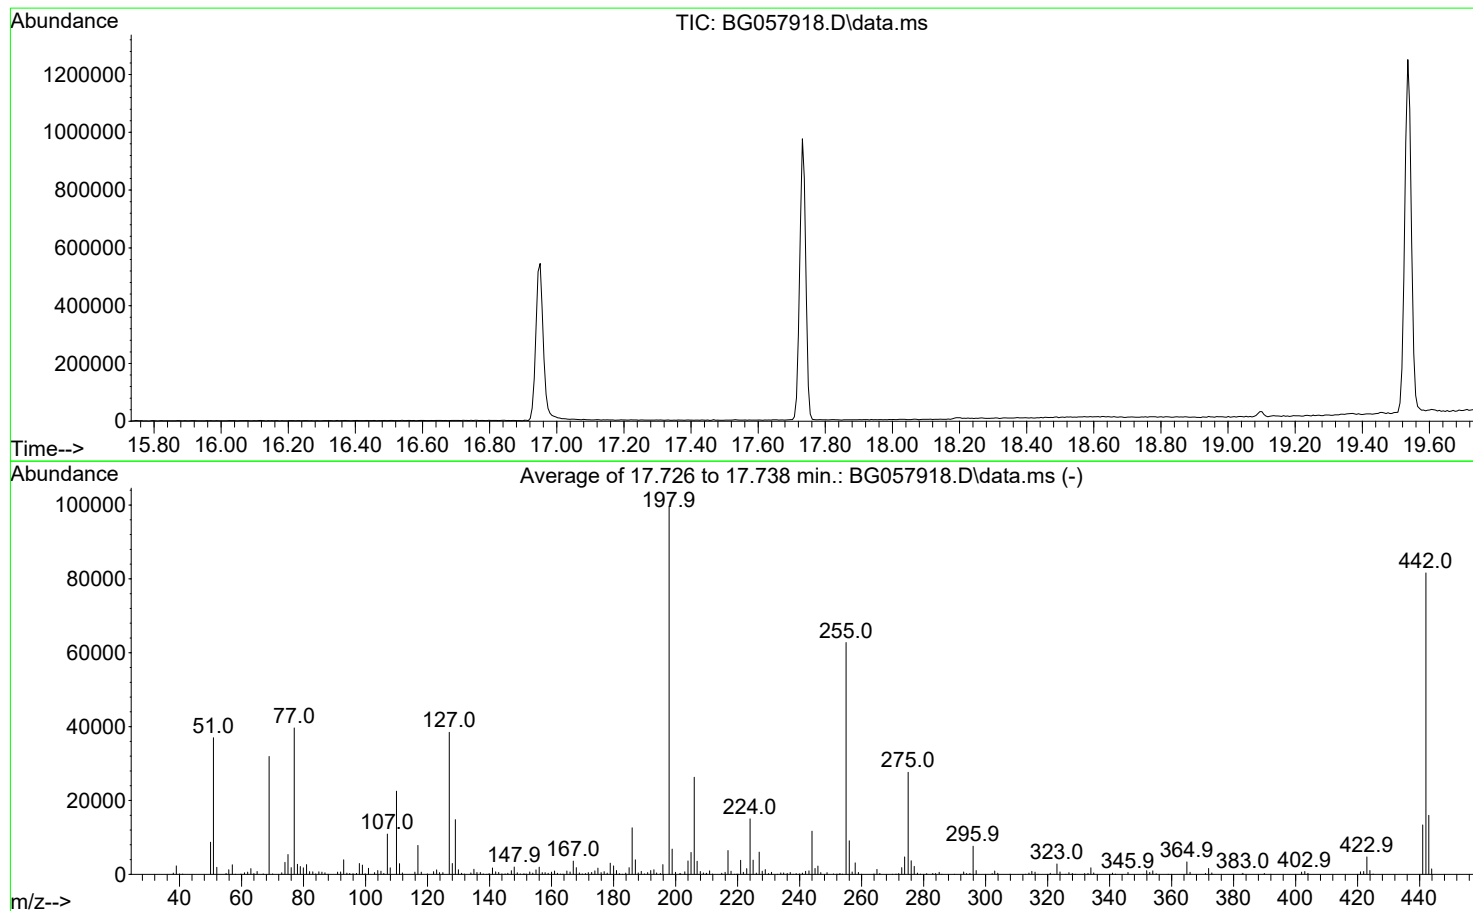




AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	36989	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.1	31924	PASS
70	69	0.00	2	0.4	116	PASS
127	198	10	80	38.6	38488	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	99595	PASS
199	198	5	9	6.9	6834	PASS
275	198	10	60	27.7	27624	PASS
365	198	1	100	3.4	3376	PASS
441	198	0.01	100	13.4	13394	PASS
442	442	50	100	100.0	81608	PASS
443	442	15	24	19.6	15976	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG063023\
Data File : BG057918.D
Acq On : 30 Jun 2023 14:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 30 18:00:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 01:12:33 2023
Response via : Initial Calibration

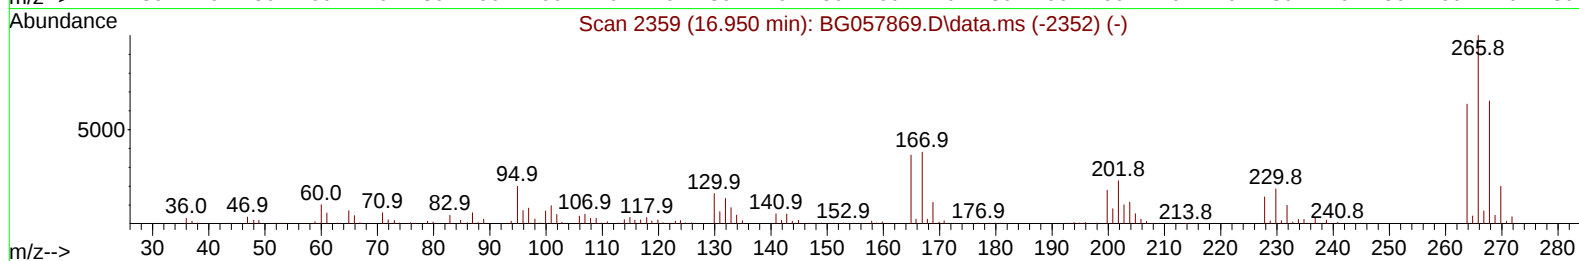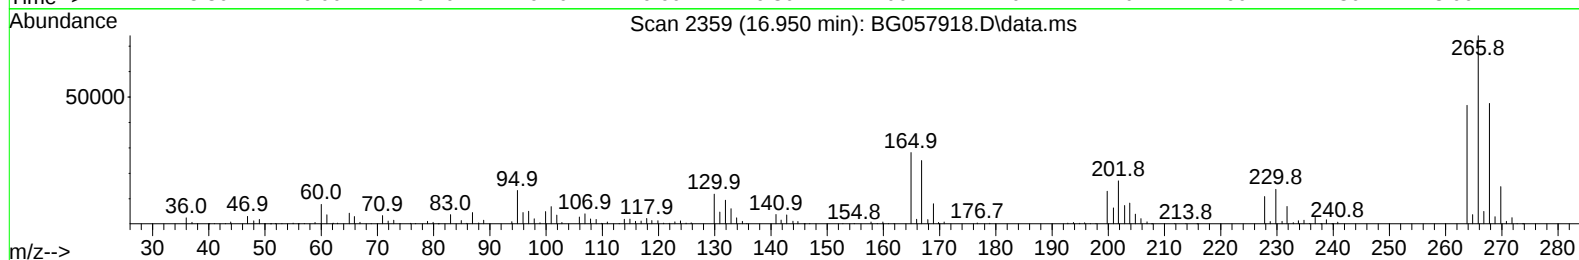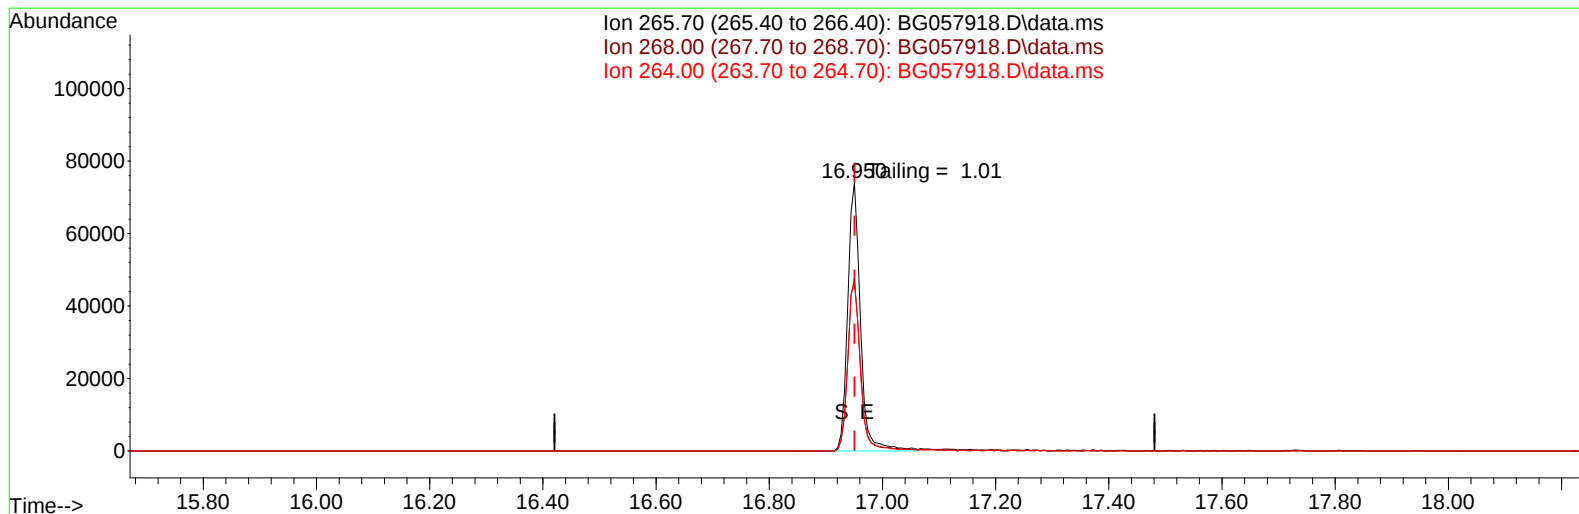

TIC: BG057918.D\data.ms

(70) Pentachlorophenol (C)

16.950min (-0.000) 193742.80 ng




response 115611

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	64.06
264.00	63.60	63.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG063023\
 Data File : BG057918.D
 Acq On : 30 Jun 2023 14:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 30 18:00:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 28 01:12:33 2023
 Response via : Initial Calibration

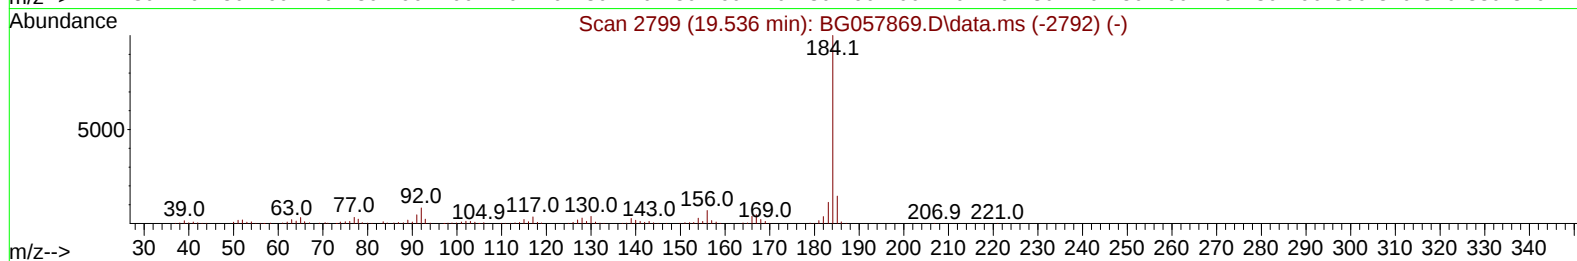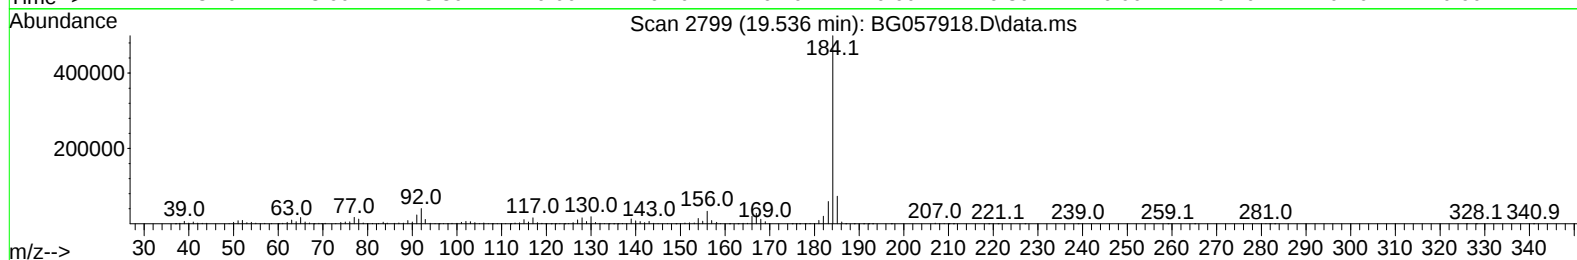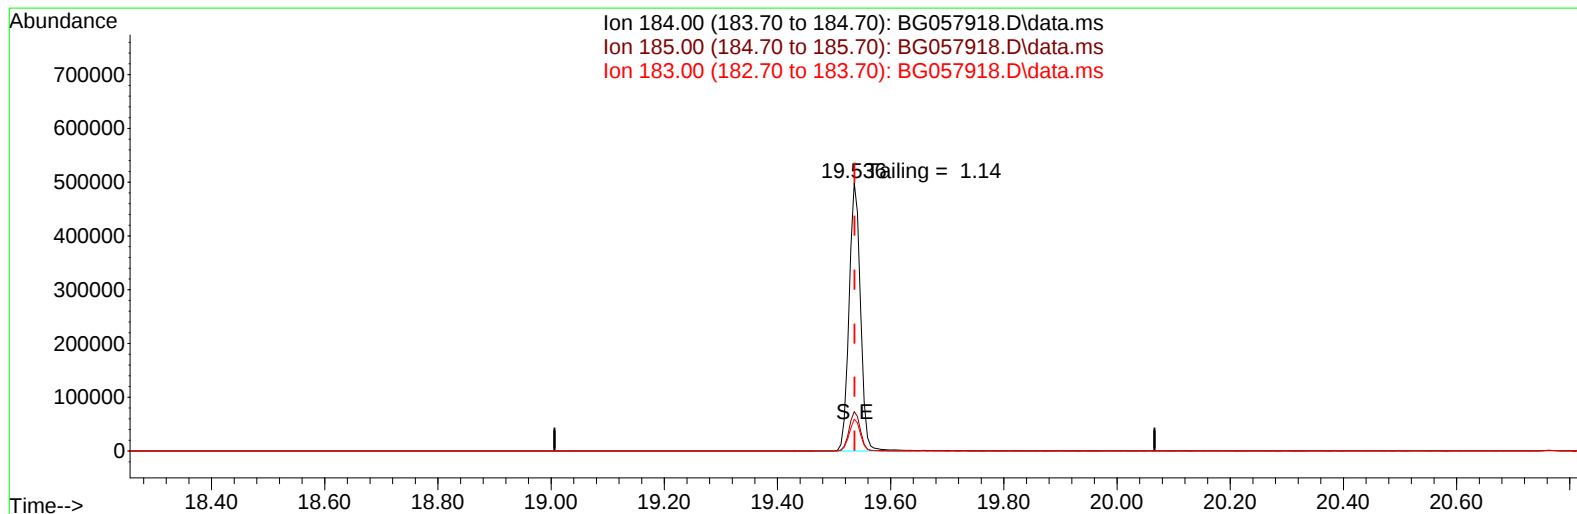

TIC: BG057918.D\data.ms

(77) Benzidine

19.536min (-0.000) 48514.75 ng

response 701134

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.66
183.00	11.20	11.88
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/30/2023	BNA_G	BG057918.D
Compound Name	Response	Retention Time
DDT	314753	20.764
DDD	6673	20.329
DDE	377	19.818
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7050	321803	2.19

Instrument :
BNA_G
ClientSampleId :
DFTPP