
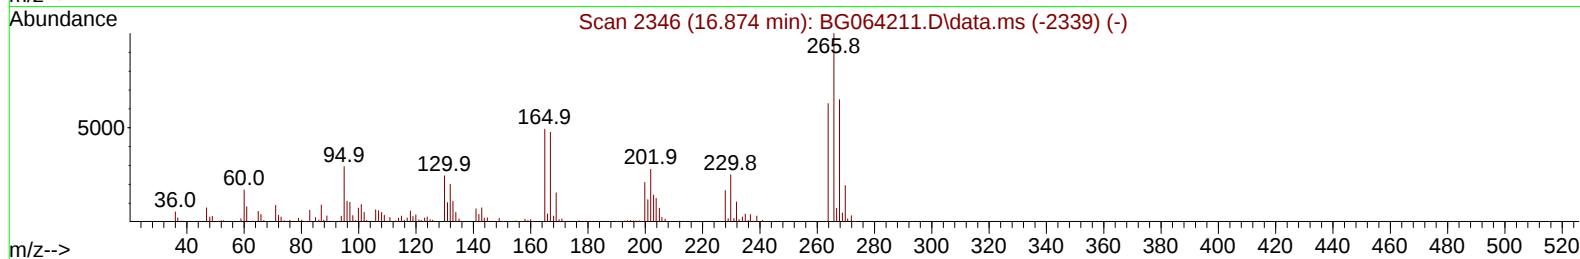
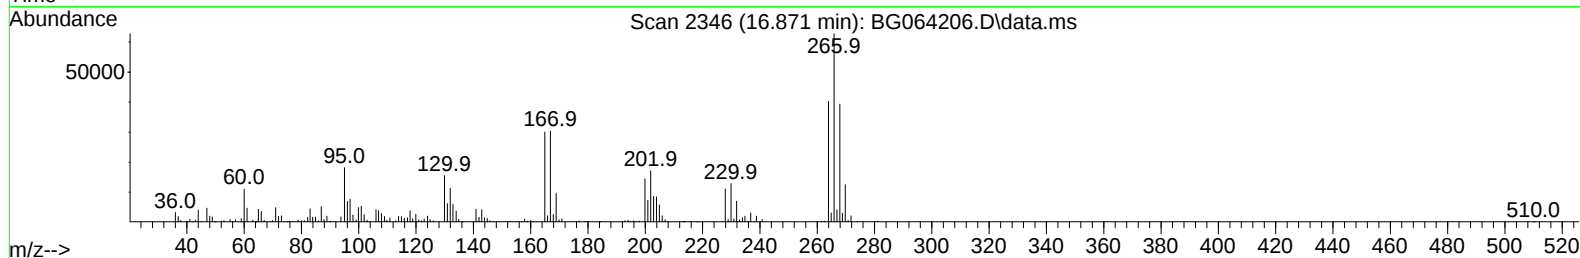


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082725\
Data File : BG064206.D
Acq On : 27 Aug 2025 11:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 27 18:05:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 27 18:02:44 2025
Response via : Initial Calibration

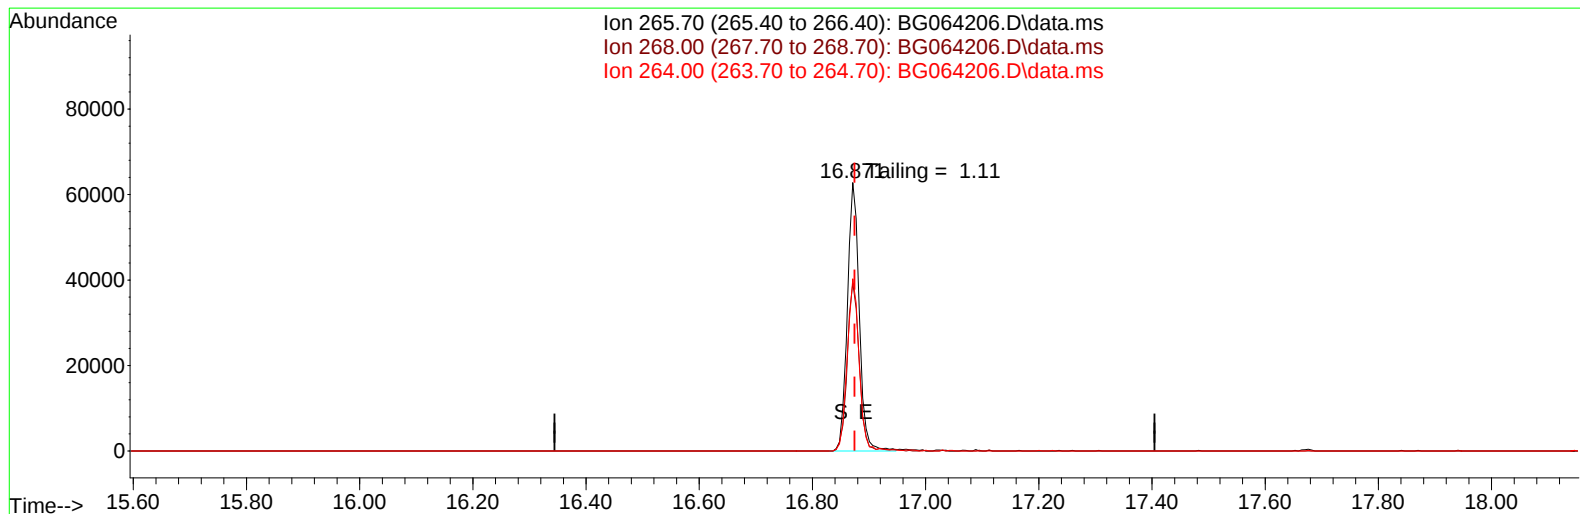

TIC: BG064206.D\data.ms

(70) Pentachlorophenol (C)




16.871min (-0.003) 25953.26 ng

response 91726

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	62.63
264.00	62.90	64.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082725\
Data File : BG064206.D
Acq On : 27 Aug 2025 11:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 27 18:05:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 27 18:02:44 2025
Response via : Initial Calibration

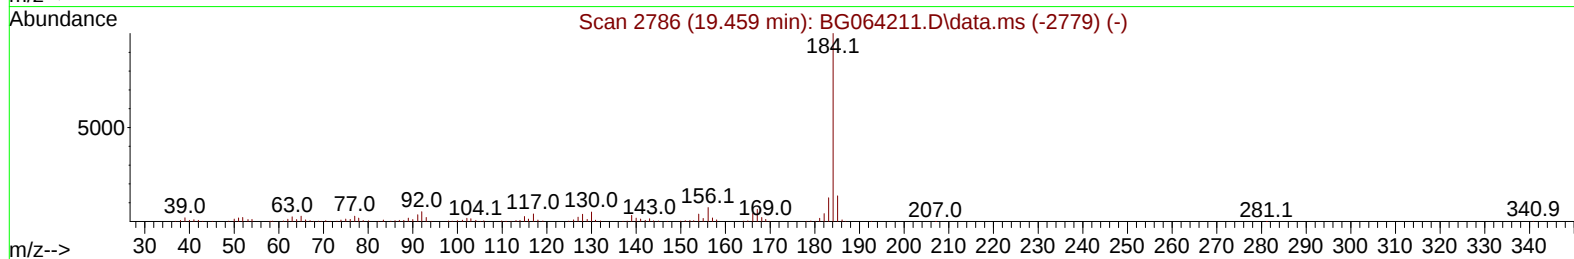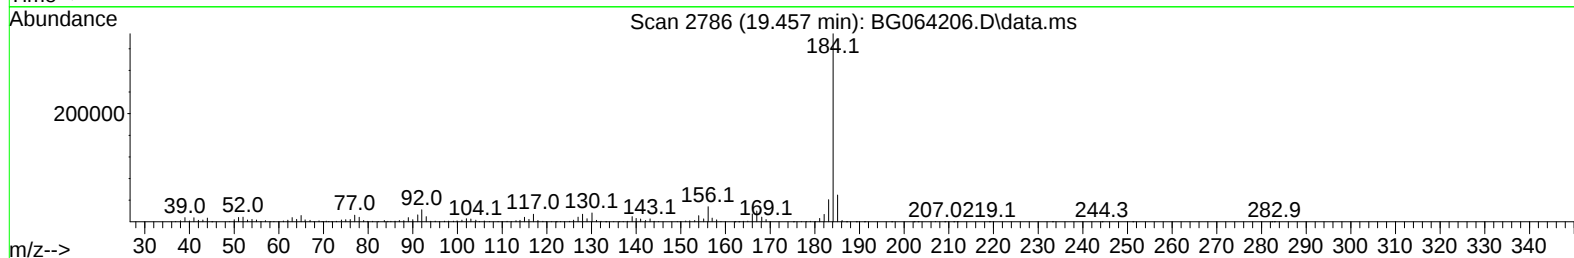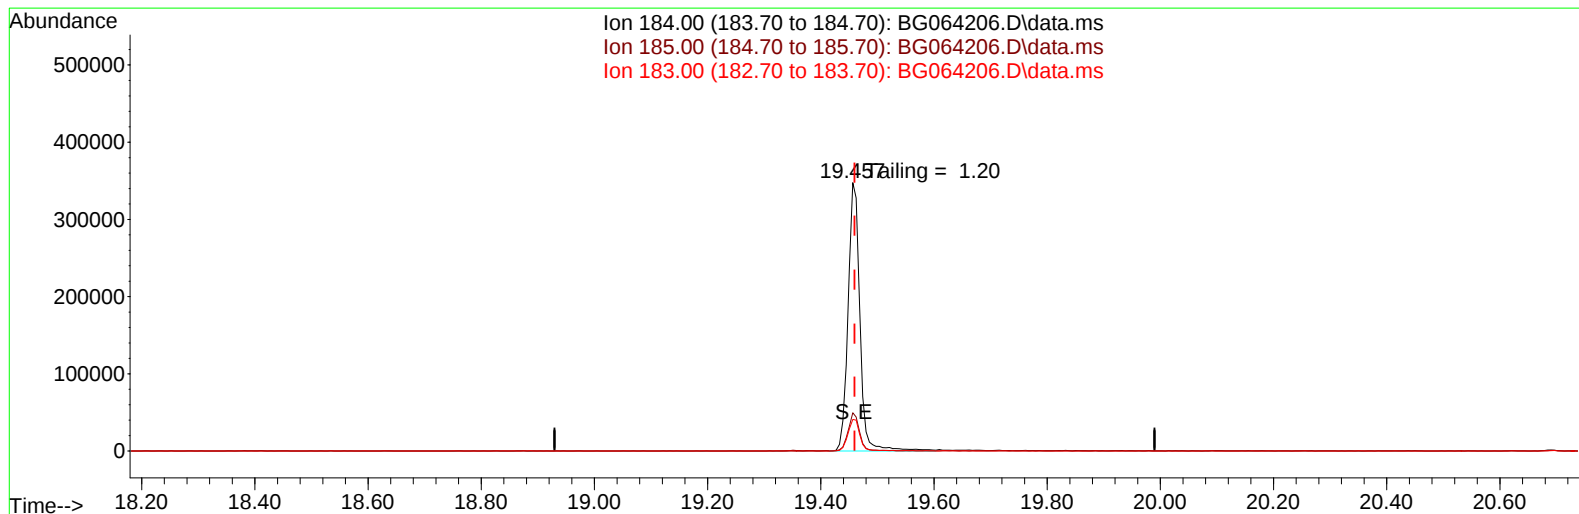

TIC: BG064206.D\data.ms

(77) Benzidine**19.457min (-0.003) 437609.98 ng****response 507353**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.28
183.00	12.60	11.78
0.00	0.00	0.00