
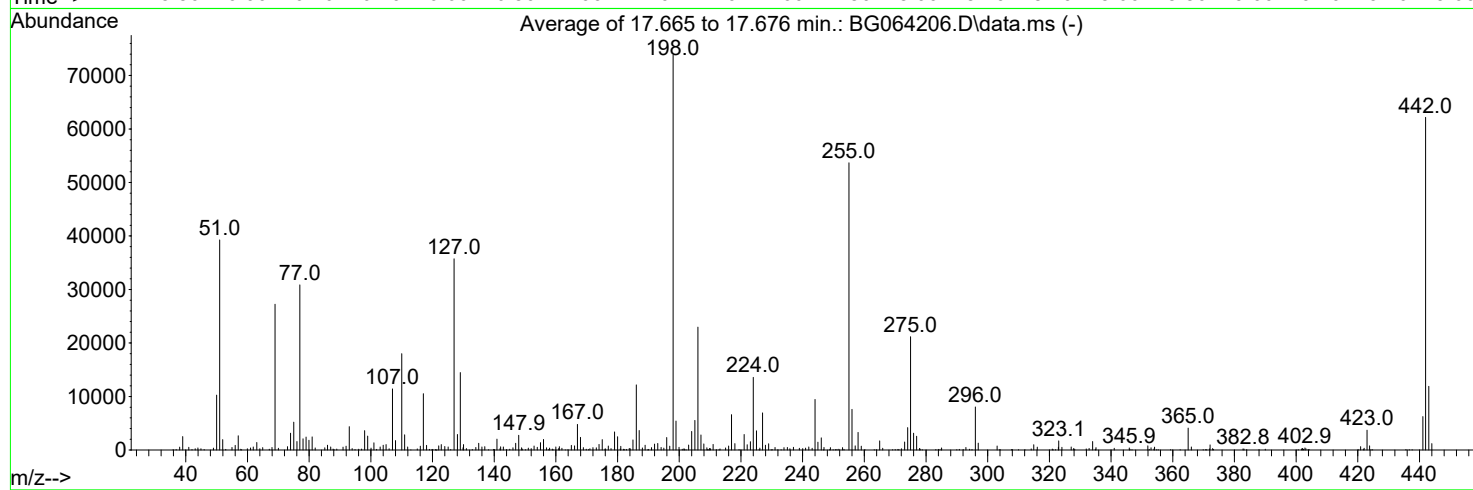


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082725\
Data File : BG064206.D
Acq On : 27 Aug 2025 11:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 27 18:02:44 2025

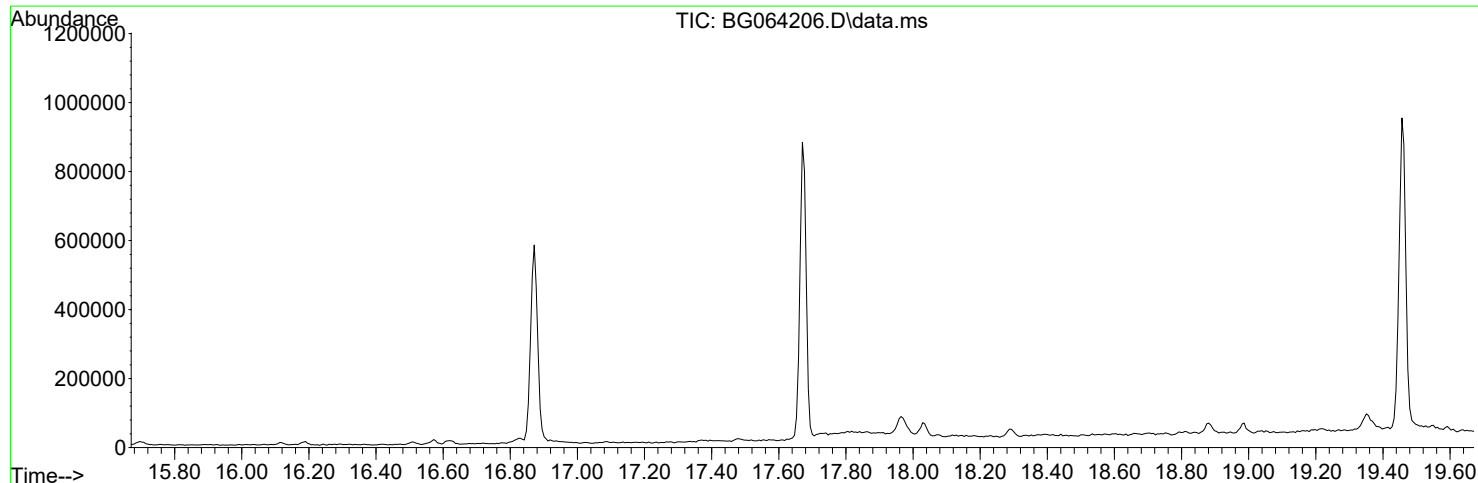

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.7	468	PASS
69	69	100	100	100.0	27248	PASS
70	69	0.00	2	1.2	321	PASS
197	198	0.00	2	1.0	719	PASS
198	198	100	100	100.0	73797	PASS
199	198	5	9	7.3	5418	PASS
365	198	1	100	5.6	4108	PASS
441	443	0.01	150	52.5	6257	PASS
442	442	100	100	100.0	62168	PASS
443	442	15	24	19.2	11913	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/27/2025	BNA_G	<u>BG064206.D</u>
Compound Name	Response	Retention Time
DDT	246912	20.69
DDD	3755	20.25
DDE	125	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3880	250792	1.55

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082725\
Data File : BG064206.D
Acq On : 27 Aug 2025 11:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 27 18:05:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 27 18:02:44 2025
Response via : Initial Calibration

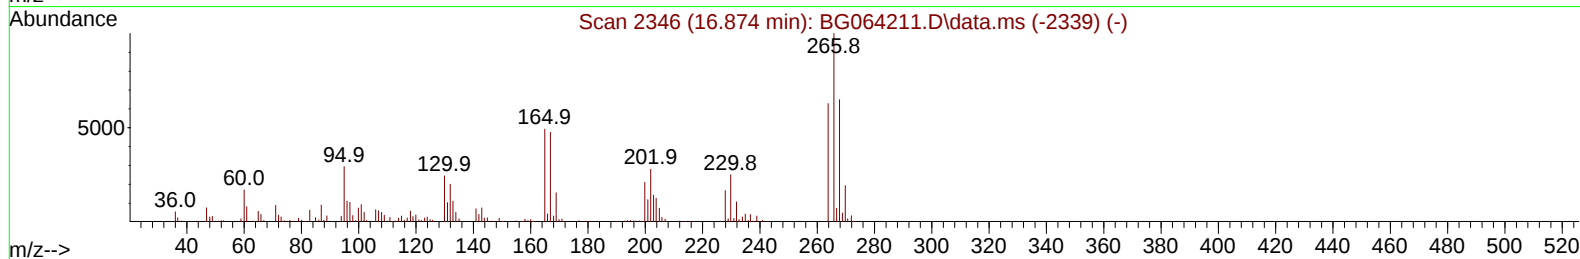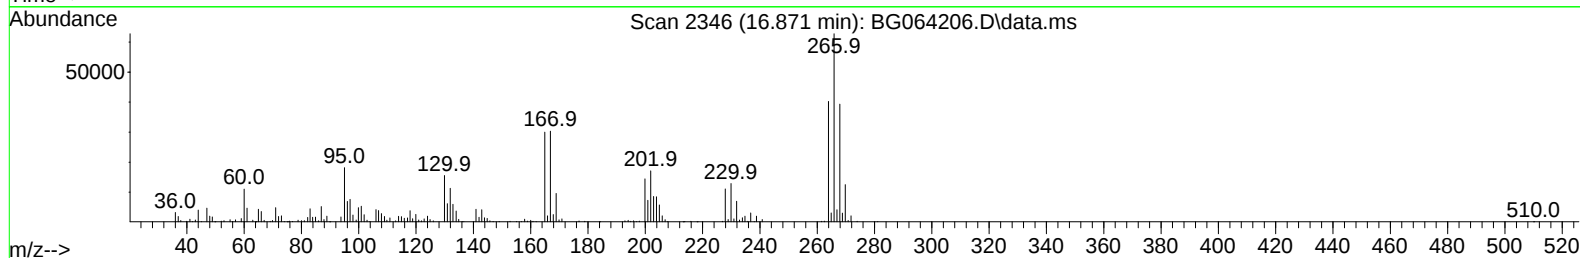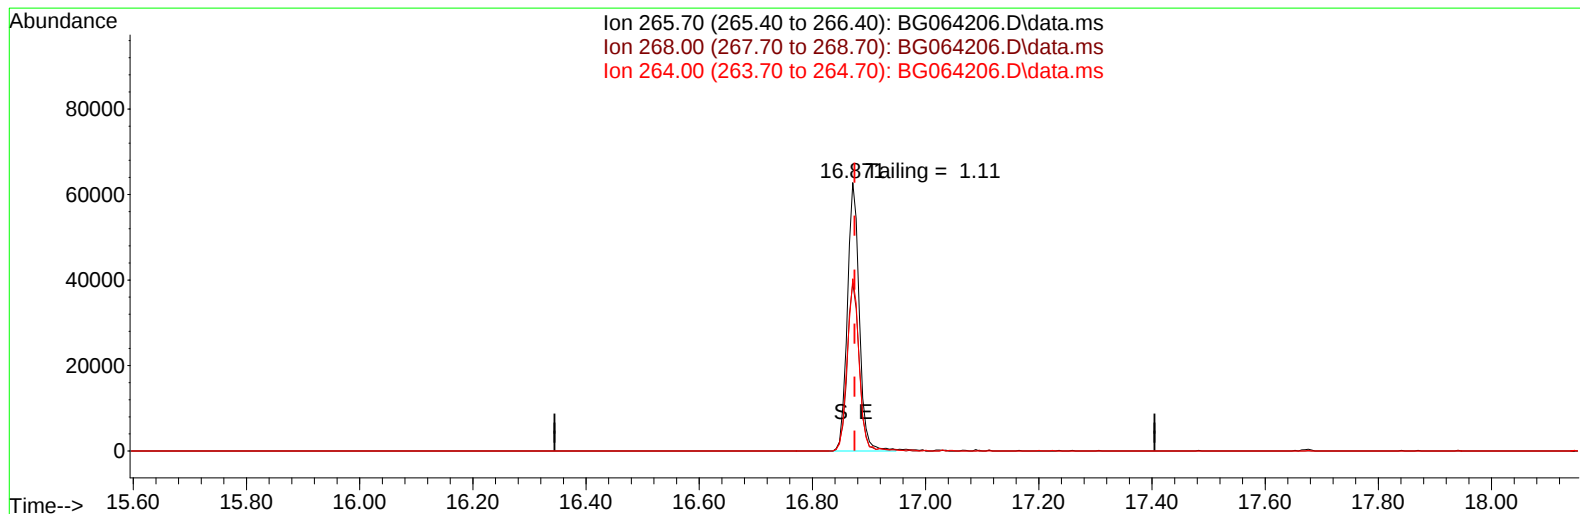

TIC: BG064206.D\data.ms

(70) Pentachlorophenol (C)

16.871min (-0.003) 25953.26 ng




response 91726

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	62.63
264.00	62.90	64.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082725\
Data File : BG064206.D
Acq On : 27 Aug 2025 11:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 27 18:05:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 27 18:02:44 2025
Response via : Initial Calibration

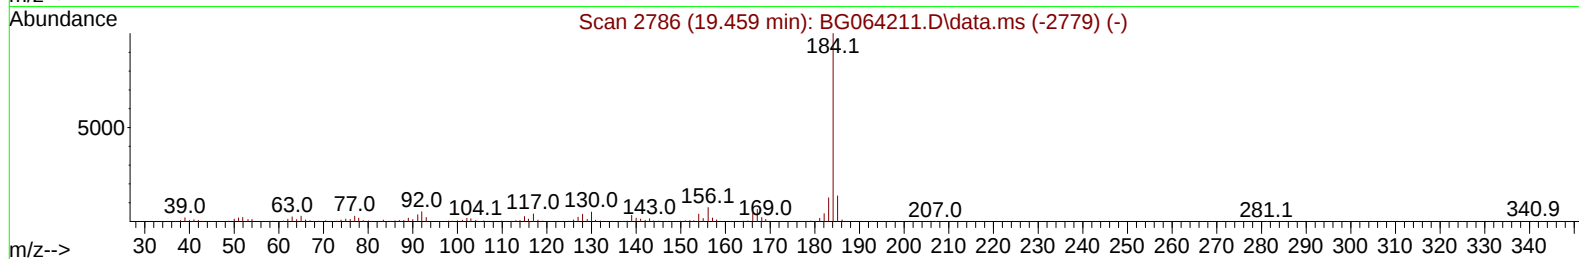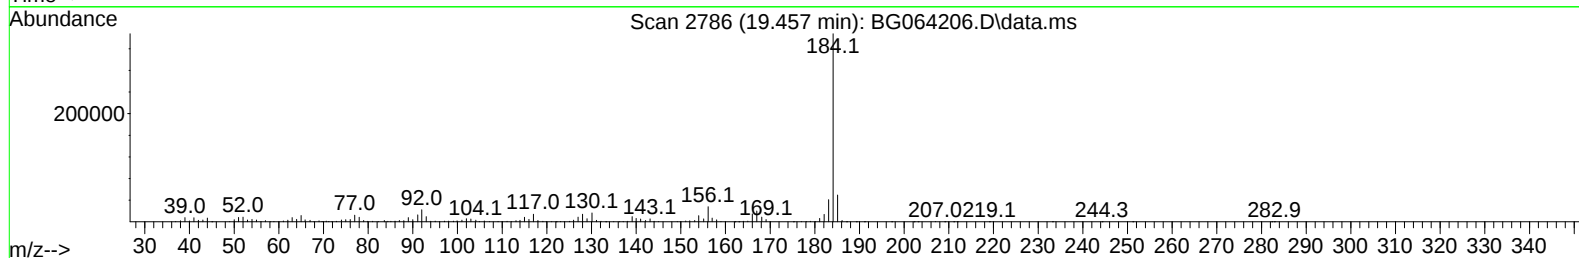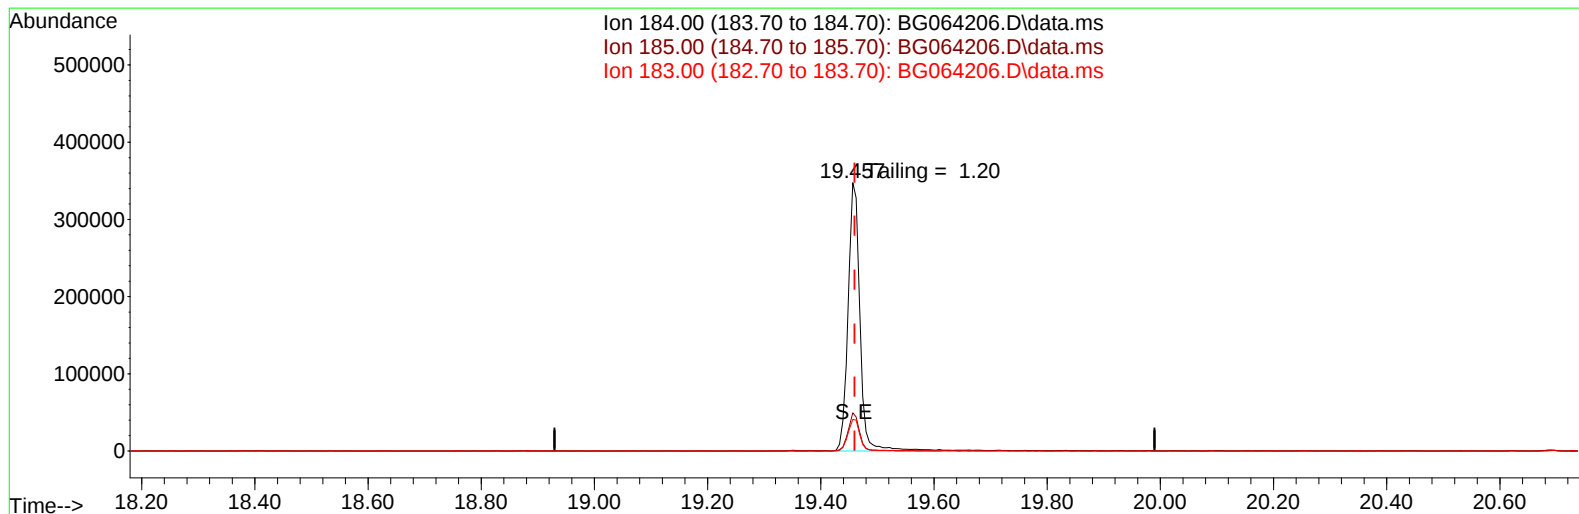

TIC: BG064206.D\data.ms

(77) Benzidine

19.457min (-0.003) 437609.98 ng

response 507353

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.28
183.00	12.60	11.78
0.00	0.00	0.00