
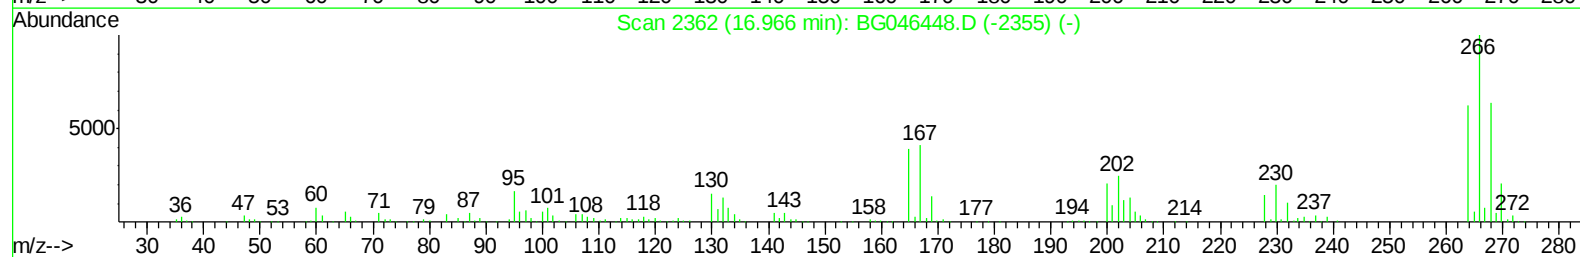
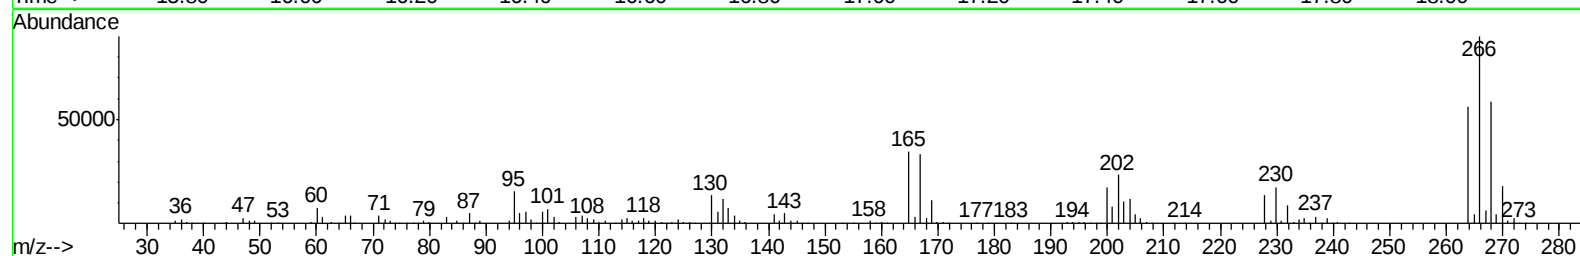


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090220\
 Data File : BG046498.D
 Acq On : 2 Sep 2020 8:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 07:39:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 02 15:06:53 2020
 Response via : Initial Calibration

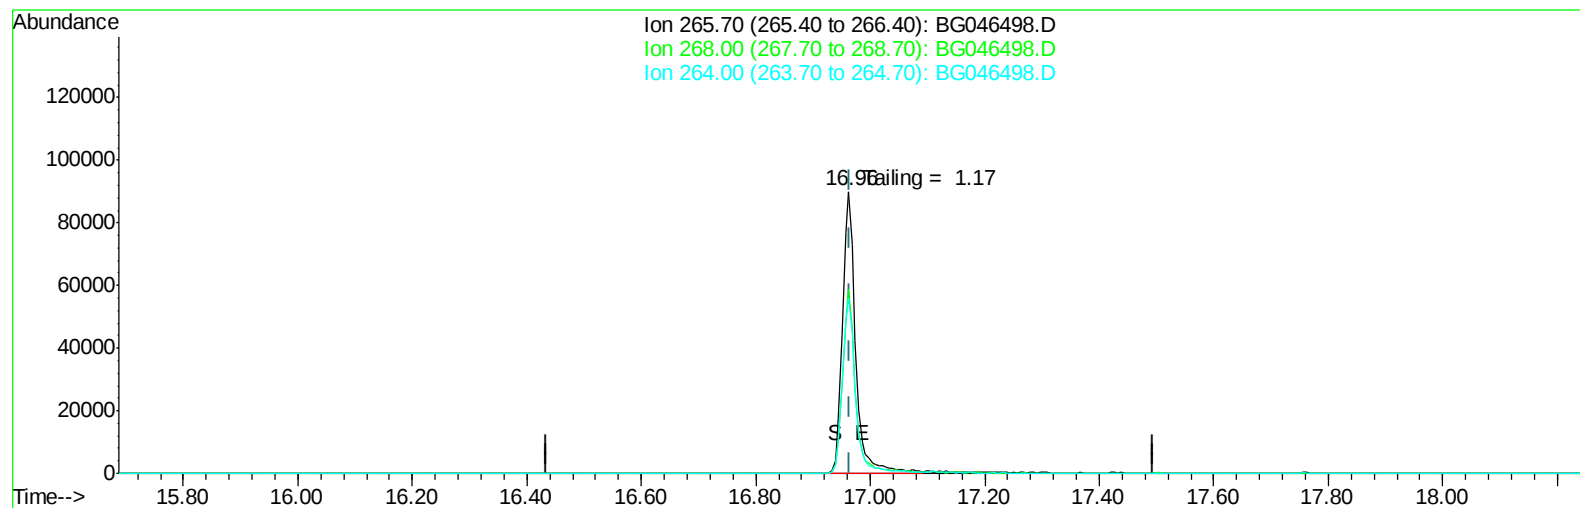

TIC: BG046498.D

(70) Pentachlorophenol (C)




16.962min (-0.003) 38947.12ng

response 146186

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.44
264.00	62.70	62.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090220\
 Data File : BG046498.D
 Acq On : 2 Sep 2020 8:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 07:39:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 02 15:06:53 2020
 Response via : Initial Calibration

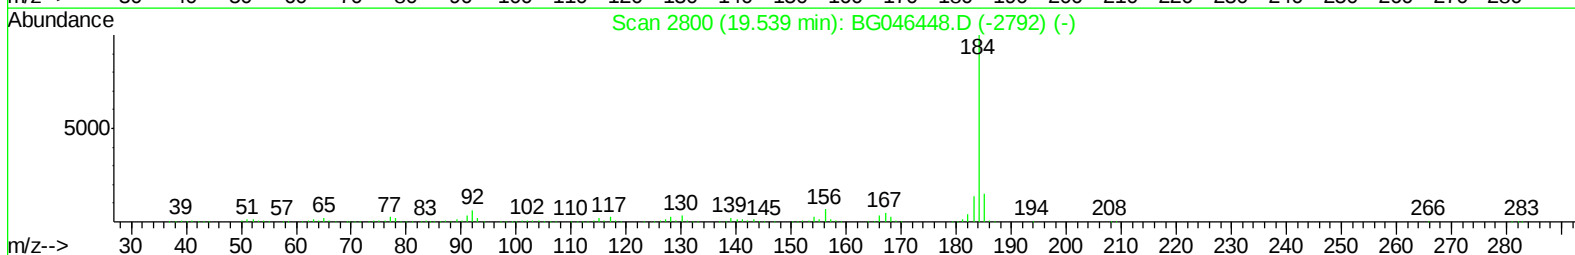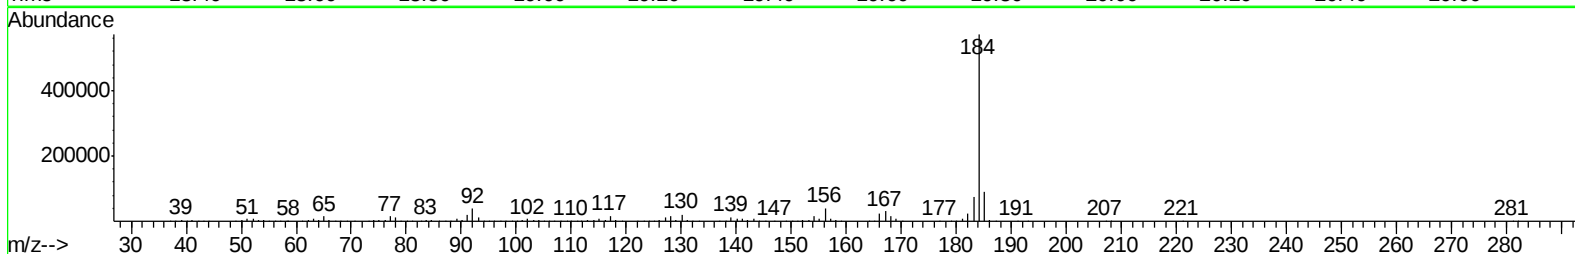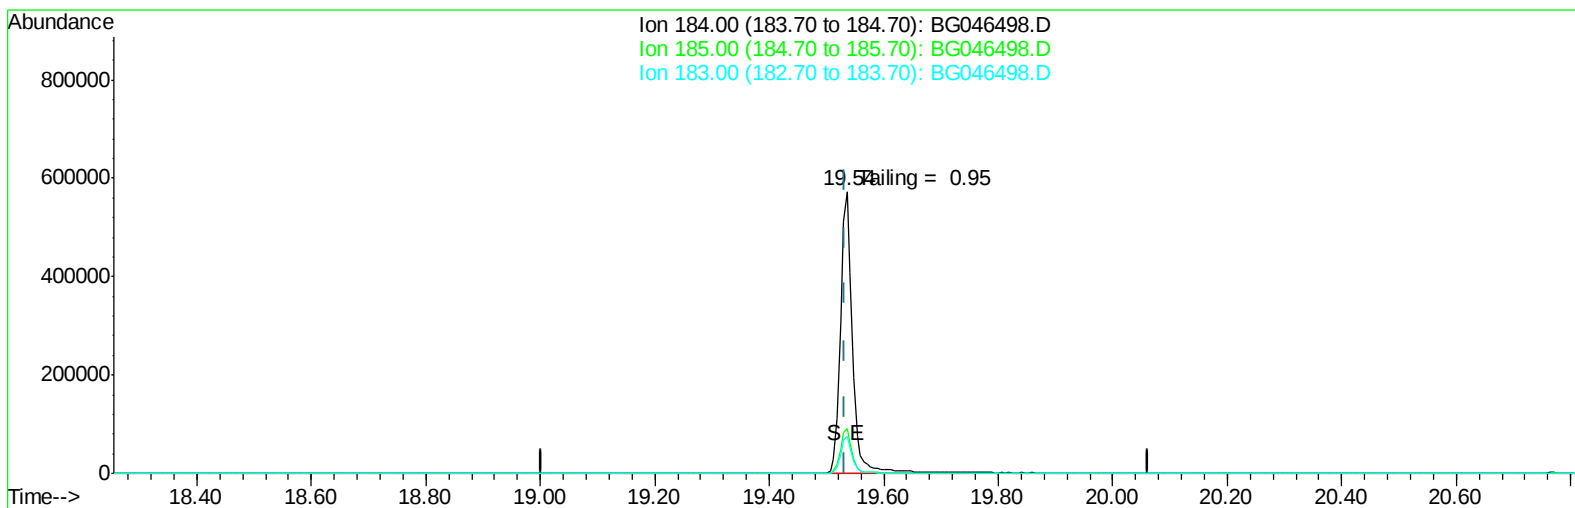

TIC: BG046498.D

(77) Benzidine

19.536min (+0.003) 0.00ng

response 860599

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	15.77
183.00	13.40	13.26
0.00	0.00	0.00