

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090420\
 Data File : BG046550.D
 Acq On : 4 Sep 2020 21:21
 Operator : CG/JU
 Sample : L3888-14 2X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 9-2-TP-4

Quant Time: Sep 05 03:02:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 02 15:06:53 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	75492	20.00	ng	0.00
21) Naphthalene-d8	10.73	136	312917	20.00	ng	0.00
39) Acenaphthene-d10	14.56	164	219718	20.00	ng	0.00
64) Phenanthrene-d10	17.30	188	481310	20.00	ng	0.00
76) Chrysene-d12	21.55	240	458968	20.00	ng	0.00
86) Perylene-d12	24.66	264	456913	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.52	112	166228	39.00	ng	0.00
7) Phenol-d6	7.10	99	221293	36.62	ng	0.00
23) Nitrobenzene-d5	9.08	82	147231	26.89	ng	0.00
42) 2,4,6-Tribromophenol	16.05	330	102055	34.28	ng	0.00
45) 2-Fluorobiphenyl	13.18	172	375044	26.06	ng	0.00
79) Terphenyl-d14	19.92	244	497086	23.05	ng	0.00
Target Compounds						
50) Dimethylphthalate	14.01	163	34999	2.059	ng	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090420\
Data File : BG046550.D
Acq On : 4 Sep 2020 21:21
Operator : CG/JU
Sample : L3888-14 2X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
9-2-TP-4

Quant Time: Sep 05 03:02:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 15:06:53 2020
Response via : Initial Calibration

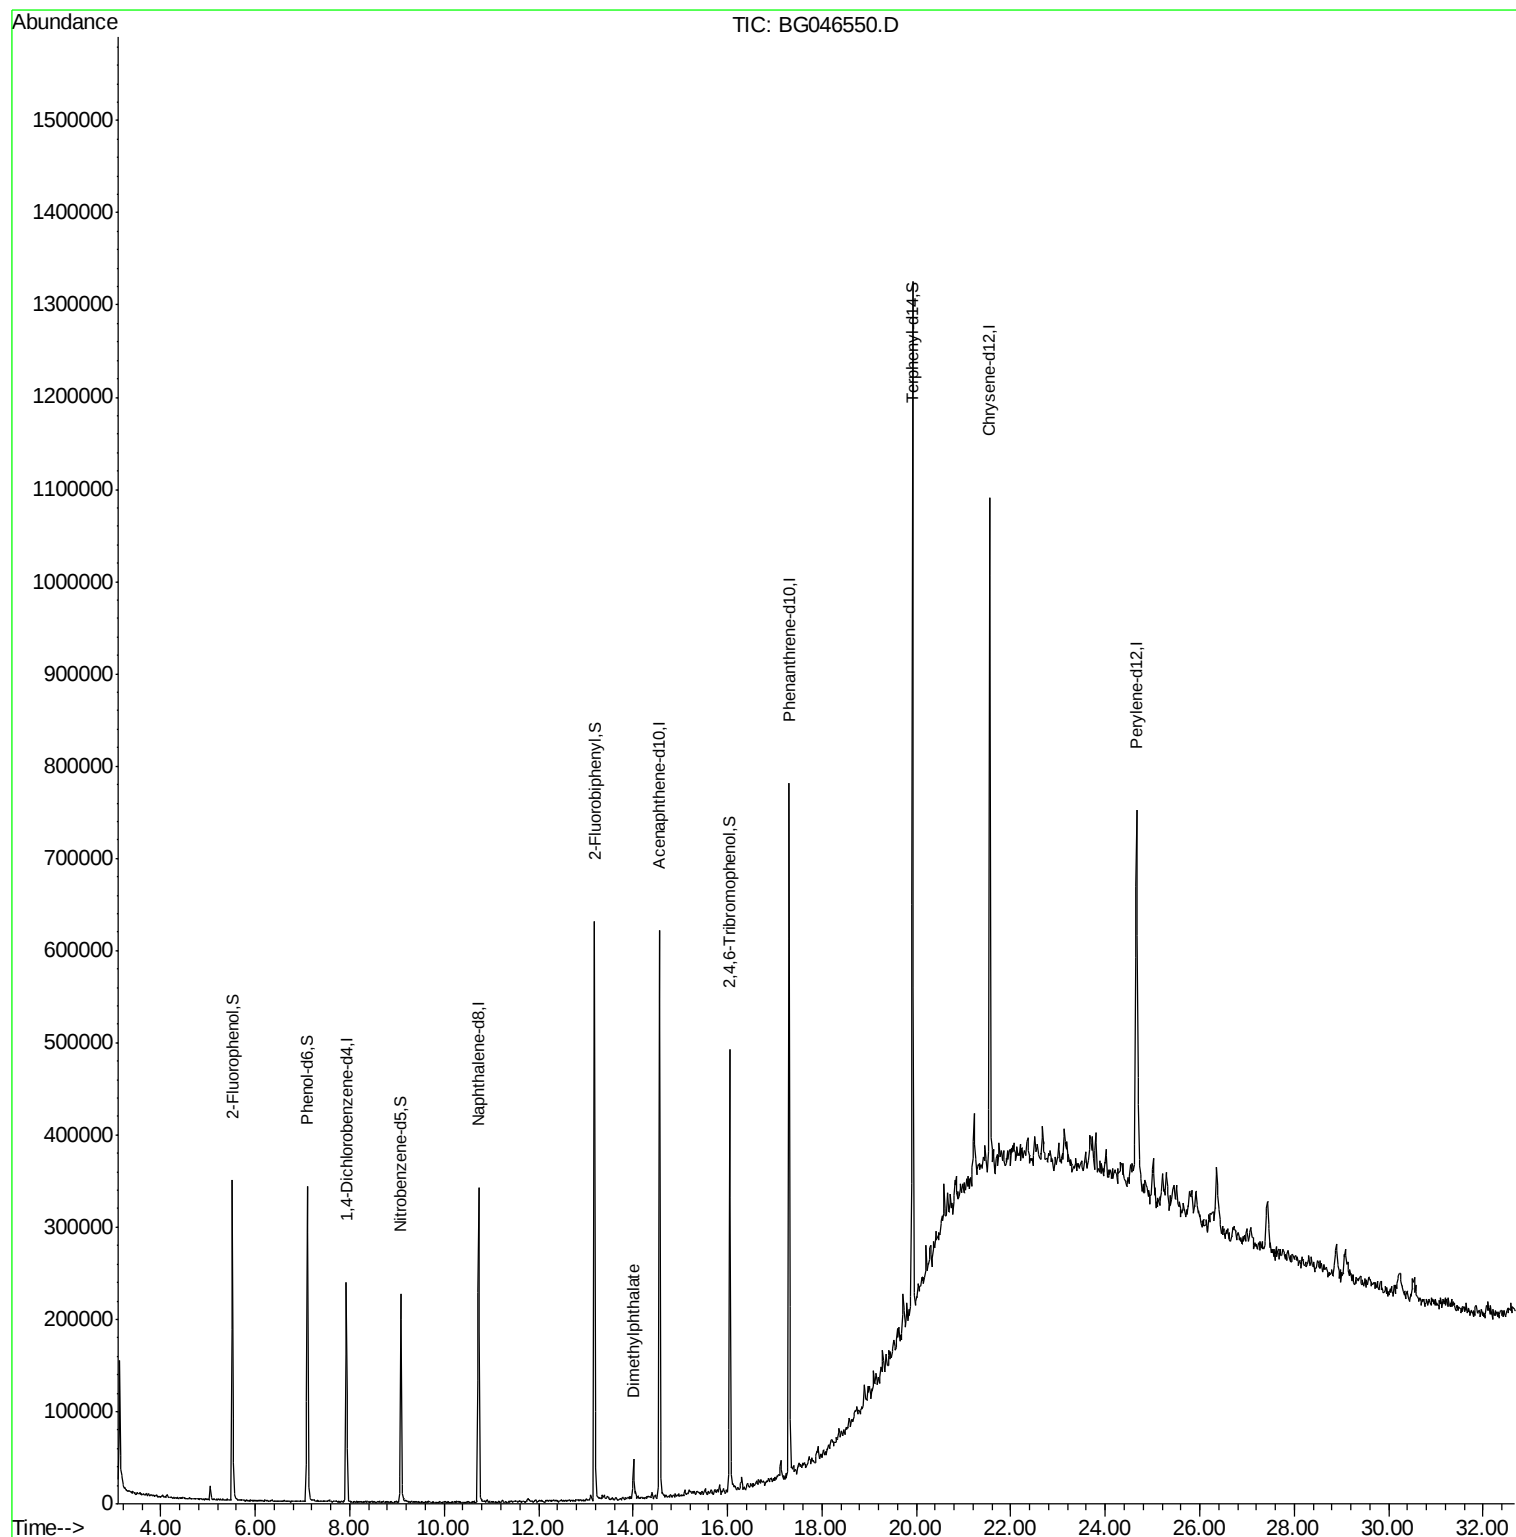

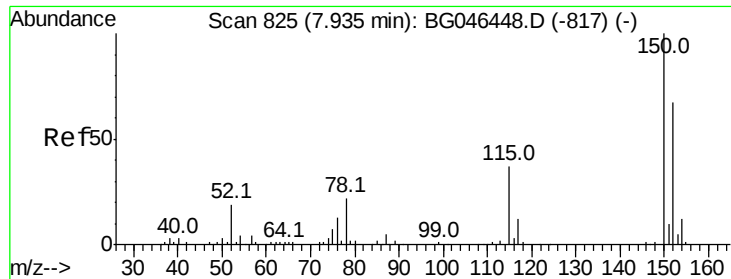


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.93 min Scan# 824
 Delta R.T. -0.00 min
 Lab File: BG046550.D
 Acq: 4 Sep 2020 21:21

Instrument :
 BNA_G
 ClientSampleId :
 9-2-TP-4

Tot Ion:152 Resp: 75492
 Ion Ratio Lower Upper
 152 100
 150 148.9 119.5 179.3
 115 53.6 44.3 66.5

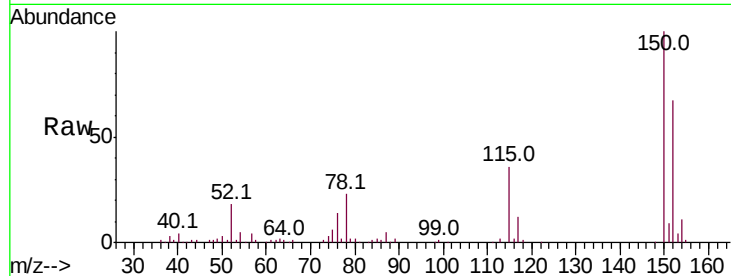


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

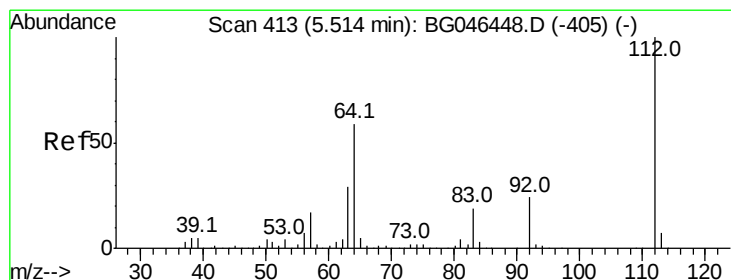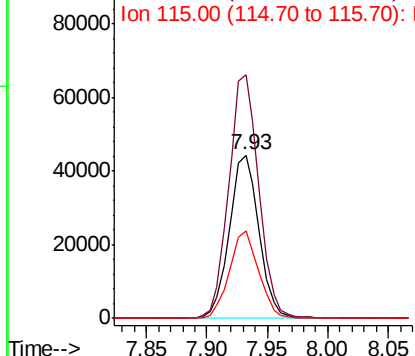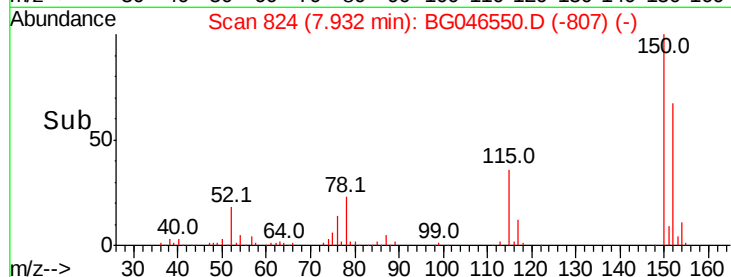



#5


2-Fluorophenol
 Concen: 39.000 ng
 RT: 5.52 min Scan# 413
 Delta R.T. 0.00 min
 Lab File: BG046550.D
 Acq: 4 Sep 2020 21:21

Tgt Ion:112 Resp: 166228
 Ion Ratio Lower Upper
 112 100
 64 60.7 47.0 70.6
 63 30.0 23.5 35.3

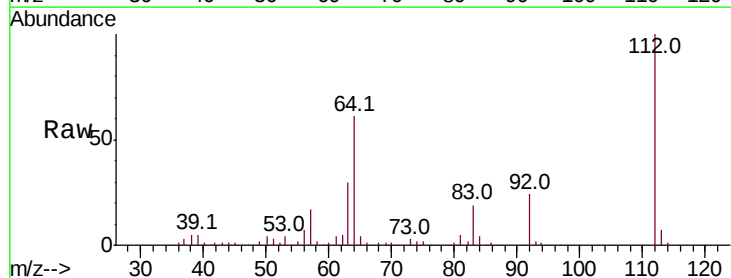

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BGC
 Ion 63.00 (62.70 to 63.70): BGC

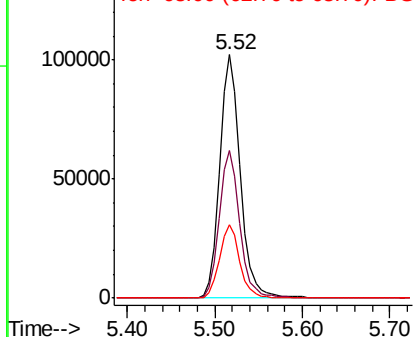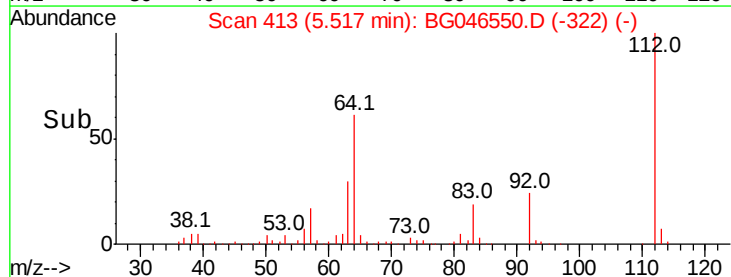

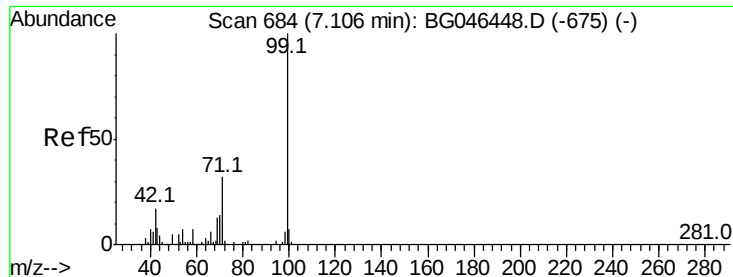

#7

Phenol-d6

Concen: 36.625 ng

RT: 7.10 min Scan# 683

Delta R.T. -0.00 min

Lab File: BG046550.D

Acq: 4 Sep 2020 21:21

Instrument :

BNA_G

ClientSampleId :

9-2-TP-4


Tot Ion: 99 Resp: 221293

Ion Ratio Lower Upper




99 100

42 16.6 13.3 19.9

71 31.8 25.3 37.9

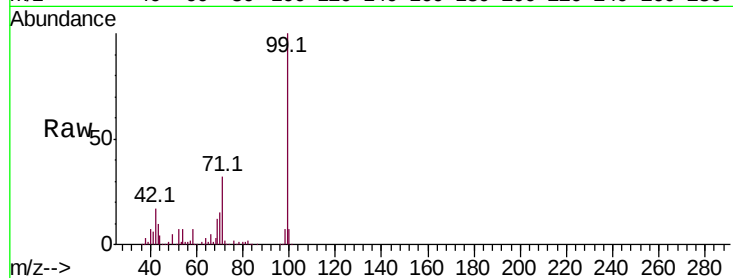

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

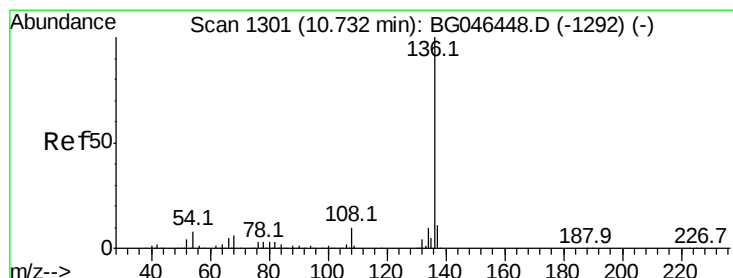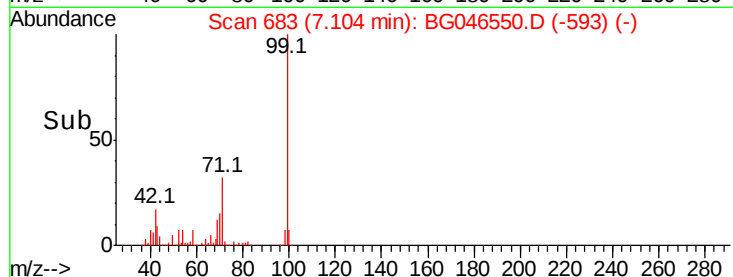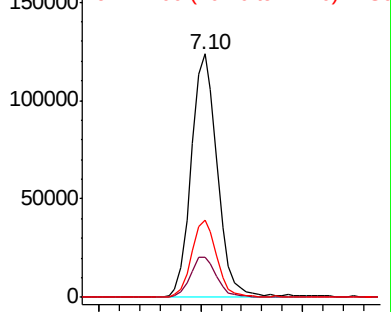

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.73 min Scan# 1300

Delta R.T. 0.00 min

Lab File: BG046550.D

Acq: 4 Sep 2020 21:21

Tgt Ion: 136 Resp: 312917


Ion Ratio Lower Upper

136 100



137 11.2 8.8 13.2


54 8.2 6.1 9.1

68 5.8 4.8 7.2

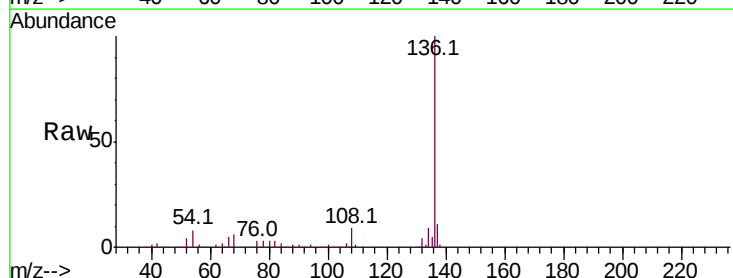

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



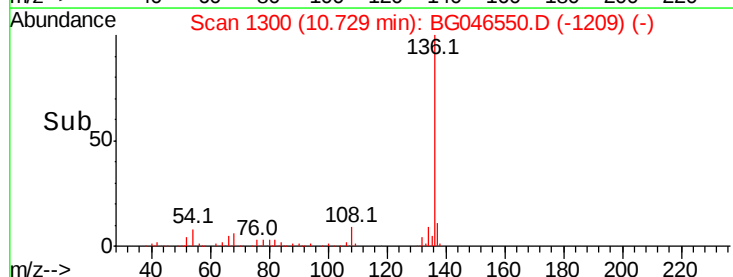
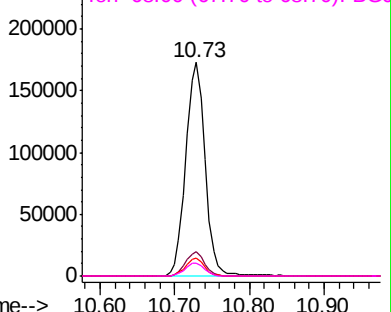


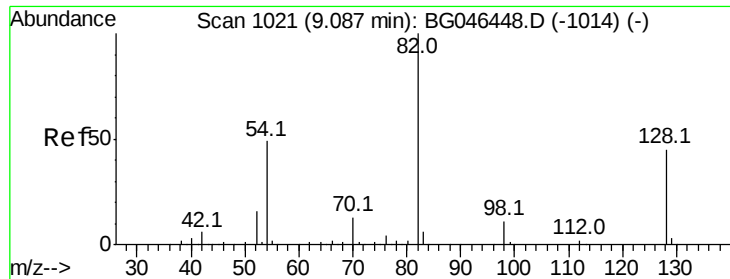

#23
 Nitrobenzene-d5
 Concen: 26.892 ng
 RT: 9.08 min Scan# 1020
 Delta R.T. -0.00 min
 Lab File: BG046550.D
 Acq: 4 Sep 2020 21:21




Instrument :
 BNA_G
 ClientSampleId :
 9-2-TP-4


Tot Ion	82	Resp	147231
Ion Ratio	Lower	Upper	
82	100		
128	44.3	35.7	53.5
54	46.6	39.4	59.0

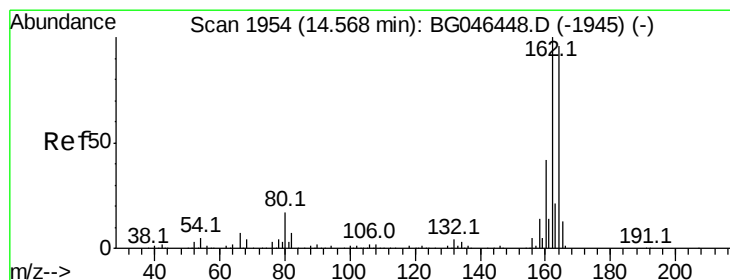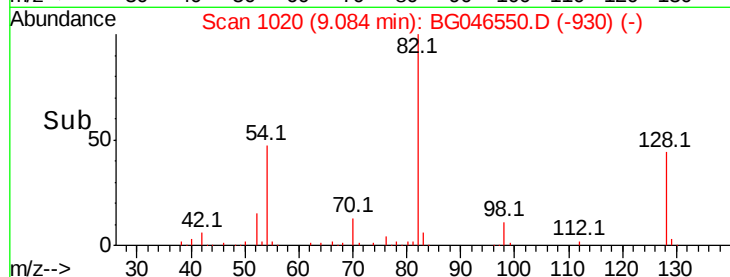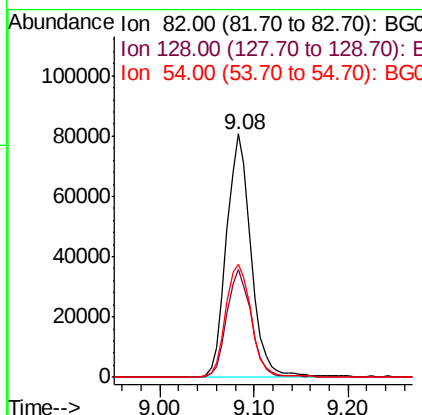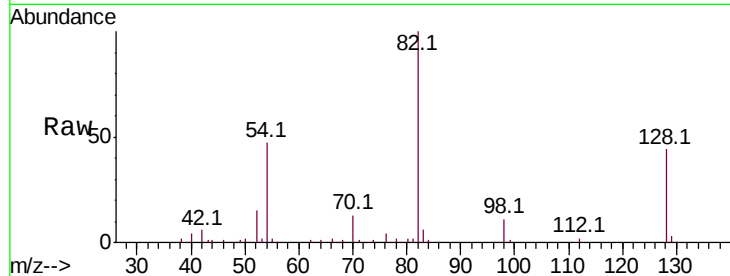

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.56 min Scan# 1952
 Delta R.T. -0.00 min
 Lab File: BG046550.D
 Acq: 4 Sep 2020 21:21

Tgt Ion	164	Resp	219718
Ion Ratio	Lower	Upper	
164	100		
162	101.2	83.3	124.9
160	44.2	35.0	52.6

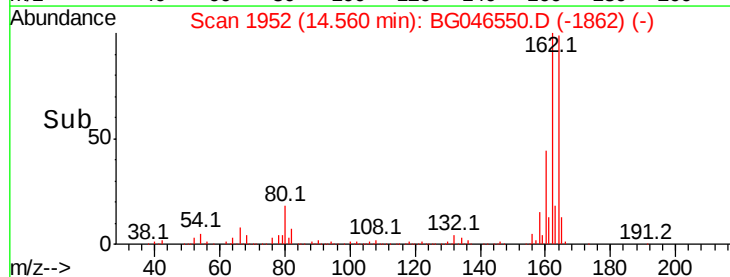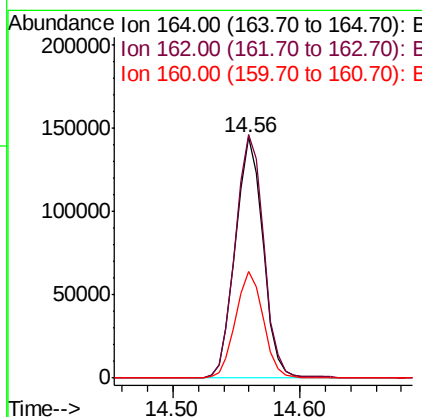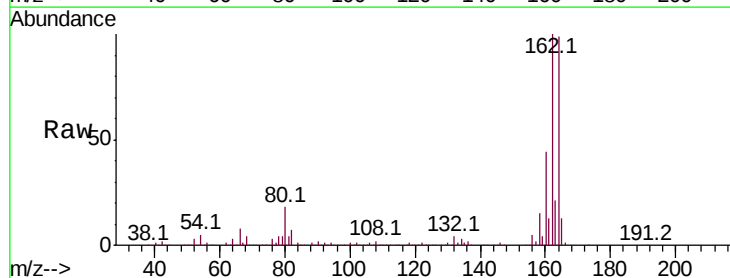


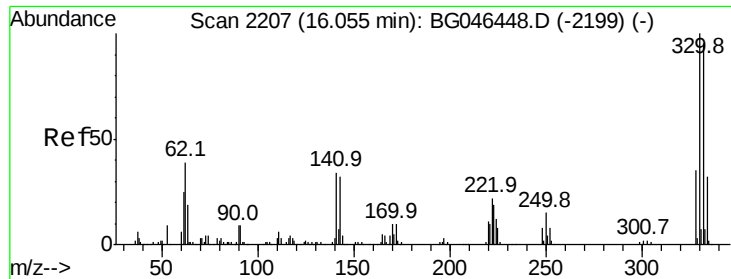




#42
 2,4,6-Tribromophenol
 Concen: 34.281 ng
 RT: 16.05 min Scan# 2206
 Delta R.T. 0.00 min
 Lab File: BG046550.D
 Acq: 4 Sep 2020 21:21

Instrument :
 BNA_G
 ClientSampleId :
 9-2-TP-4

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.3	76.1	114.1
141	34.1	26.1	39.1

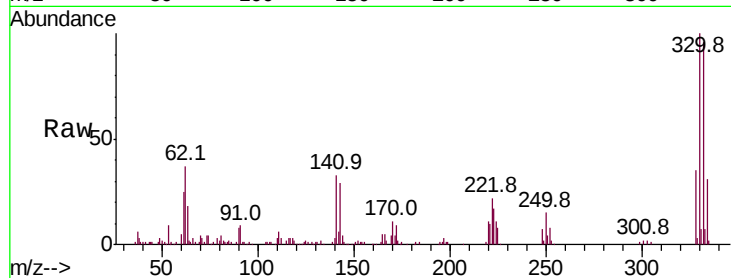


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

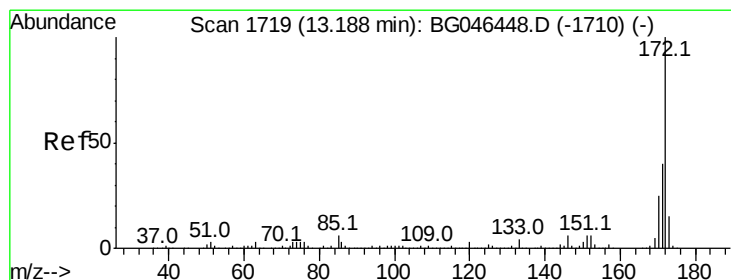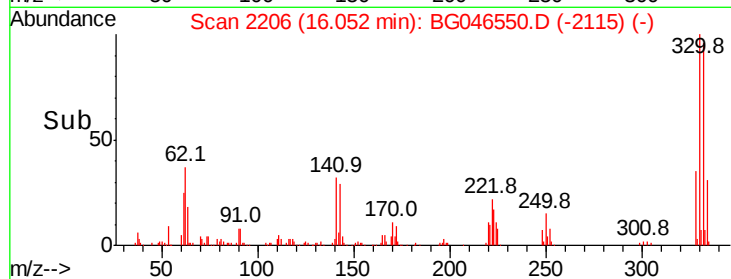
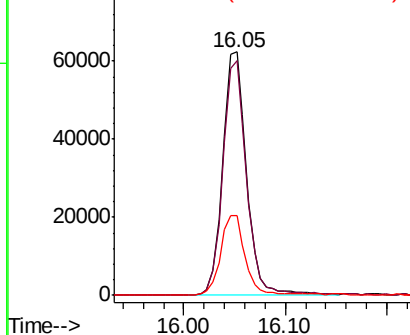



#45
 2-Fluorobiphenyl
 Concen: 26.057 ng
 RT: 13.18 min Scan# 1718
 Delta R.T. -0.00 min
 Lab File: BG046550.D
 Acq: 4 Sep 2020 21:21

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.3	31.8	47.6
170	23.4	20.3	30.5

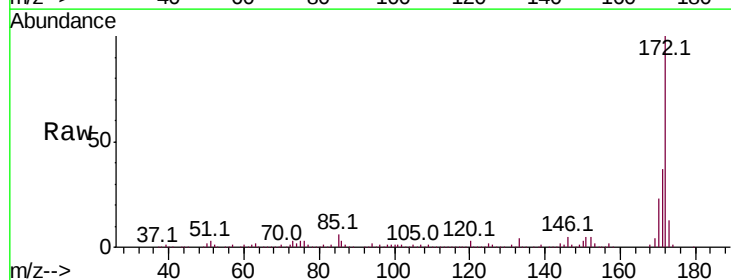

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

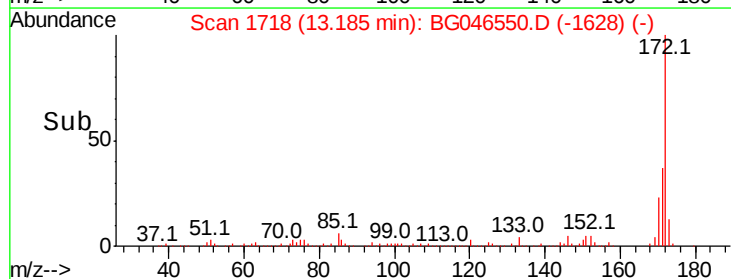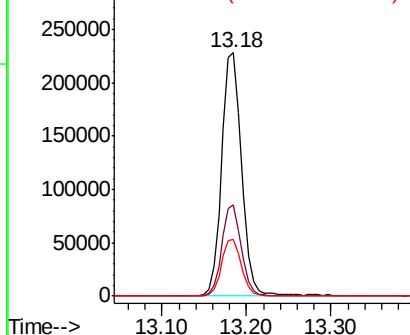

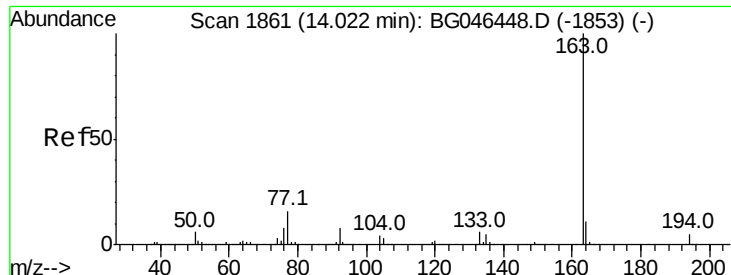

#50

Dimethylphthalate

Concen: 2.059 ng

RT: 14.01 min Scan# 1859

Delta R.T. -0.00 min

Lab File: BG046550.D

Acq: 4 Sep 2020 21:21

Instrument :

BNA_G

ClientSampled :

9-2-TP-4


Tot Ion:163 Resp: 34999

Ion Ratio Lower Upper

163 100

194 4.2 3.7 5.5




164 9.4 8.6 12.8

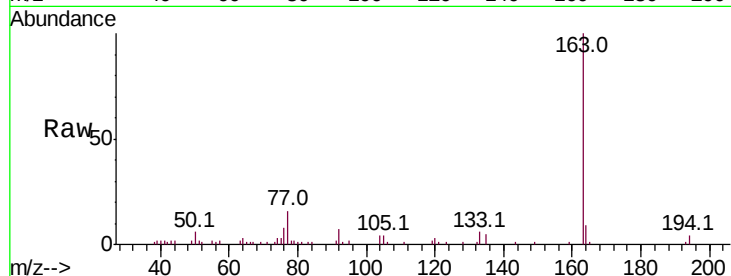

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

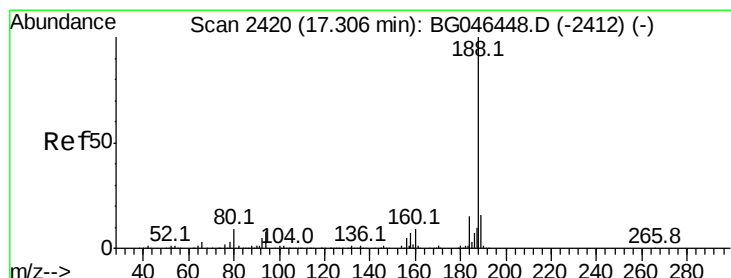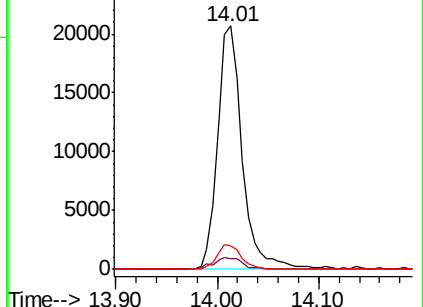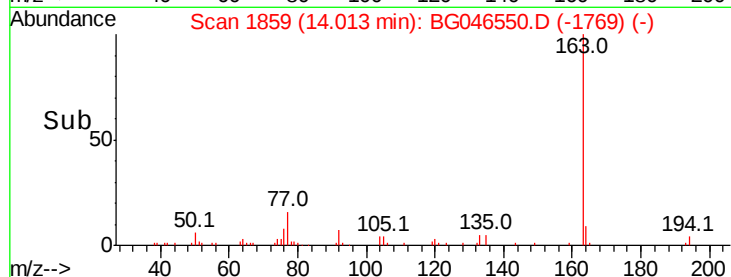

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.30 min Scan# 2419

Delta R.T. -0.00 min

Lab File: BG046550.D

Acq: 4 Sep 2020 21:21


Tgt Ion:188 Resp: 481310

Ion Ratio Lower Upper

188 100

94 7.6 6.3 9.5



80 9.0 6.9 10.3

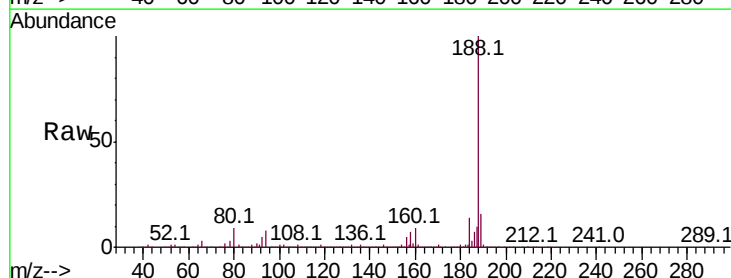


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

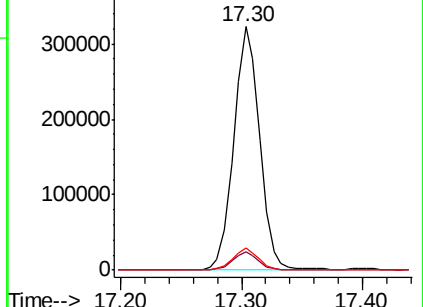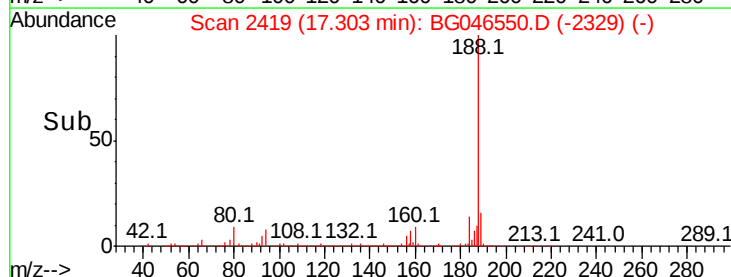


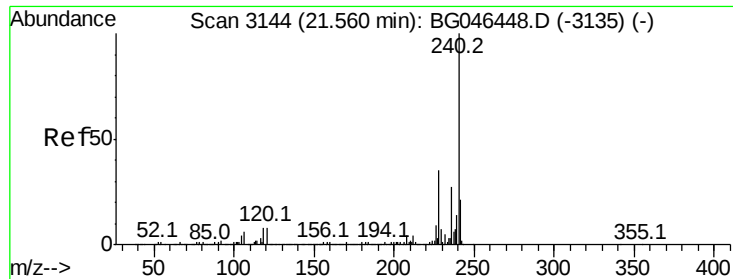




#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.55 min Scan# 3142
Delta R.T. -0.00 min
Lab File: BG046550.D
Acq: 4 Sep 2020 21:21

Instrument :
BNA_G
ClientSampleId :
9-2-TP-4

Tot Ion:240 Resp: 458968
Ion Ratio Lower Upper
240 100
120 8.6 6.6 10.0
236 27.4 21.4 32.2

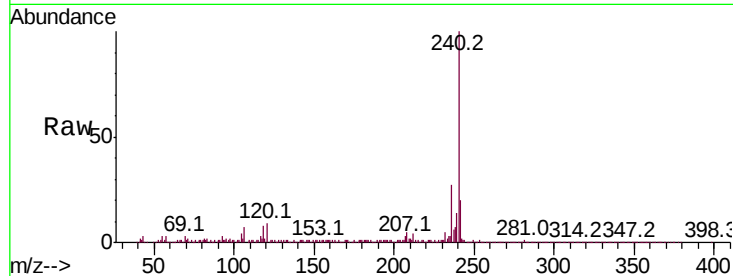


Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

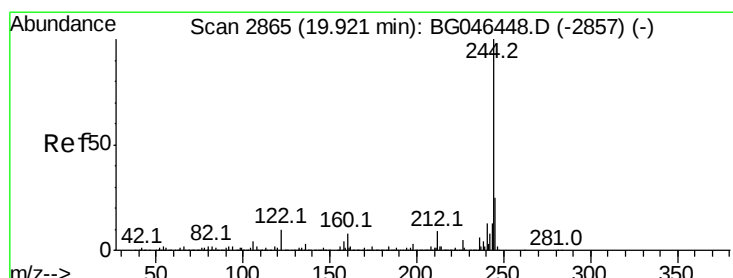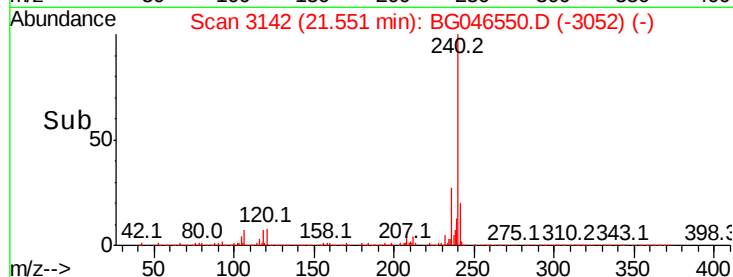
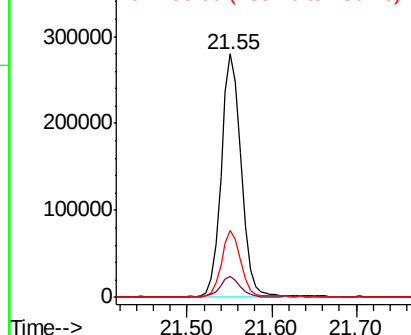



#79
Terphenyl-d14
Concen: 23.049 ng
RT: 19.92 min Scan# 2864
Delta R.T. -0.00 min
Lab File: BG046550.D
Acq: 4 Sep 2020 21:21

Tgt Ion:244 Resp: 497086
Ion Ratio Lower Upper
244 100
212 7.3 6.9 10.3
122 8.2 8.2 12.4

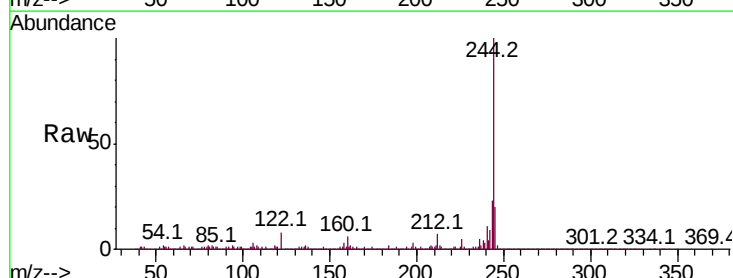

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

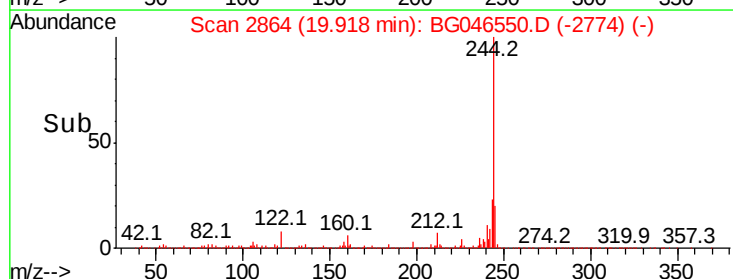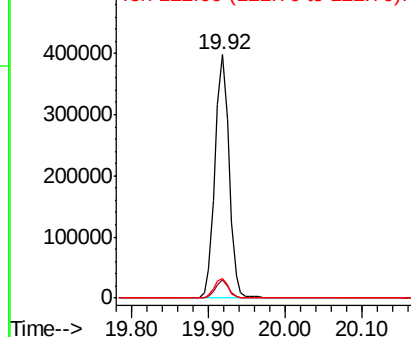

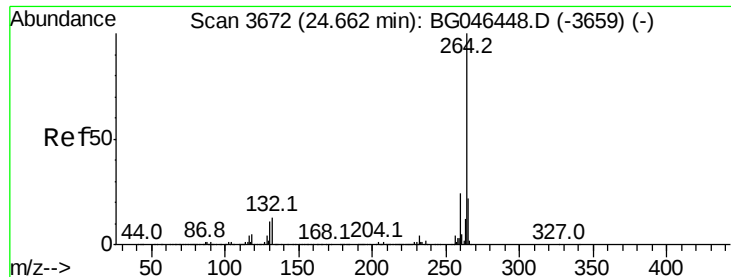

#86
Pervlene-d12
Concen: 20.000 ng
RT: 24.66 min Scan# 3671
Delta R.T. 0.00 min
Lab File: BG046550.D
Acq: 4 Sep 2020 21:21

Instrument :
BNA_G
ClientSampleId :
9-2-TP-4

Tot Ion	Ion	Ratio	Lower	Upper
264	100			
260	24.3	19.2	28.8	
265	22.1	17.9	26.9	

