


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090420\
 Data File : BG046533.D
 Acq On : 4 Sep 2020 9:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 02 15:06:53 2020

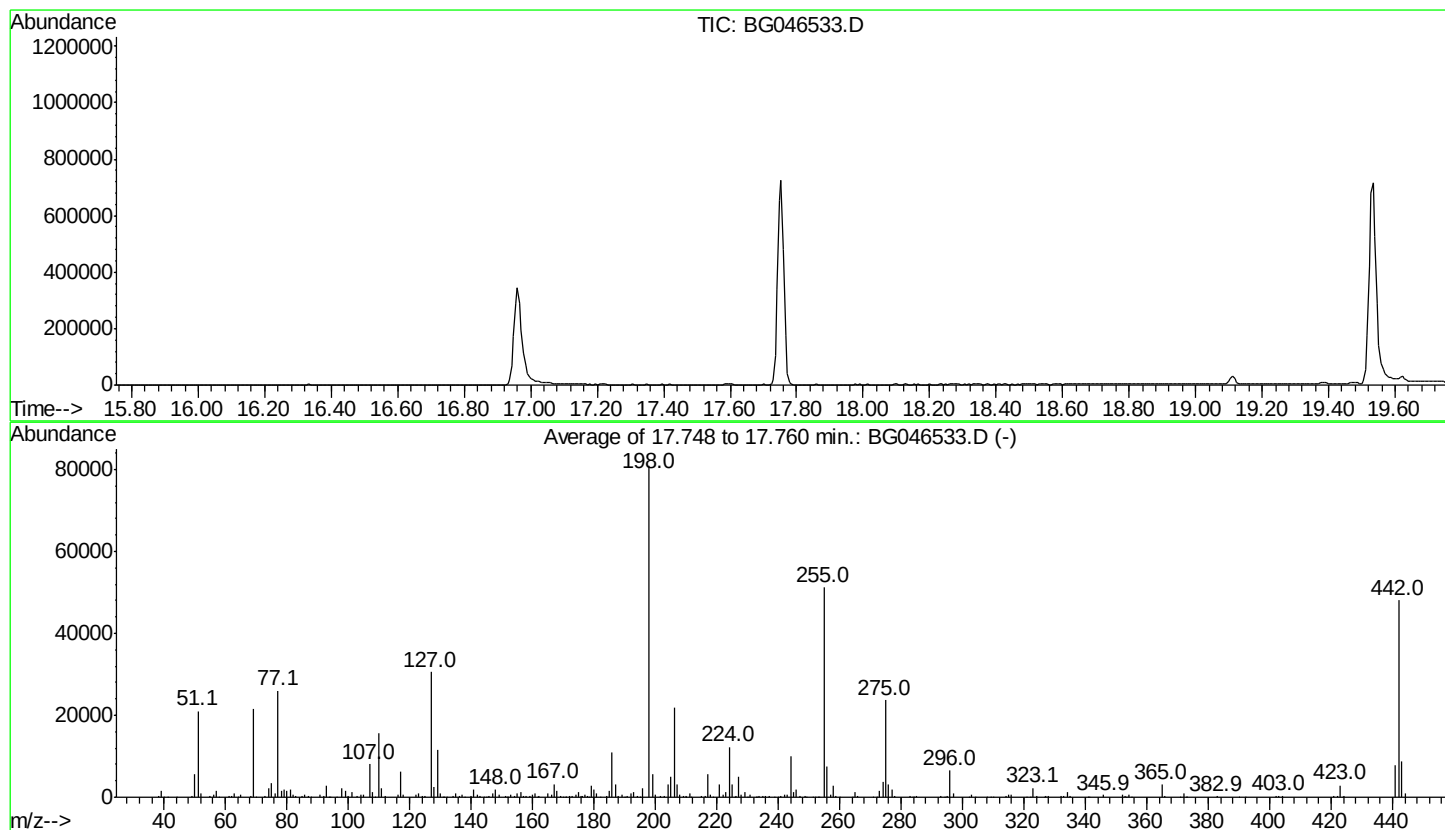

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.0	21067	PASS
68	69	0.00	2	0.8	183	PASS
69	198	0.00	100	26.7	21643	PASS
70	69	0.00	2	0.3	55	PASS
127	198	10	80	37.7	30496	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	80968	PASS
199	198	5	9	6.9	5571	PASS
275	198	10	60	29.3	23720	PASS
365	198	1	100	3.8	3042	PASS
441	198	0.01	100	9.7	7871	PASS
442	198	50	100	59.3	48032	PASS
443	442	15	24	18.2	8734	PASS